

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082522\
Data File : FF011297.D
Signal(s) : FID2B.ch
Acq On : 25 Aug 2022 14:40
Operator : YP\AJ
Sample : PB147272BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 25 18:43:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.790	1648232	15.165 ug/ml
Target Compounds				
18)	N-TETRACONTANE	21.715	110984	1.013 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082522\
Data File : FF011297.D
Signal(s) : FID2B.ch
Acq On : 25 Aug 2022 14:40
Operator : YP\AJ
Sample : PB147272BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 25 18:43:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

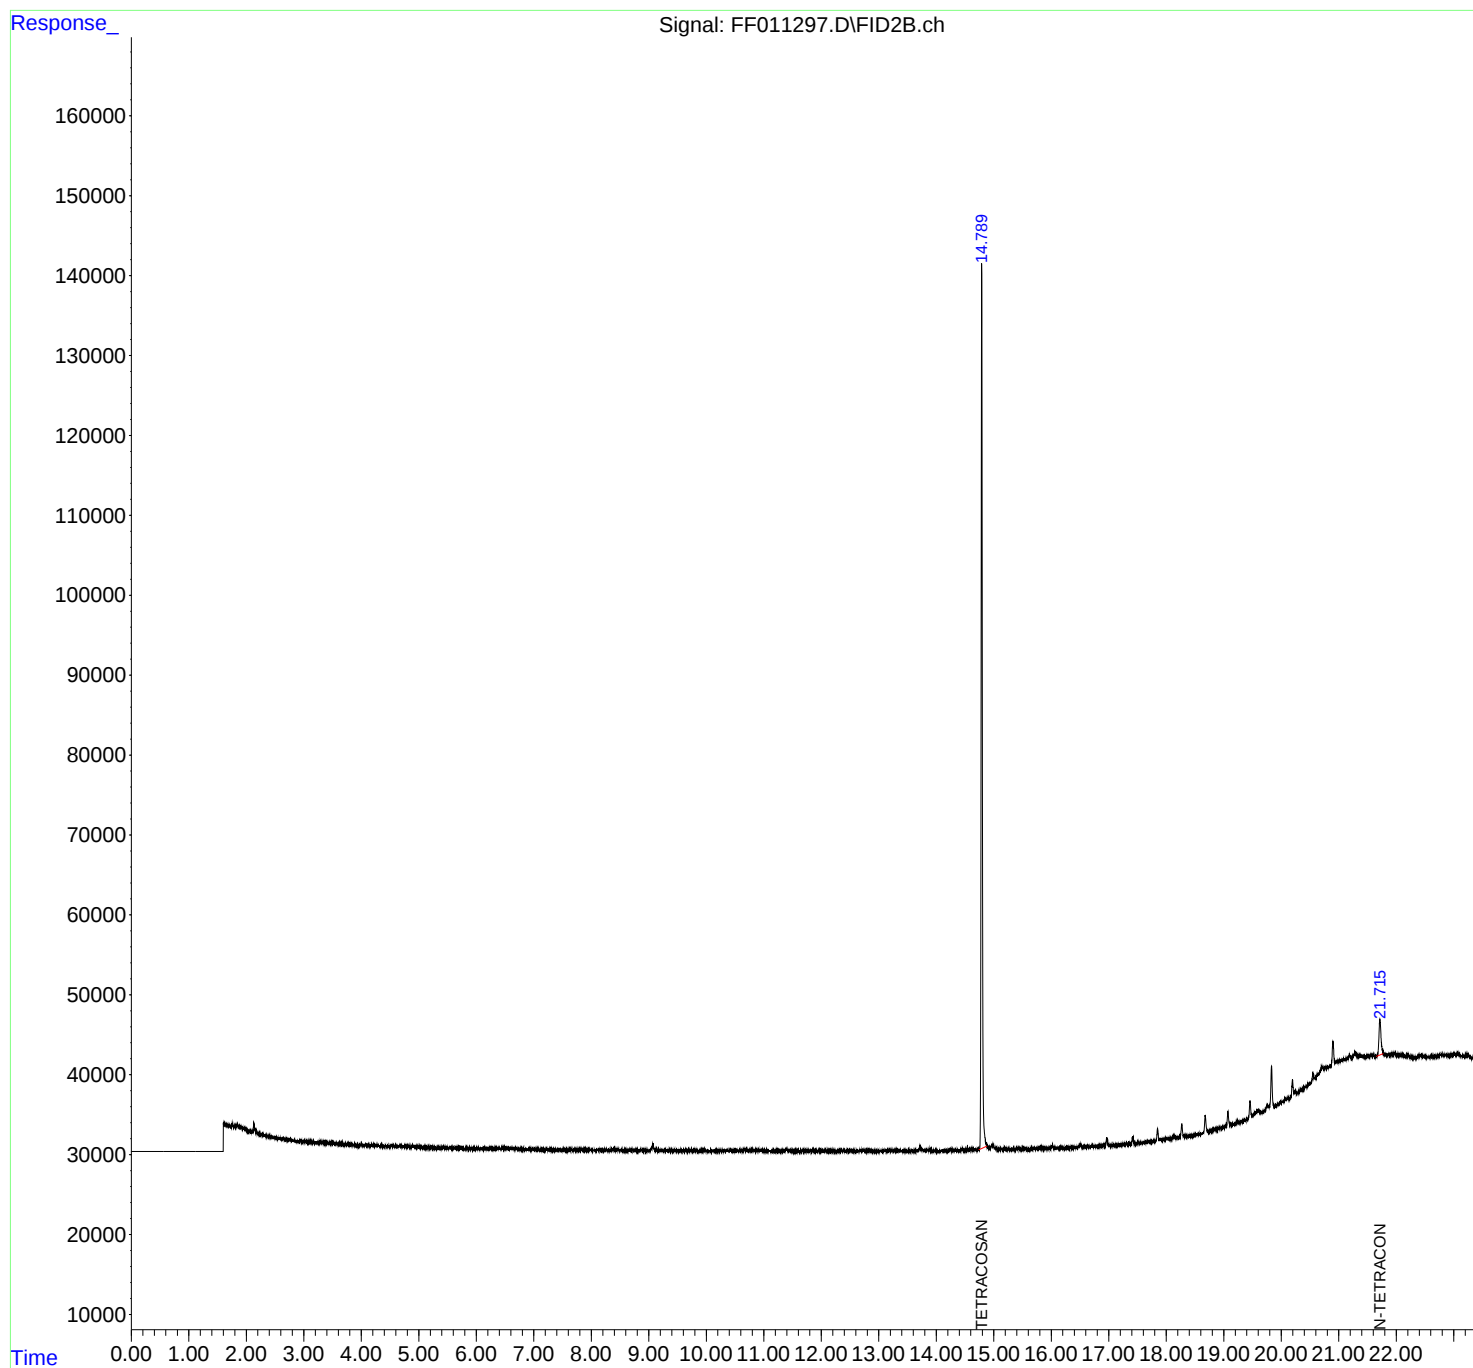


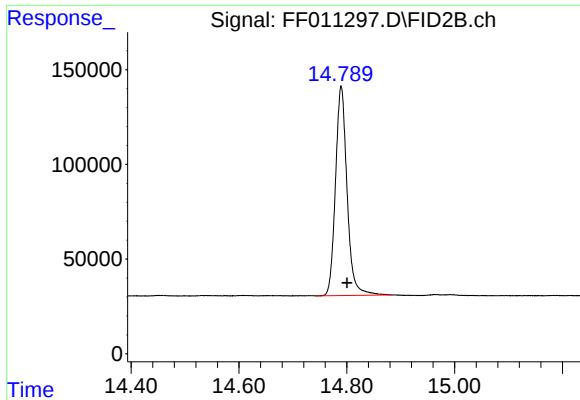

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.790 min
Delta R.T.: -0.011 min
Response: 1648232
Conc: 15.16 ug/ml

Instrument :
FID_F
ClientSampleId :

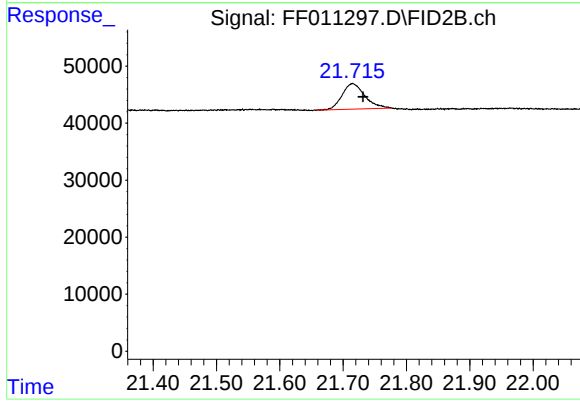

#18 N-TETRACONTANE

R.T.: 21.715 min
Delta R.T.: -0.017 min
Response: 110984
Conc: 1.01 ug/ml