

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082525\
Data File : FF016209.D
Signal(s) : FID2B.ch
Acq On : 25 Aug 2025 21:33
Operator : YP\AJ
Sample : PB169373BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB169373BL

Integration File: autoint1.e
Quant Time: Aug 26 04:25:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
Quant Title :
QLast Update : Wed Aug 06 13:50:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.080	2081271	18.646 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082525\
Data File : FF016209.D
Signal(s) : FID2B.ch
Acq On : 25 Aug 2025 21:33
Operator : YP\AJ
Sample : PB169373BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB169373BL

Integration File: autoint1.e
Quant Time: Aug 26 04:25:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
Quant Title :
QLast Update : Wed Aug 06 13:50:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

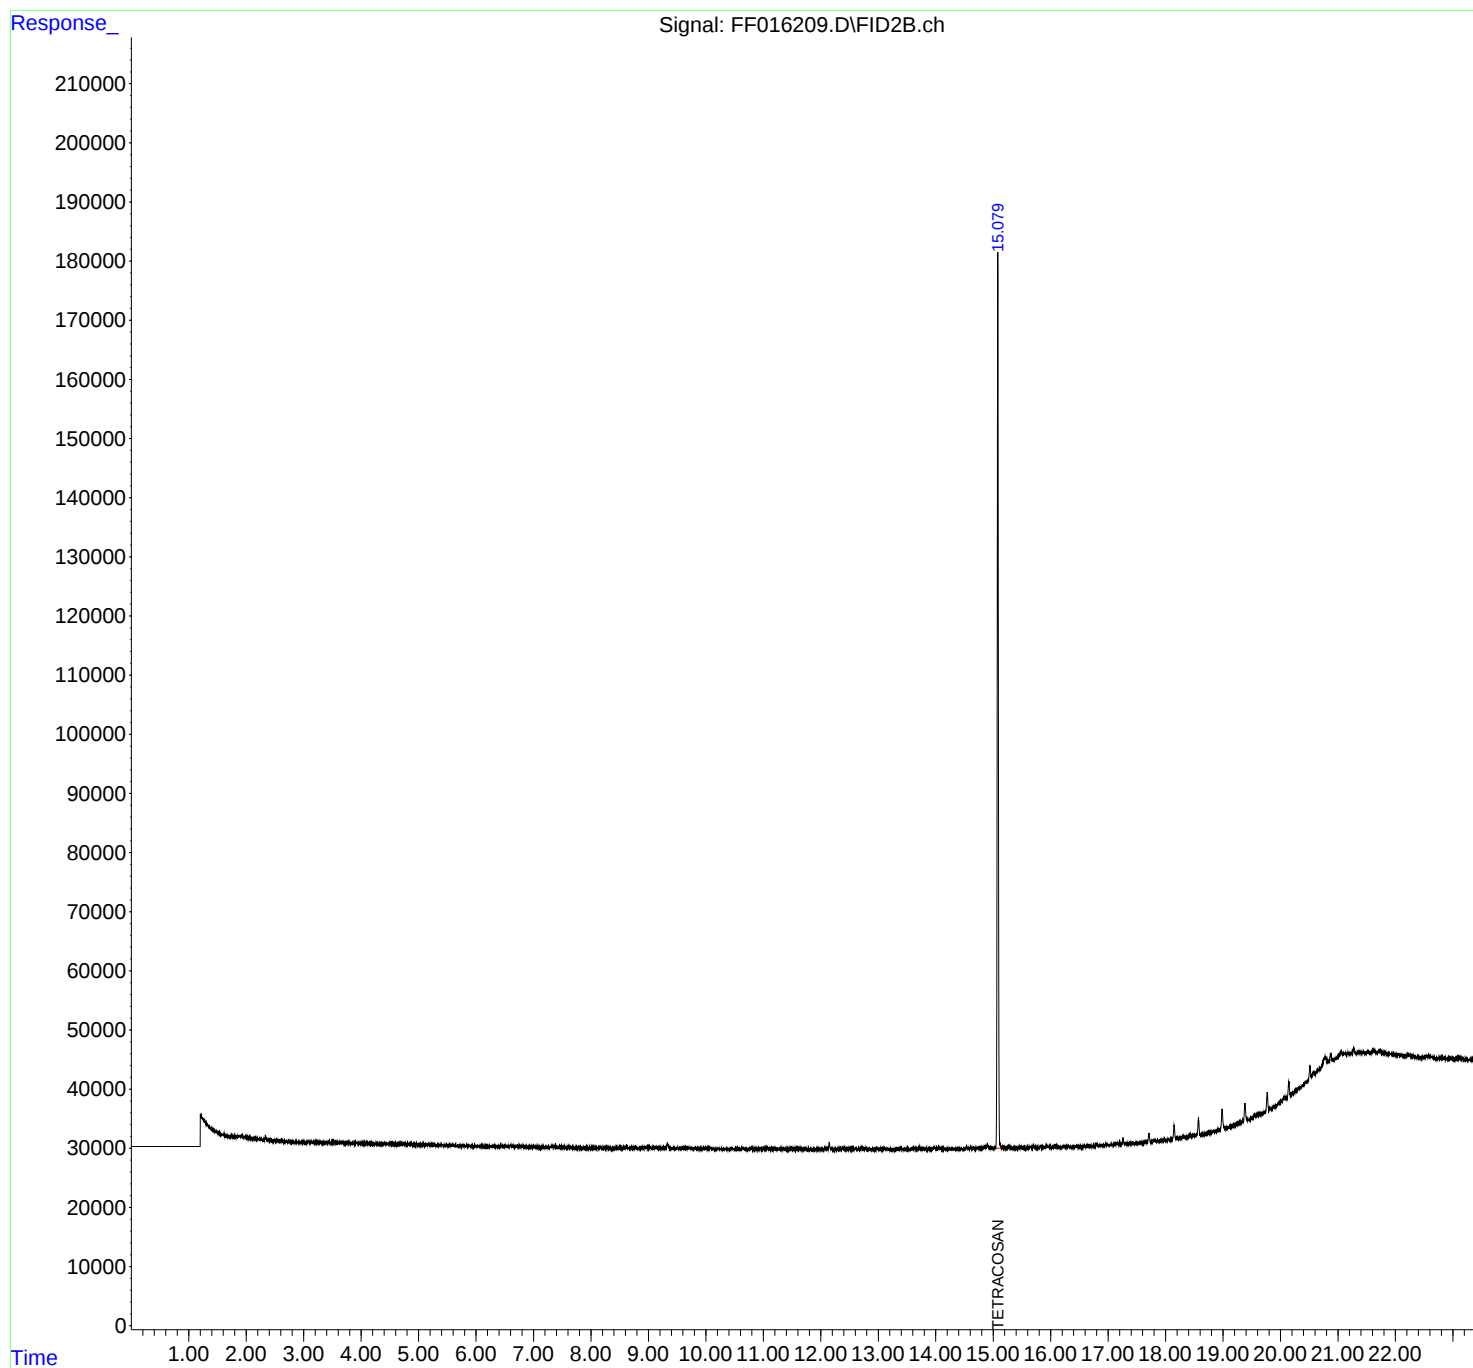

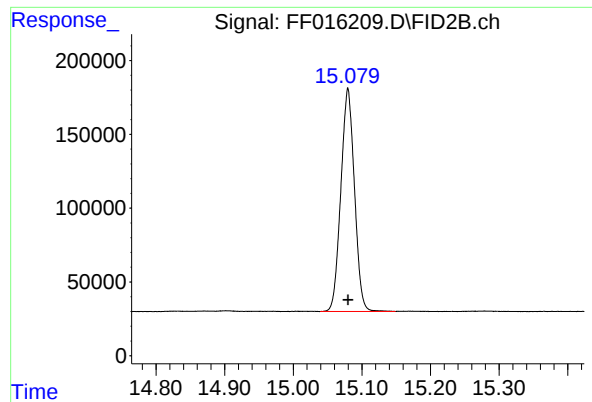

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.080 min
Delta R.T.: 0.000 min
Response: 2081271
Conc: 18.65 ug/ml

Instrument :
FID_F
ClientSampleId :
PB169373BL