

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082625\
Data File : FF016221.D
Signal(s) : FID2B.ch
Acq On : 26 Aug 2025 10:38
Operator : YP\AJ
Sample : PB169373BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB169373BL

Integration File: autoint1.e
Quant Time: Aug 27 04:33:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
Quant Title :
QLast Update : Wed Aug 06 13:50:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.077	2040950	18.285 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082625\
Data File : FF016221.D
Signal(s) : FID2B.ch
Acq On : 26 Aug 2025 10:38
Operator : YP\AJ
Sample : PB169373BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB169373BL

Integration File: autoint1.e
Quant Time: Aug 27 04:33:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
Quant Title :
QLast Update : Wed Aug 06 13:50:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

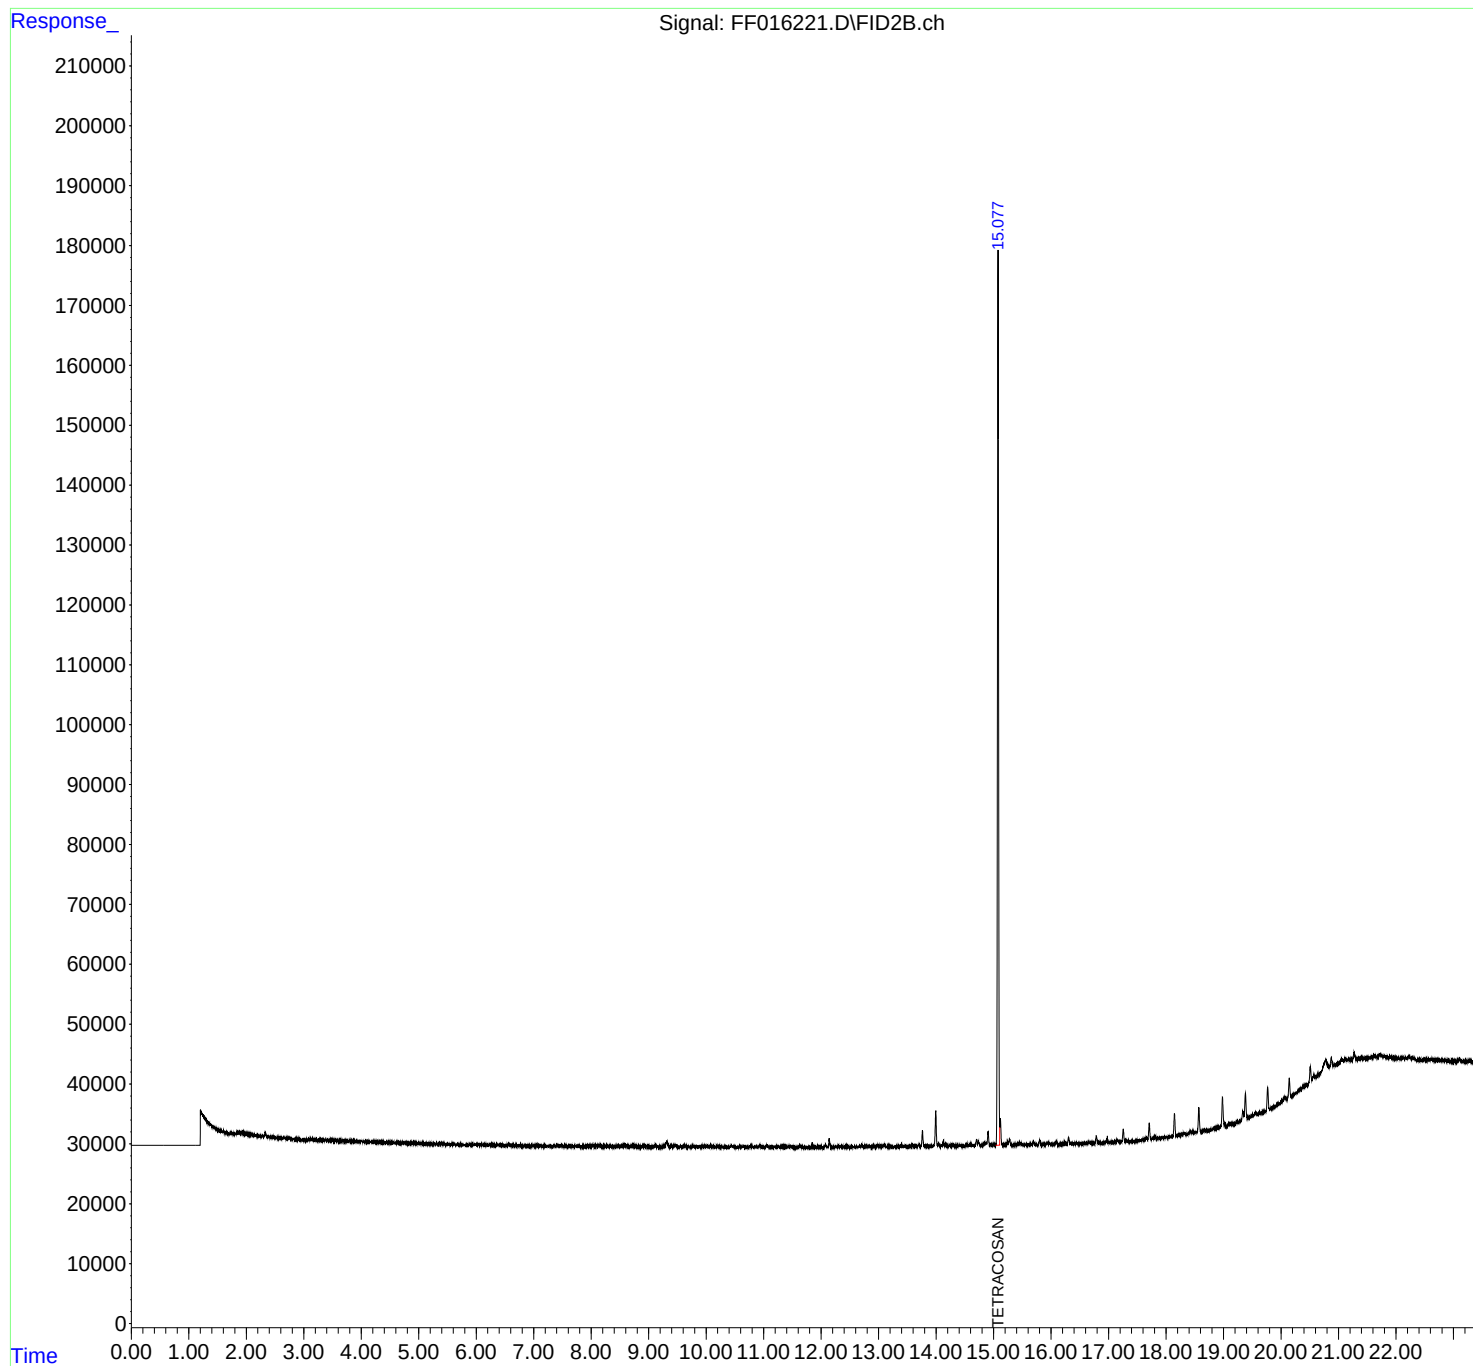

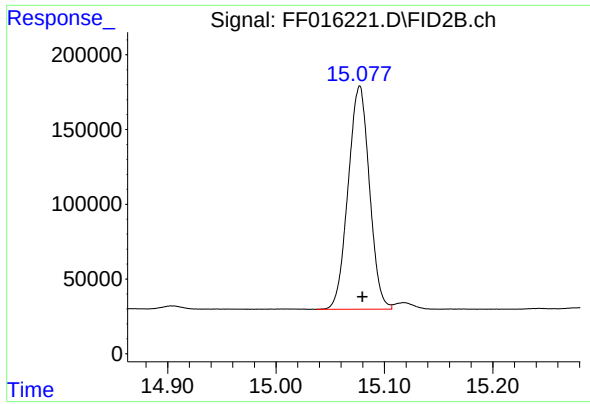

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.077 min
Delta R.T.: -0.002 min
Response: 2040950
Conc: 18.28 ug/ml

Instrument :
FID_F
ClientSampleId :
PB169373BL