

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082719\
Data File : FF005354.D
Signal(s) : FID2B.ch
Acq On : 27 Aug 2019 10:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 27 22:31:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.640	2011069	18.261 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	20.139	10893	0.097 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082719\
Data File : FF005354.D
Signal(s) : FID2B.ch
Acq On : 27 Aug 2019 10:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 27 22:31:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

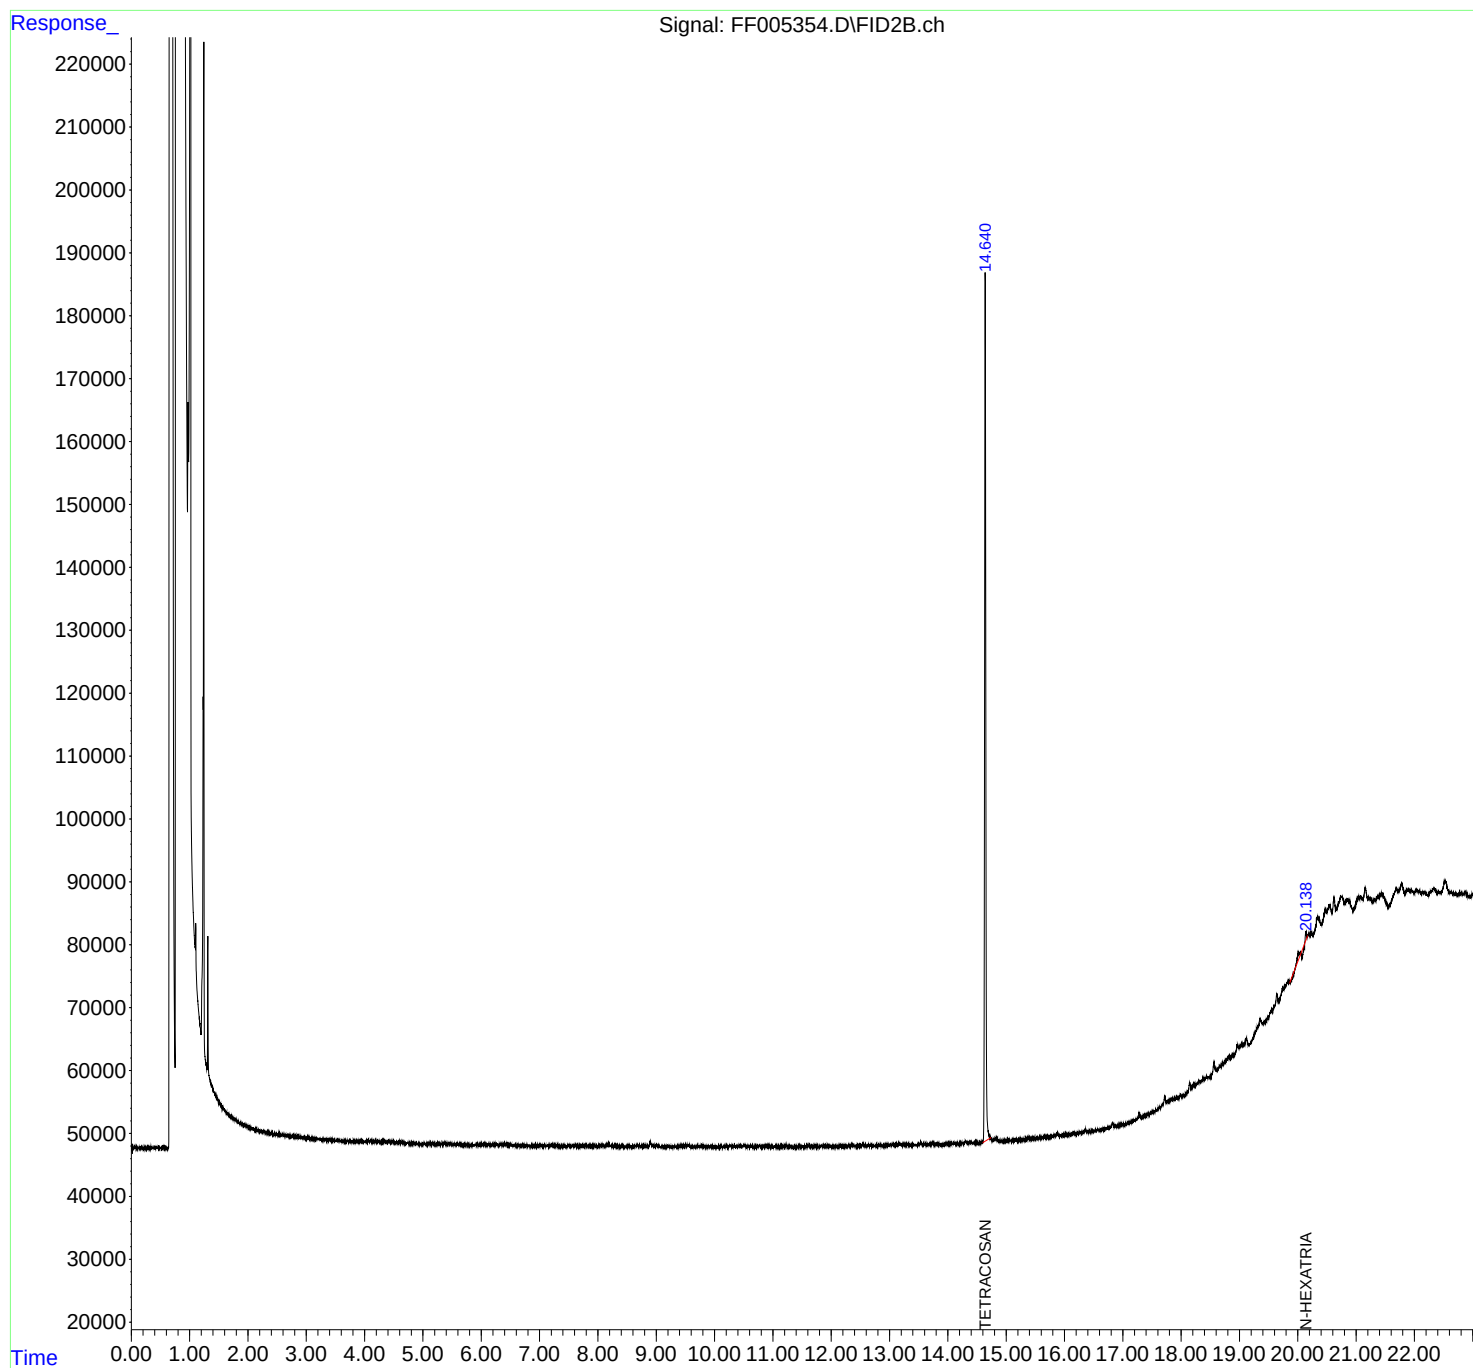


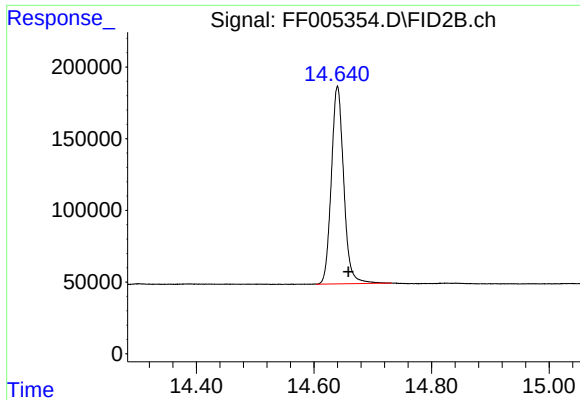

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.640 min
Delta R.T.: -0.018 min
Response: 2011069
Conc: 18.26 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

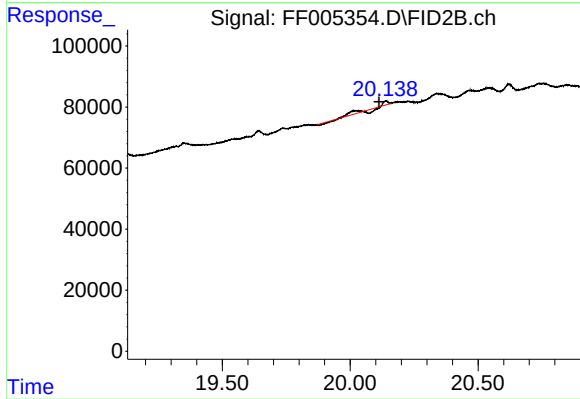

#16 N-HEXATRIACONTANE

R.T.: 20.139 min
Delta R.T.: 0.026 min
Response: 10893
Conc: 0.10 ug/ml