

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082719\
 Data File : FF005362.D
 Signal(s) : FID2B.ch
 Acq On : 27 Aug 2019 17:46
 Operator : DD\AJ
 Sample : PB122590BS
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB122590BS

Integration File: autoint1.e
 Quant Time: Aug 27 22:34:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
 Quant Title :
 QLast Update : Tue Jul 30 14:33:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.640	2183687	19.829 ug/ml
Target Compounds			
2) N-DECANE	4.360	2830631	19.647 ug/ml
3) N-DODECANE	6.381	2863843	19.627 ug/ml
4) N-TETRADECANE	8.175	2812307	19.539 ug/ml
5) N-HEXADECANE	9.777	2782519	19.625 ug/ml
6) N-OCTADECANE	11.221	2718775	19.856 ug/ml
7) N-EICOSANE	12.534	2664103	19.856 ug/ml
8) N-DOCOSANE	13.736	2620358	20.254 ug/ml
10) N-TETRACOSANE	14.845	2629406	20.870 ug/ml
11) N-HEXACOSANE	15.869	2631354	21.296 ug/ml
12) N-OCTACOSANE	16.825	2681171	21.464 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082719\
Data File : FF005362.D
Signal(s) : FID2B.ch
Acq On : 27 Aug 2019 17:46
Operator : DD\AJ
Sample : PB122590BS
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
PB122590BS

Integration File: autoint1.e
Quant Time: Aug 27 22:34:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

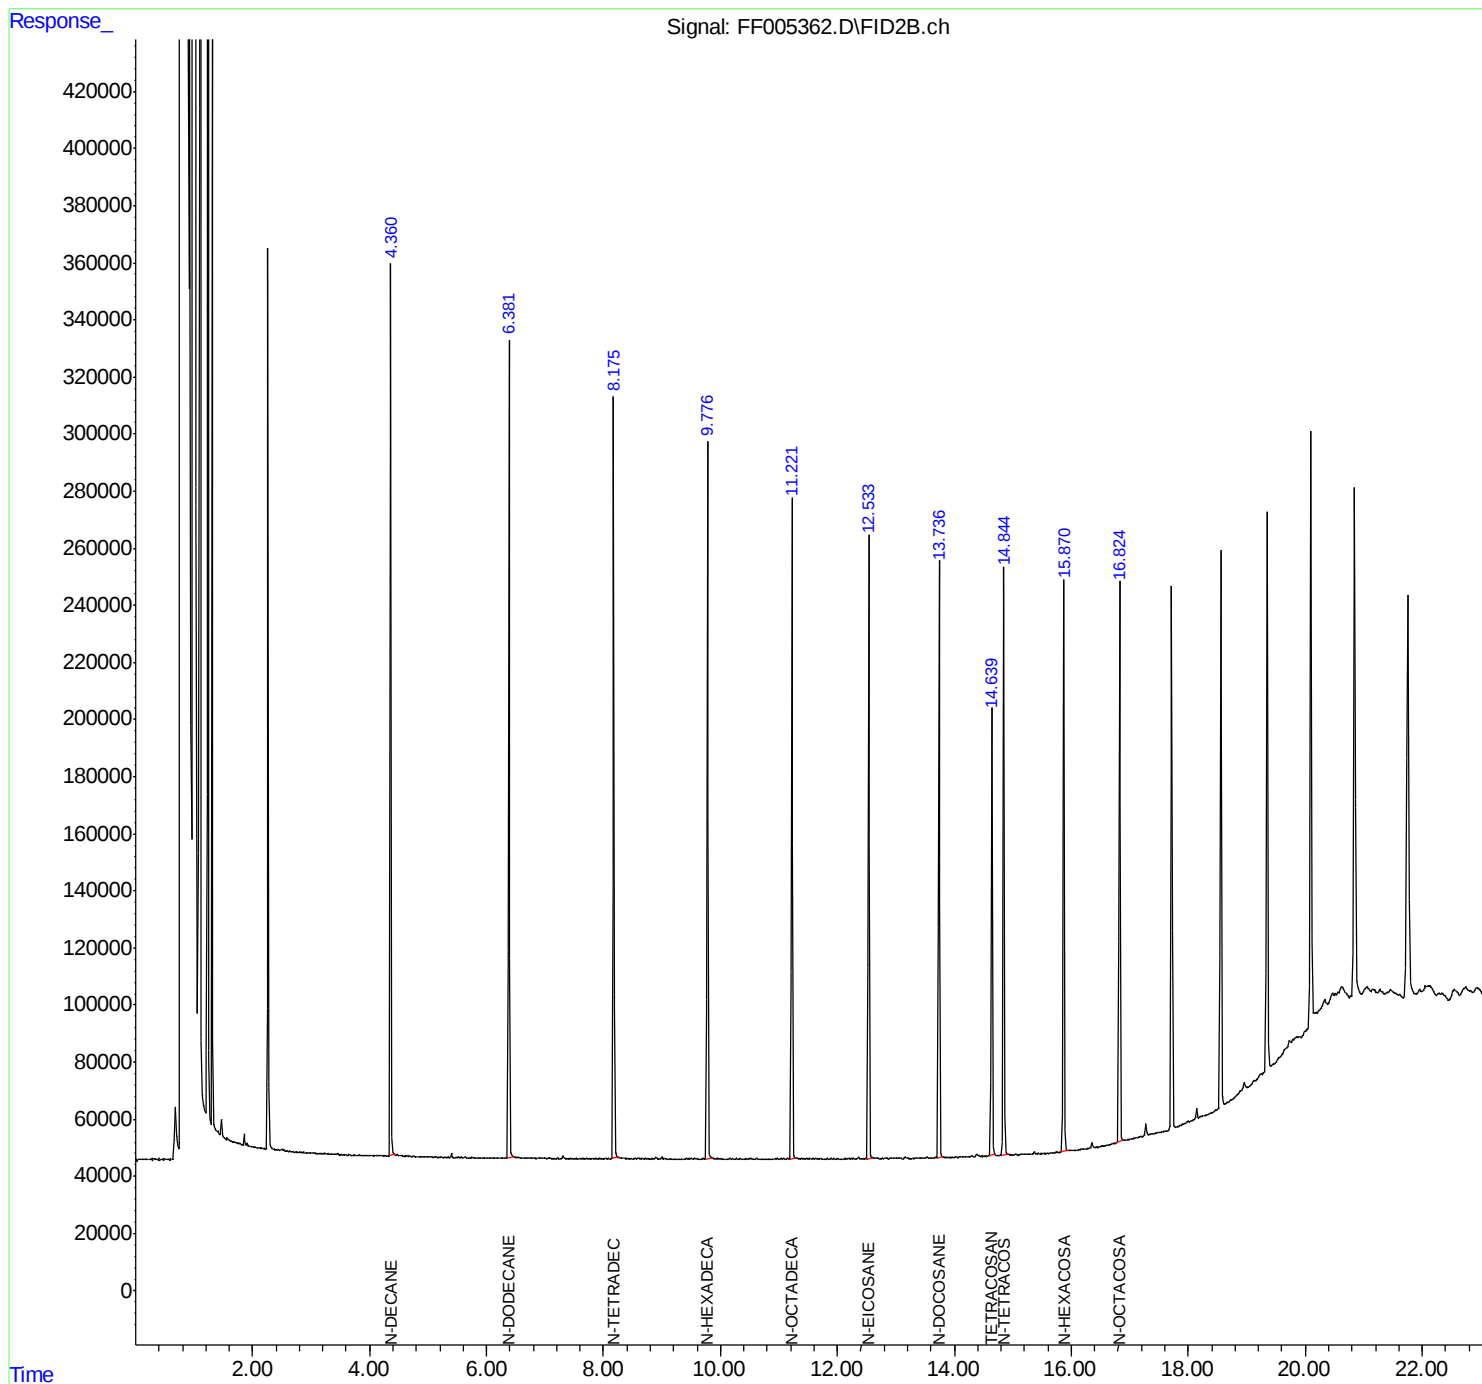


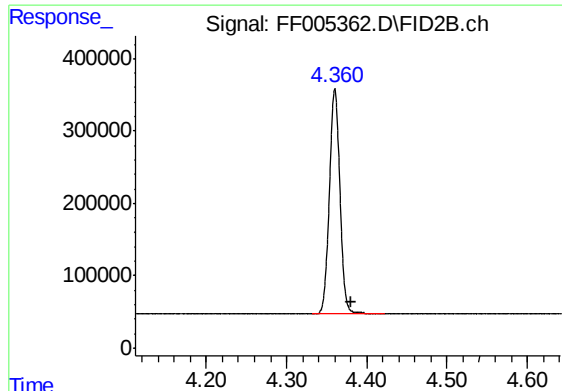

#2 N-DECANE


R.T.: 4.360 min
Delta R.T.: -0.020 min
Response: 2830631
Conc: 19.65 ug/ml

Instrument :
FID_F
ClientSampleId :
PB122590BS

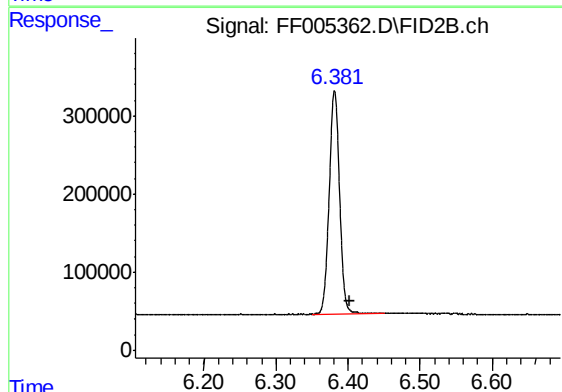


#3 N-DODECANE

R.T.: 6.381 min
Delta R.T.: -0.021 min
Response: 2863843
Conc: 19.63 ug/ml

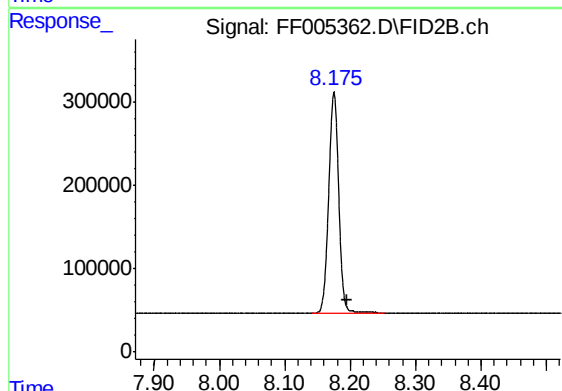


#4 N-TETRADECANE

R.T.: 8.175 min
Delta R.T.: -0.021 min
Response: 2812307
Conc: 19.54 ug/ml

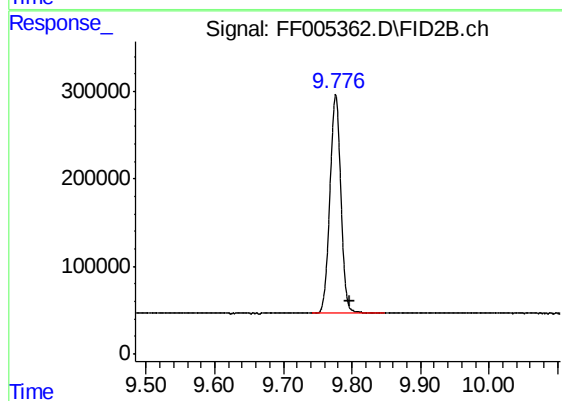

#5 N-HEXADECANE


R.T.: 9.777 min
Delta R.T.: -0.021 min
Response: 2782519
Conc: 19.62 ug/ml

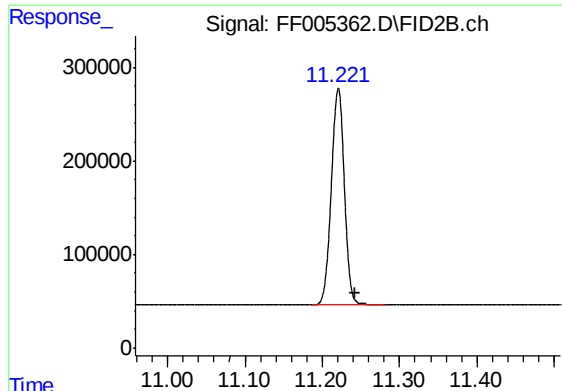

#6 N-OCTADECANE


R.T.: 11.221 min
Delta R.T.: -0.021 min
Response: 2718775
Conc: 19.86 ug/ml

Instrument :
FID_F
ClientSampleId :
PB122590BS

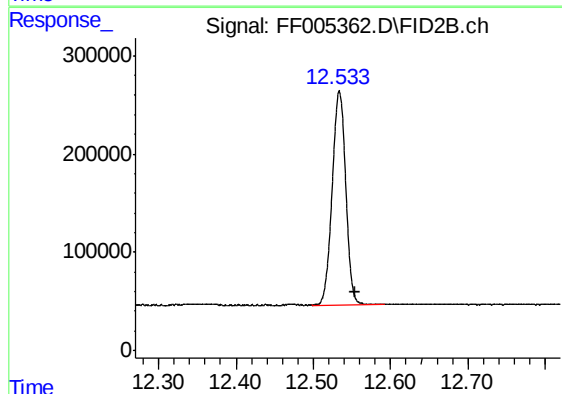


#7 N-EICOSANE

R.T.: 12.534 min
Delta R.T.: -0.020 min
Response: 2664103
Conc: 19.86 ug/ml

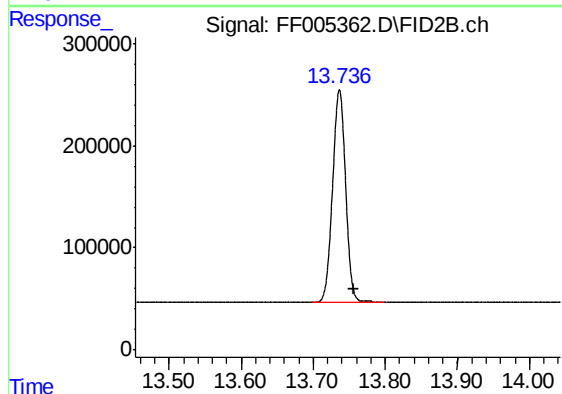


#8 N-DOCOSANE

R.T.: 13.736 min
Delta R.T.: -0.020 min
Response: 2620358
Conc: 20.25 ug/ml

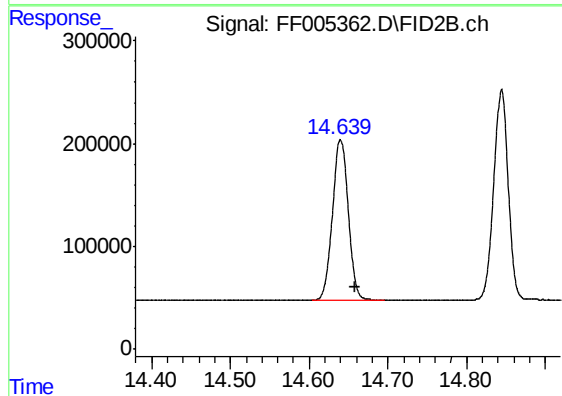

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.640 min
Delta R.T.: -0.019 min
Response: 2183687
Conc: 19.83 ug/ml

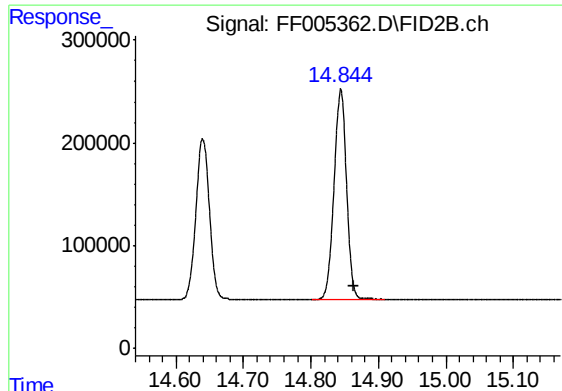

#10 N-TETRACOSANE


R.T.: 14.845 min
Delta R.T.: -0.020 min
Response: 2629406
Conc: 20.87 ug/ml

Instrument :
FID_F
ClientSampleId :
PB122590BS

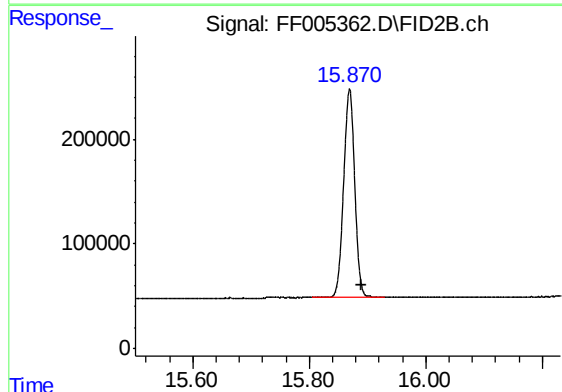

#11 N-HEXACOSANE

R.T.: 15.869 min
Delta R.T.: -0.020 min
Response: 2631354
Conc: 21.30 ug/ml

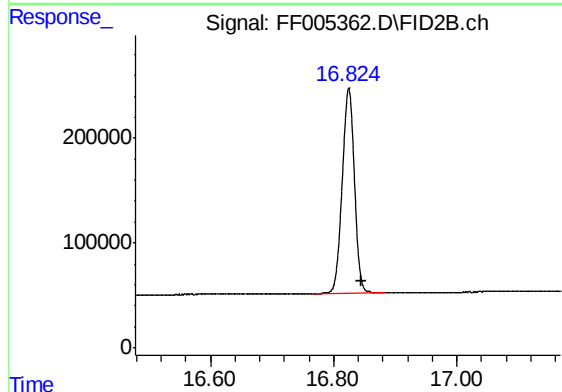

#12 N-OCTACOSANE

R.T.: 16.825 min
Delta R.T.: -0.020 min
Response: 2681171
Conc: 21.46 ug/ml