

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082725\  
 Data File : FF016235.D  
 Signal(s) : FID2B.ch  
 Acq On : 27 Aug 2025 10:10  
 Operator : YP\AJ  
 Sample : PB169406BL  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 PB169406BL

Integration File: autoint1.e  
 Quant Time: Aug 28 02:31:38 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF080625.M  
 Quant Title :  
 QLast Update : Wed Aug 06 13:50:48 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.078	2241342	20.080 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.146	67484	0.528 ug/ml
14) N-DOTRIACONTANE	18.981	105200	0.845 ug/ml
15) N-TETRATRIACONTANE	19.768	76376	0.682 ug/ml
16) N-HEXATRIACONTANE	20.509	48199	0.524 ug/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082725\  
 Data File : FF016235.D  
 Signal(s) : FID2B.ch  
 Acq On : 27 Aug 2025 10:10  
 Operator : YP\AJ  
 Sample : PB169406BL  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 PB169406BL

Integration File: autoint1.e  
 Quant Time: Aug 28 02:31:38 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF080625.M  
 Quant Title :  
 QLast Update : Wed Aug 06 13:50:48 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

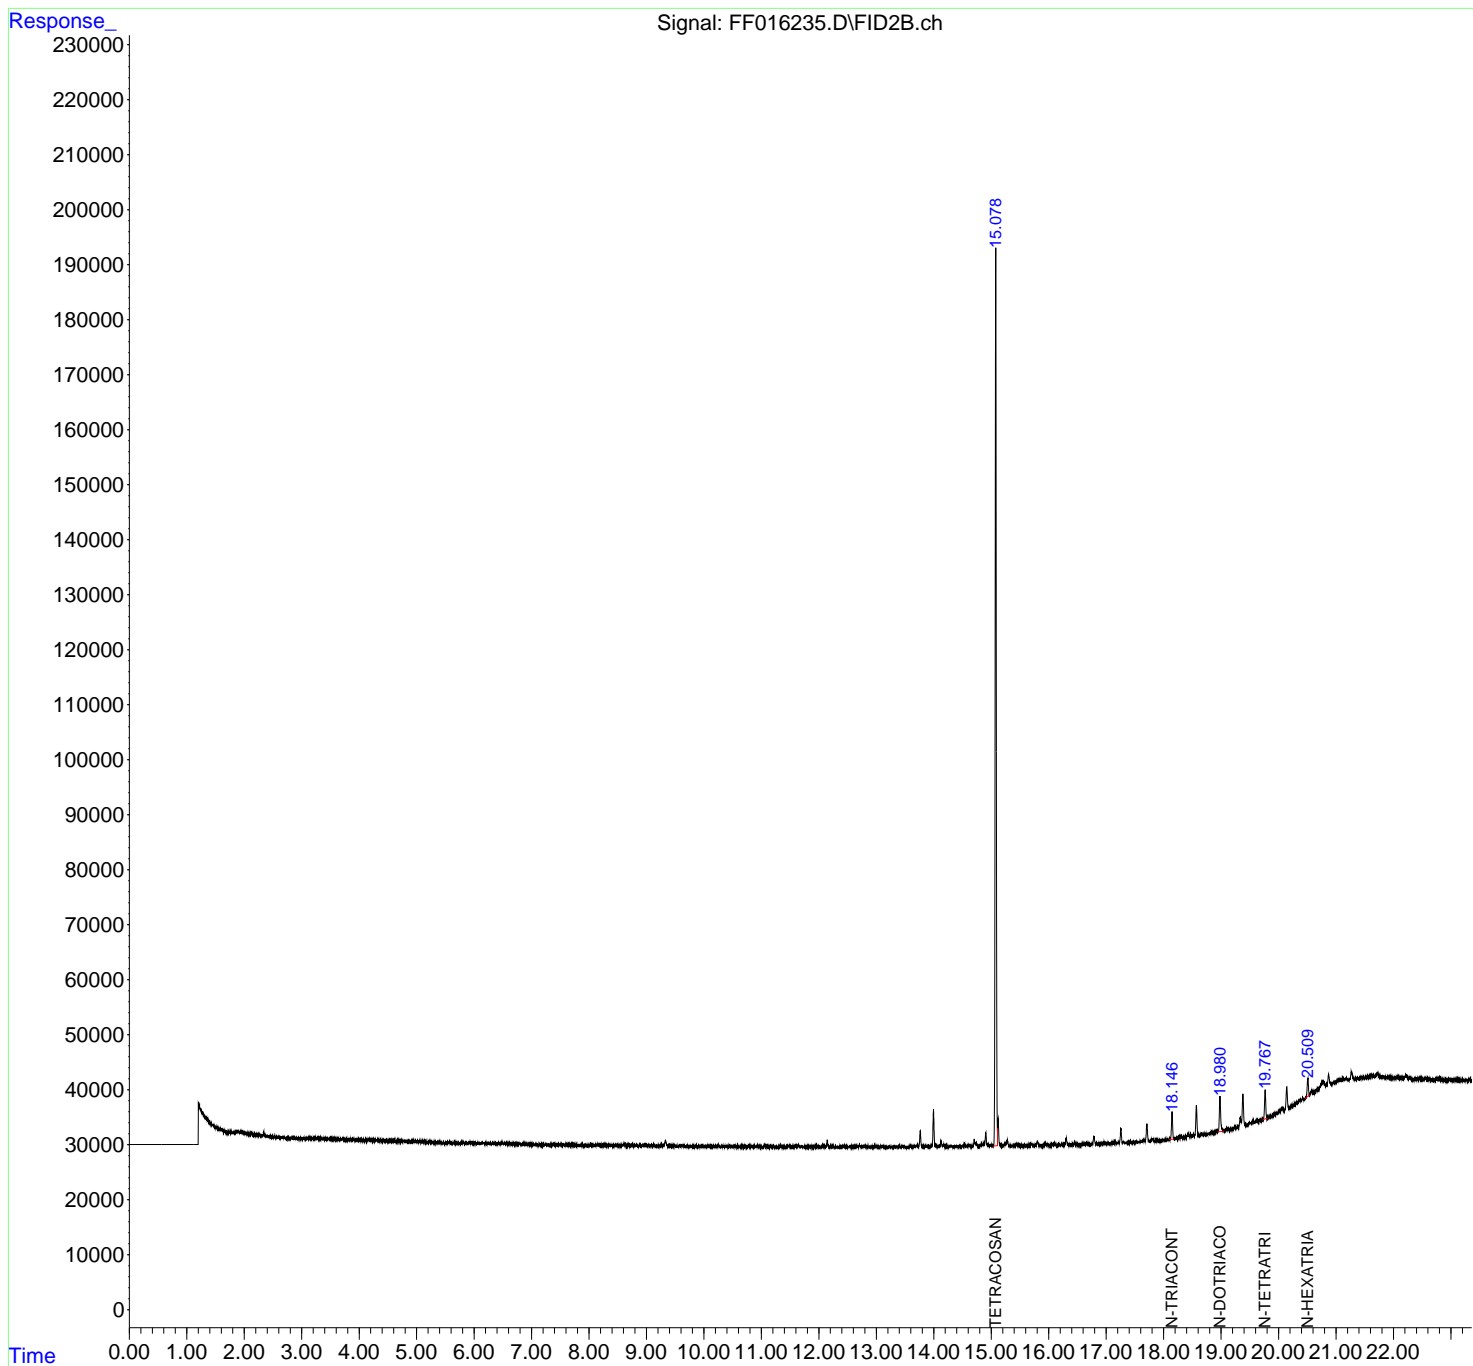


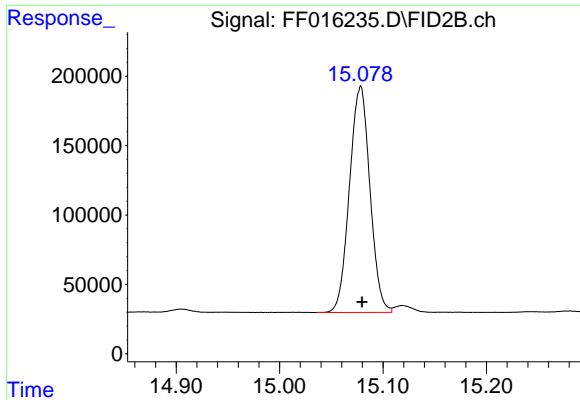

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.078 min  
 Delta R.T.: -0.001 min  
 Response: 2241342  
 Conc: 20.08 ug/ml

Instrument :  
 FID\_F  
 ClientSampleId :  
 PB169406BL

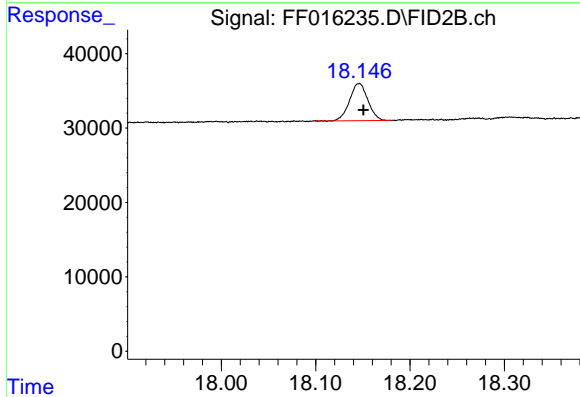


#13 N-TRIACONTANE

R.T.: 18.146 min  
 Delta R.T.: -0.004 min  
 Response: 67484  
 Conc: 0.53 ug/ml

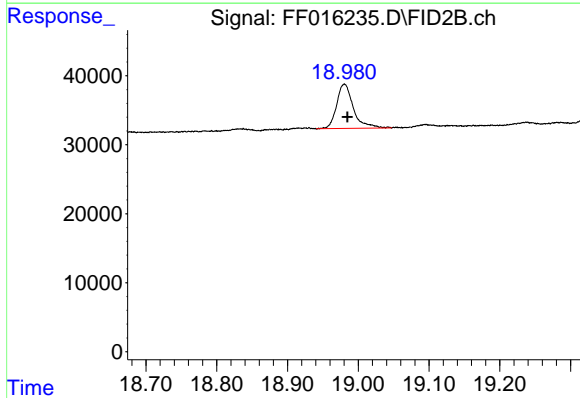


#14 N-DOTRIACONTANE

R.T.: 18.981 min  
 Delta R.T.: -0.004 min  
 Response: 105200  
 Conc: 0.85 ug/ml

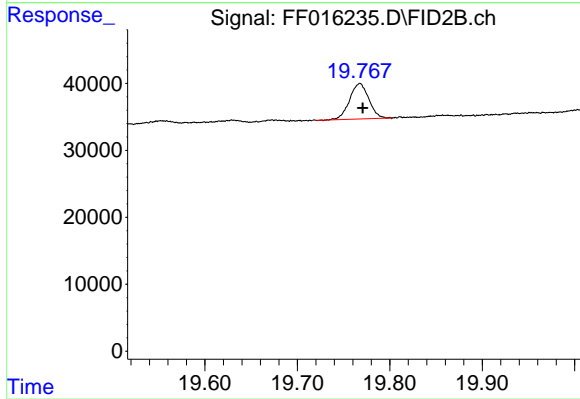

#15 N-TETRATRIACONTANE

R.T.: 19.768 min  
 Delta R.T.: -0.003 min  
 Response: 76376  
 Conc: 0.68 ug/ml

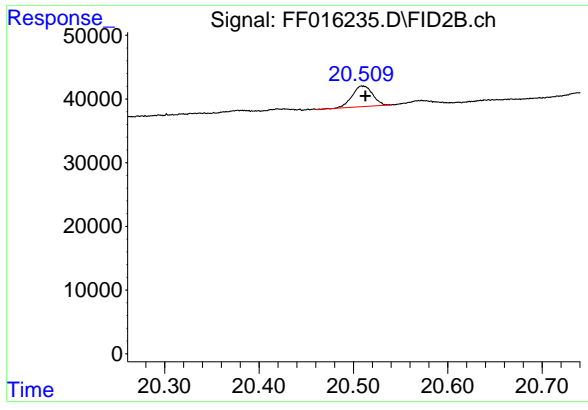

#16 N-HEXATRIACONTANE

R.T.: 20.509 min  
Delta R.T.: -0.003 min  
Response: 48199  
Conc: 0.52 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
PB169406BL