

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082725\
 Data File : FF016244.D
 Signal(s) : FID2B.ch
 Acq On : 27 Aug 2025 15:09
 Operator : YP\AJ
 Sample : PB169404BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB169404BL

Integration File: autoint1.e
 Quant Time: Aug 28 02:34:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
 Quant Title :
 QLast Update : Wed Aug 06 13:50:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.078	2202432	19.731 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082725\
 Data File : FF016244.D
 Signal(s) : FID2B.ch
 Acq On : 27 Aug 2025 15:09
 Operator : YP\AJ
 Sample : PB169404BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB169404BL

Integration File: autoint1.e
 Quant Time: Aug 28 02:34:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
 Quant Title :
 QLast Update : Wed Aug 06 13:50:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

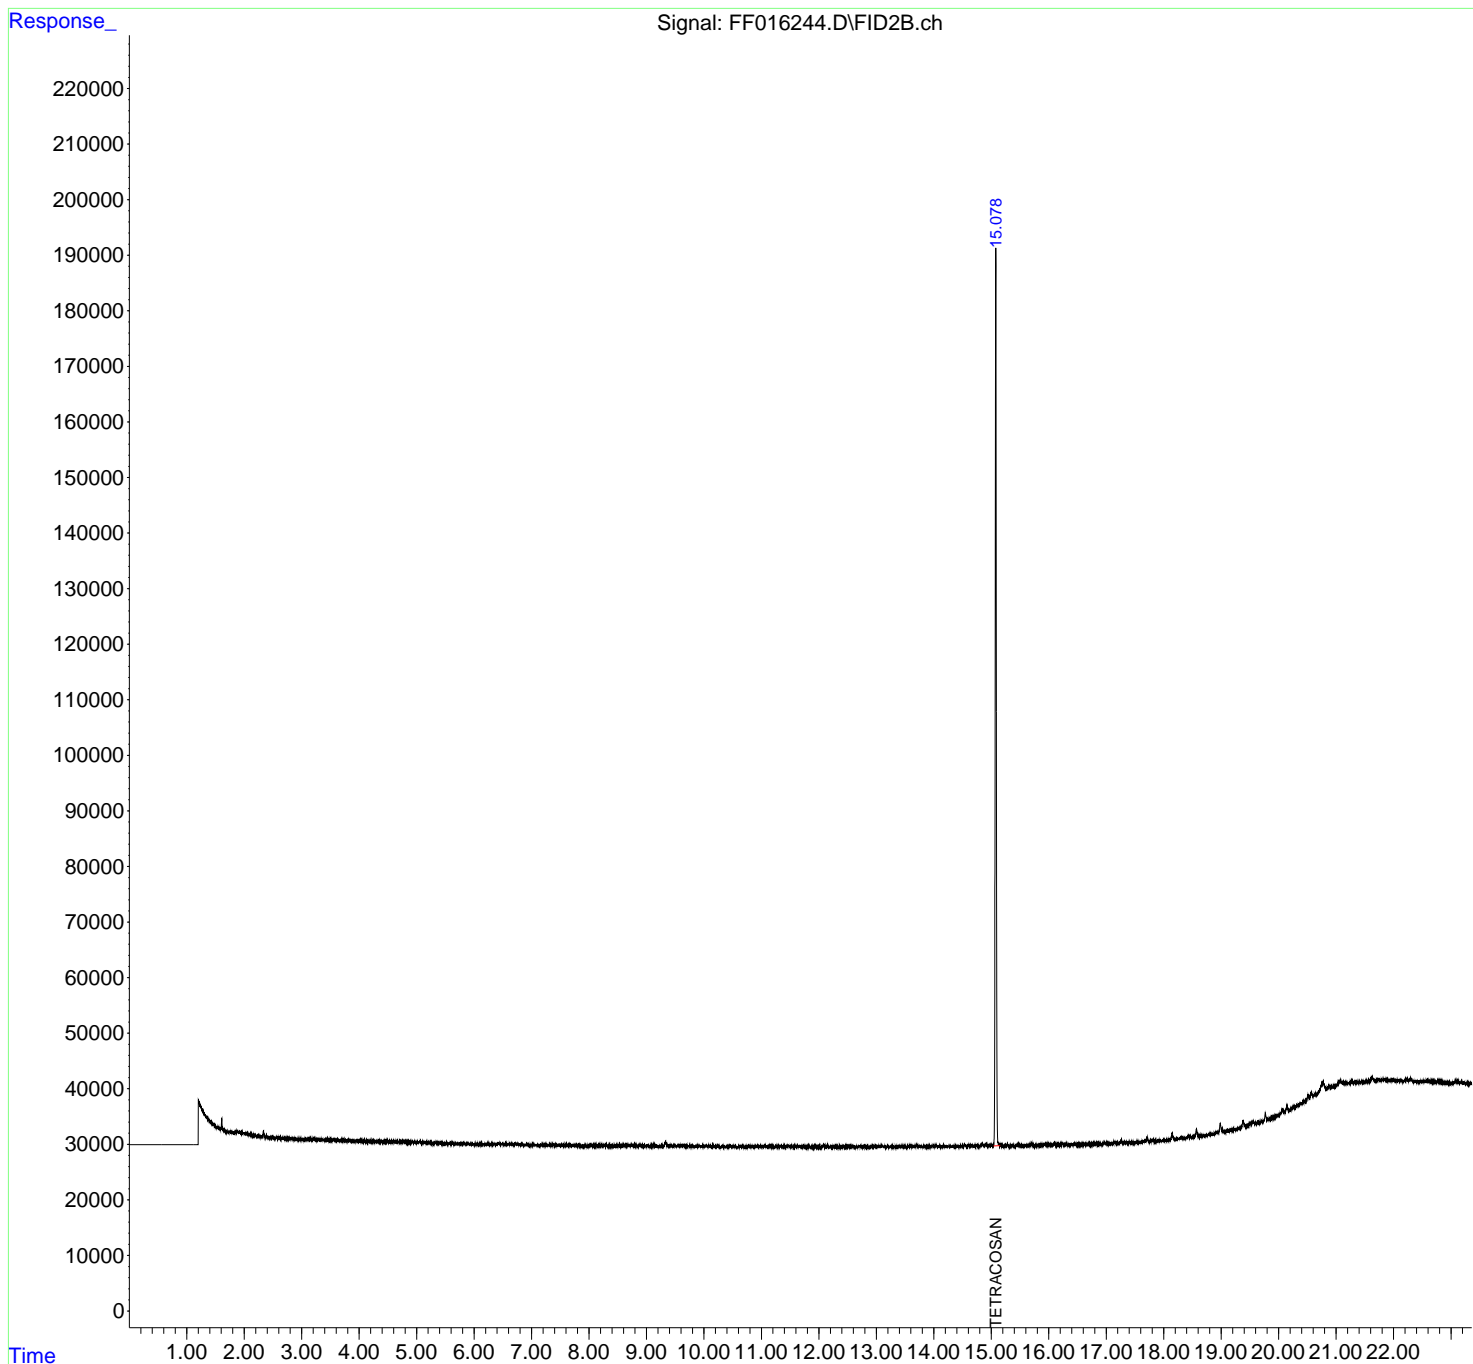

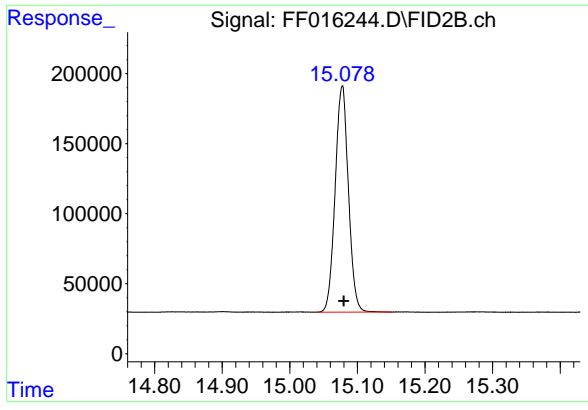

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.078 min
Delta R.T.: -0.002 min
Response: 2202432
Conc: 19.73 ug/ml

Instrument :
FID_F
ClientSampleId :
PB169404BL