

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082818\
 Data File : FF001952.D
 Signal(s) : FID2B.ch
 Acq On : 28 Aug 2018 14:18
 Operator : AJ\SJ
 Sample : J4276-05 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 29 04:32:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.301	229528	1.817 ug/ml
Target Compounds			
7) N-EICOSANE	12.209	318799	2.139 ug/ml
8) N-DOCOSANE	13.440	160936	1.102 ug/ml
10) N-TETRACOSANE	14.499	1305774	9.154 ug/ml
11) N-HEXACOSANE	15.521	96120	0.682 ug/ml
12) N-OCTACOSANE	16.468	270200	1.927 ug/ml
13) N-TRIACONTANE	17.356	267579	1.933 ug/ml
14) N-DOTRIACONTANE	18.186	433866	3.326 ug/ml
15) N-TETRATRIACONTANE	18.969	282472	2.337 ug/ml
16) N-HEXATRIACONTANE	19.711	310888	2.794 ug/ml
17) N-OCTATRIACONTANE	20.416	171851	1.724 ug/ml
18) N-TETRACONTANE	21.195	181532	1.822 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082818\
Data File : FF001952.D
Signal(s) : FID2B.ch
Acq On : 28 Aug 2018 14:18
Operator : AJ\SJ
Sample : J4276-05 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 29 04:32:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

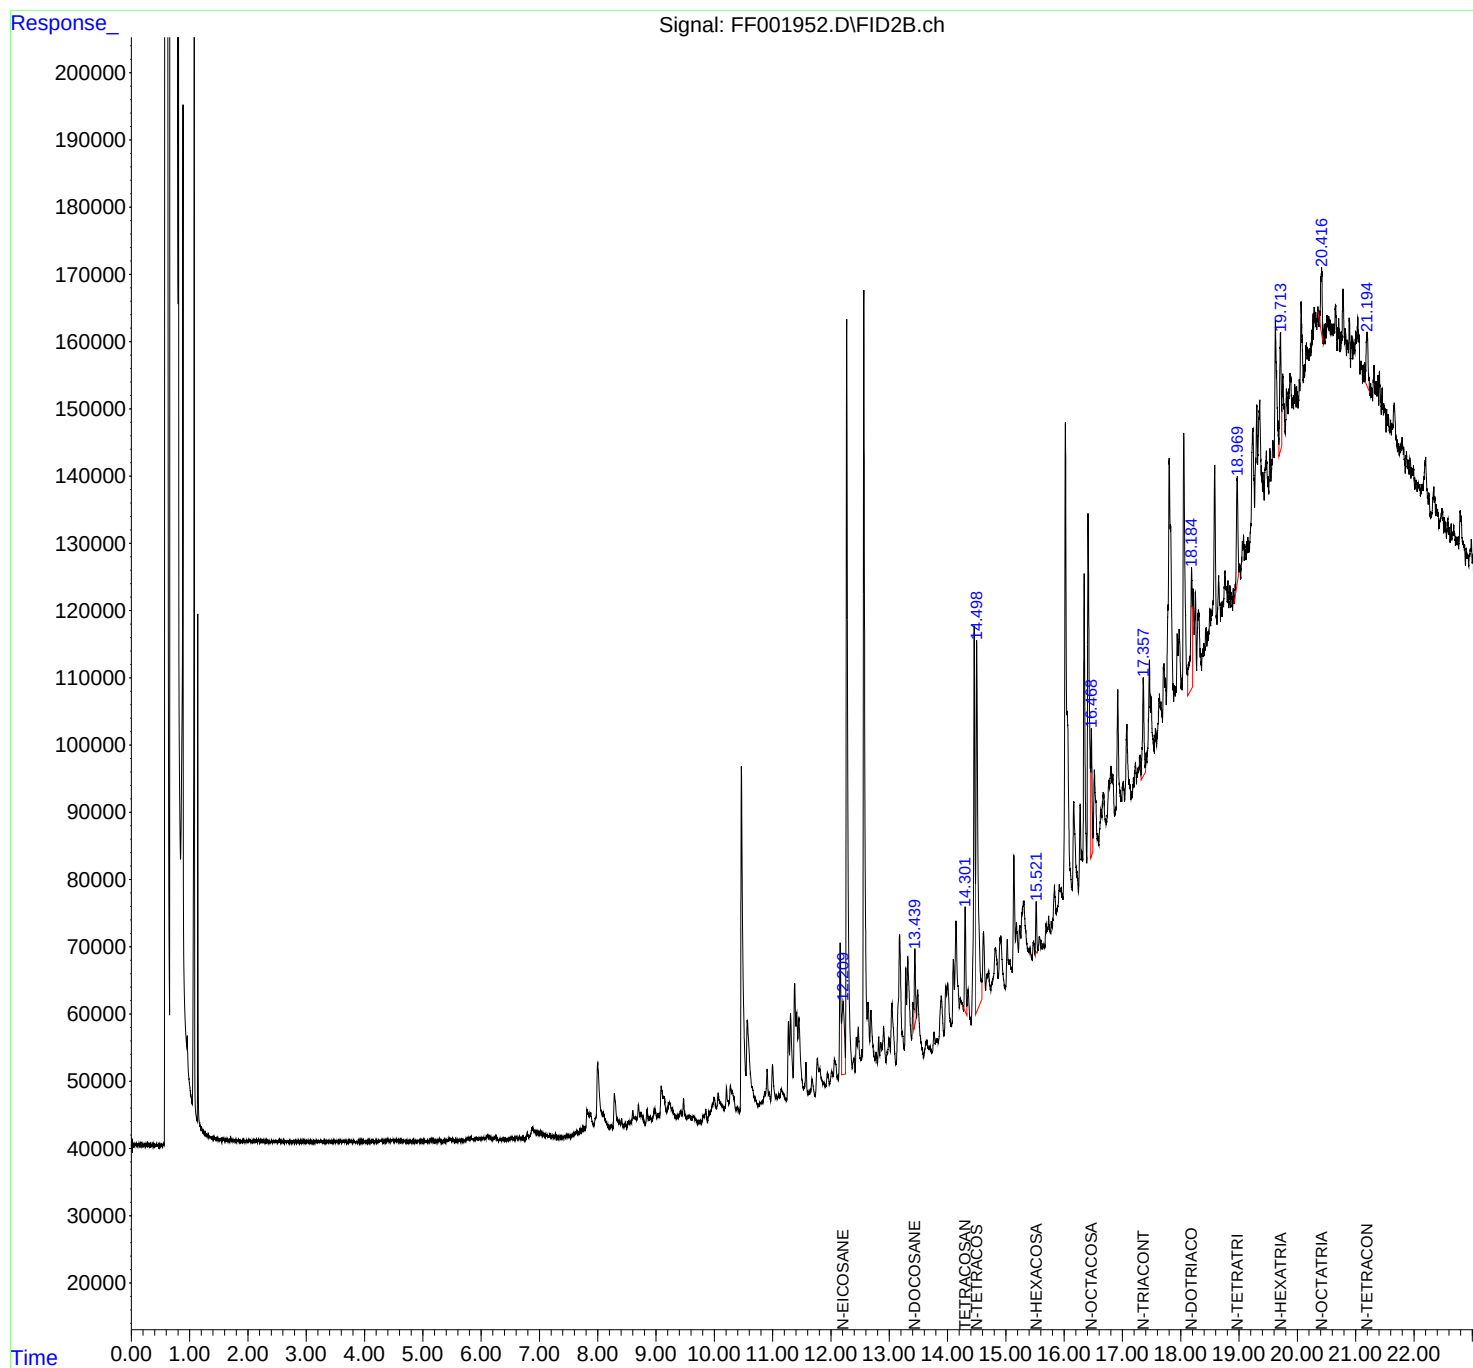

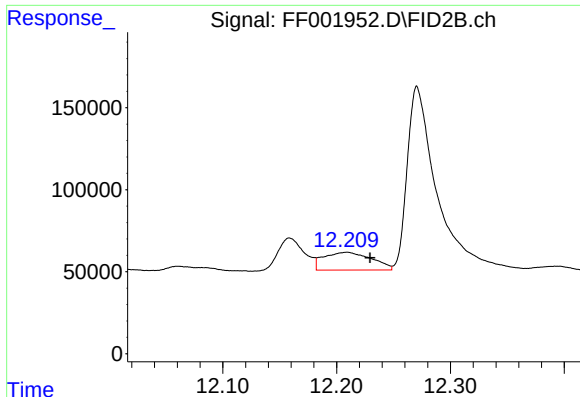


#7 N-EICOSANE

R.T.: 12.209 min
Delta R.T.: -0.020 min
Response: 318799
Conc: 2.14 ug/ml

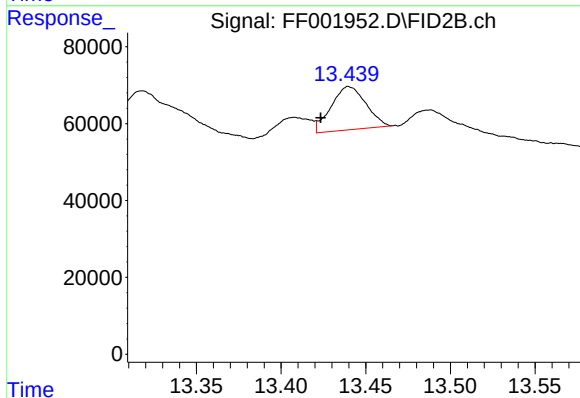


#8 N-DOCOSANE

R.T.: 13.440 min
Delta R.T.: 0.017 min
Response: 160936
Conc: 1.10 ug/ml

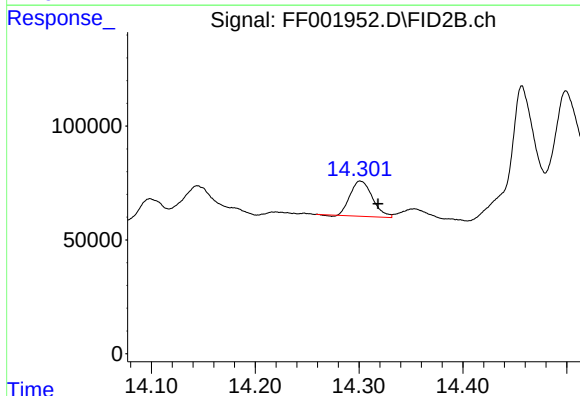


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.301 min
Delta R.T.: -0.017 min
Response: 229528
Conc: 1.82 ug/ml

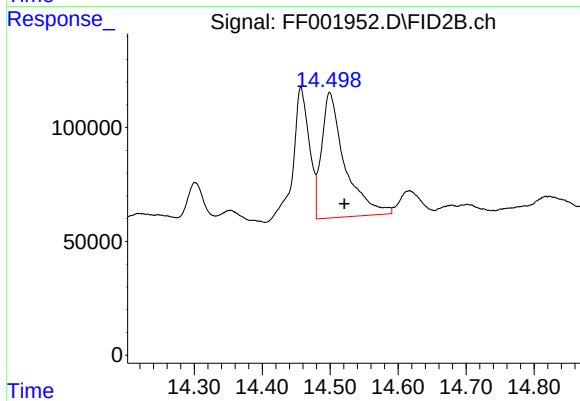


#10 N-TETRACOSANE

R.T.: 14.499 min
Delta R.T.: -0.022 min
Response: 1305774
Conc: 9.15 ug/ml

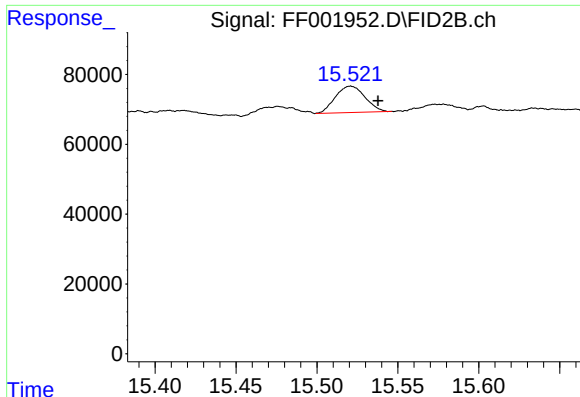


#11 N-HEXACOSANE

R.T.: 15.521 min
Delta R.T.: -0.017 min
Response: 96120
Conc: 0.68 ug/ml

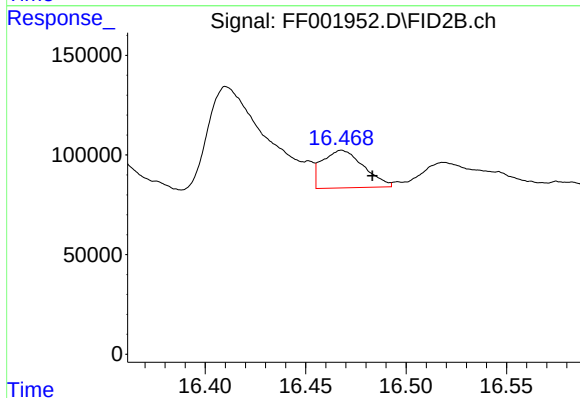


#12 N-OCTACOSANE

R.T.: 16.468 min
Delta R.T.: -0.015 min
Response: 270200
Conc: 1.93 ug/ml

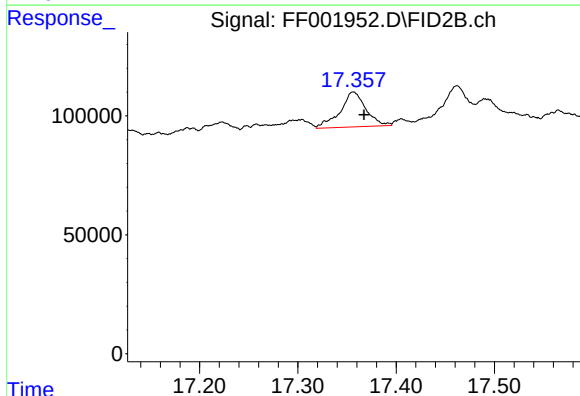


#13 N-TRIACONTANE

R.T.: 17.356 min
Delta R.T.: -0.011 min
Response: 267579
Conc: 1.93 ug/ml

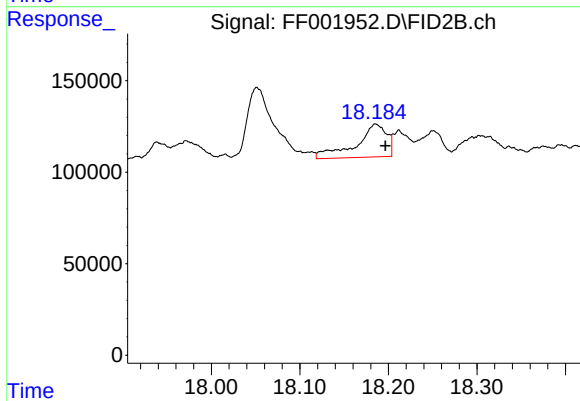


#14 N-DOTRIACONTANE

R.T.: 18.186 min
Delta R.T.: -0.011 min
Response: 433866
Conc: 3.33 ug/ml

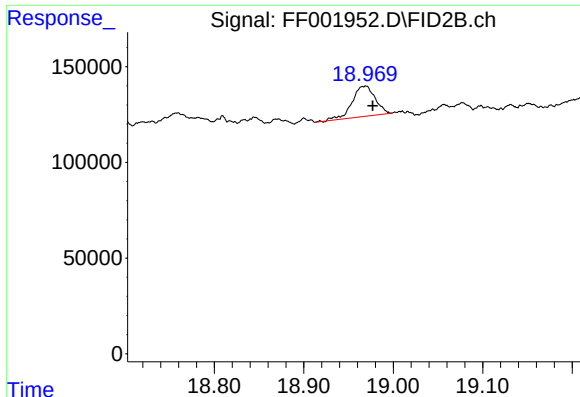


#15 N-TETRATRIACONTANE

R.T.: 18.969 min
Delta R.T.: -0.008 min
Response: 282472
Conc: 2.34 ug/ml

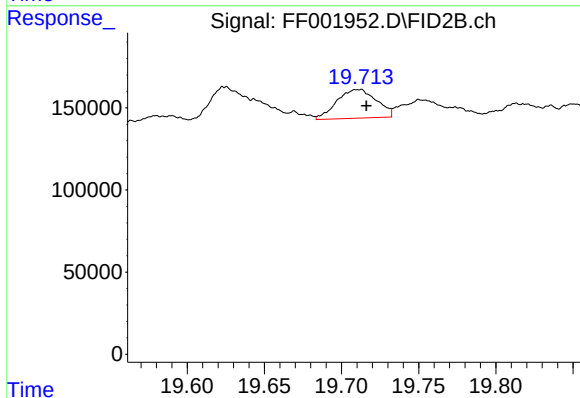


#16 N-HEXATRIACONTANE

R.T.: 19.711 min
Delta R.T.: -0.005 min
Response: 310888
Conc: 2.79 ug/ml

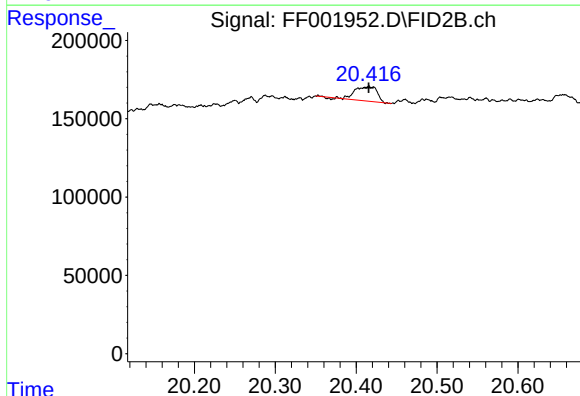

#17 N-OCTATRIACONTANE

R.T.: 20.416 min
Delta R.T.: 0.000 min
Response: 171851
Conc: 1.72 ug/ml

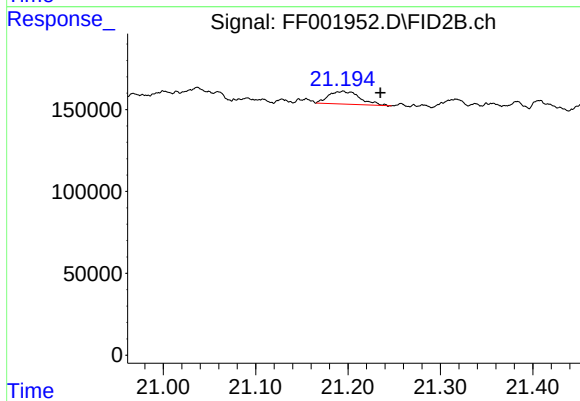

#18 N-TETRACONTANE

R.T.: 21.195 min
Delta R.T.: -0.040 min
Response: 181532
Conc: 1.82 ug/ml