

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082818\
 Data File : FF001956.D
 Signal(s) : FID2B.ch
 Acq On : 28 Aug 2018 16:19
 Operator : AJ\SJ
 Sample : J4277-09 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 29 04:33:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.305	129748	1.027 ug/ml
Target Compounds			
7) N-EICOSANE	12.283f	382181	2.564 ug/ml
10) N-TETRACOSANE	14.511	238822	1.674 ug/ml
12) N-OCTACOSANE	16.467	97193	0.693 ug/ml
13) N-TRIACONTANE	17.360	131895	0.953 ug/ml
15) N-TETRATRIACONTANE	18.972	98826	0.818 ug/ml
16) N-HEXATRIACONTANE	19.713	115433	1.037 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082818\
Data File : FF001956.D
Signal(s) : FID2B.ch
Acq On : 28 Aug 2018 16:19
Operator : AJ\SJ
Sample : J4277-09 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 29 04:33:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

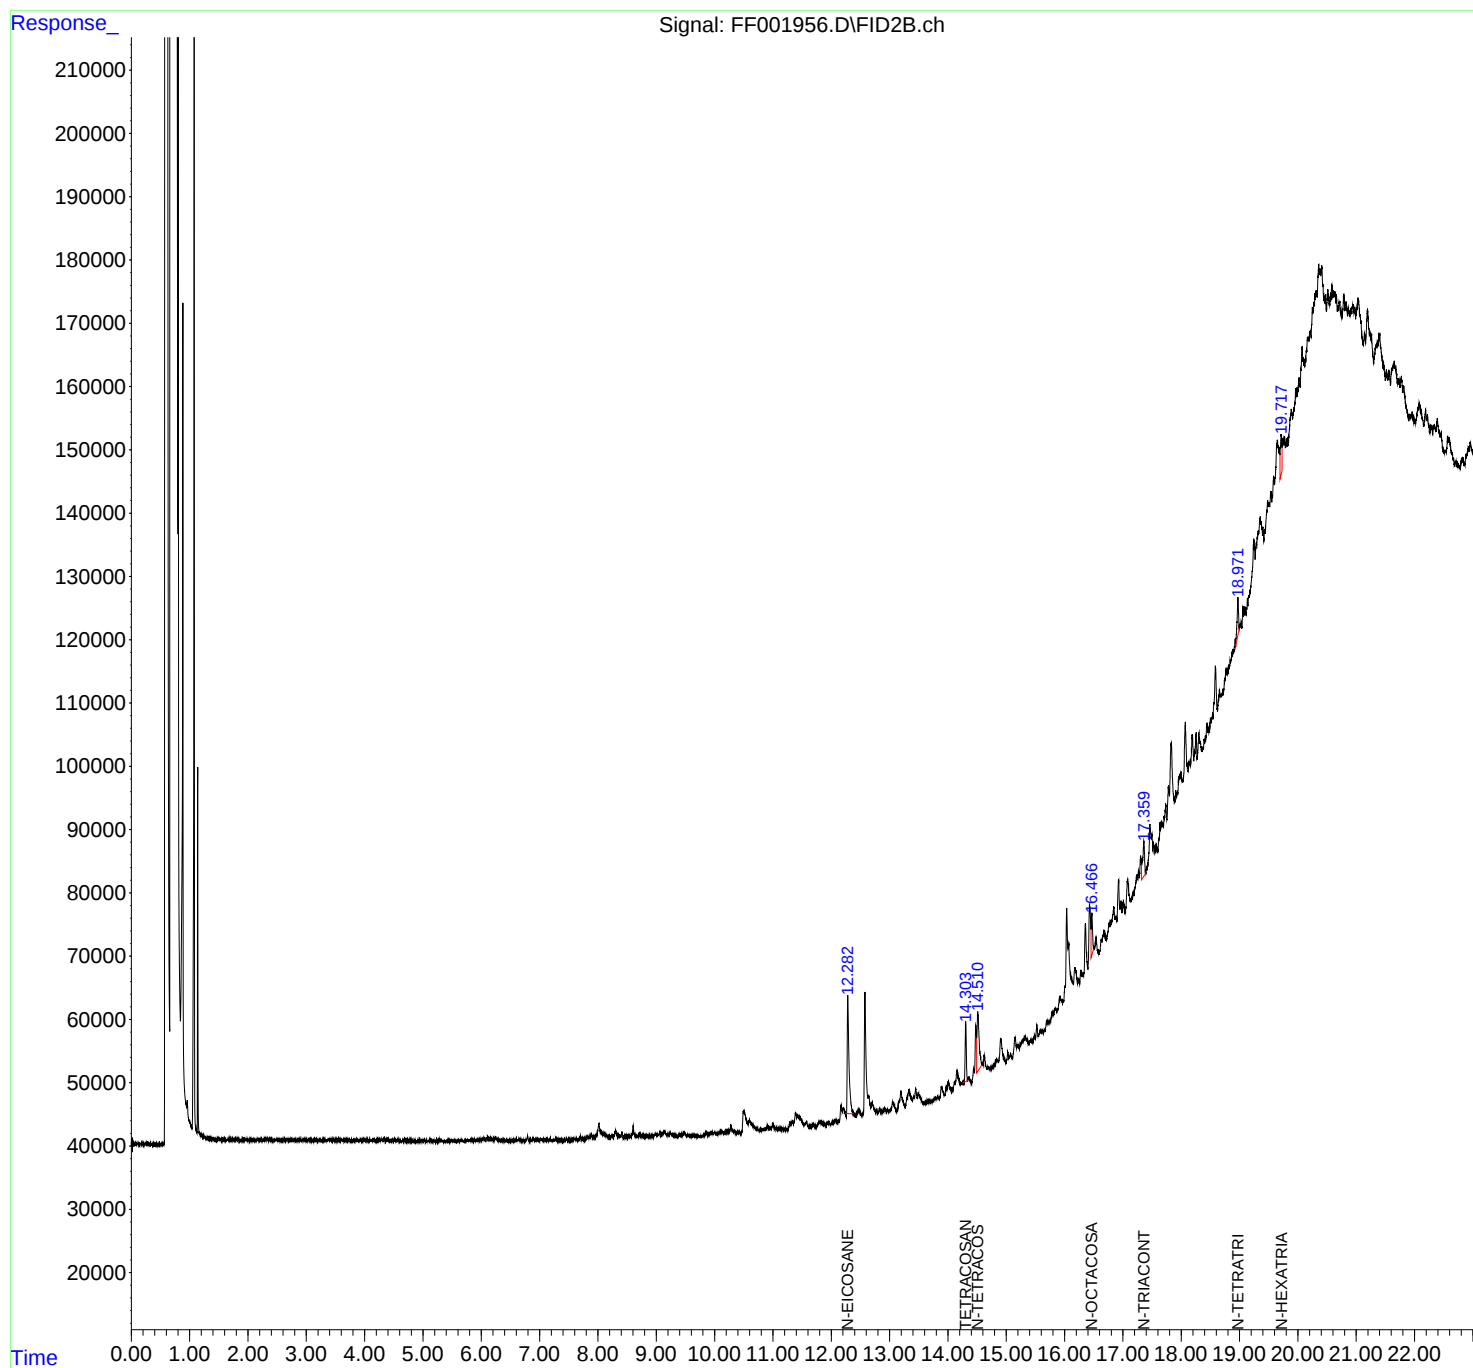

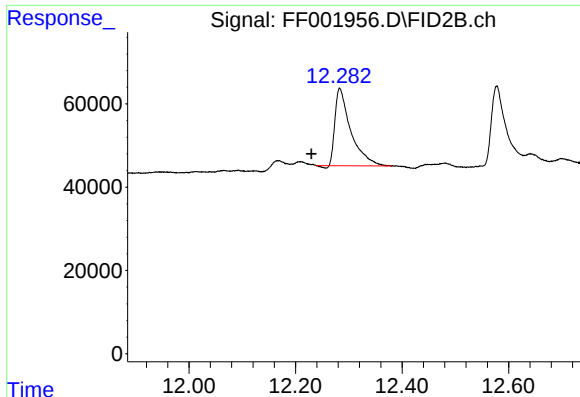


#7 N-EICOSANE

R.T.: 12.283 min
Delta R.T.: 0.053 min
Response: 382181
Conc: 2.56 ug/ml

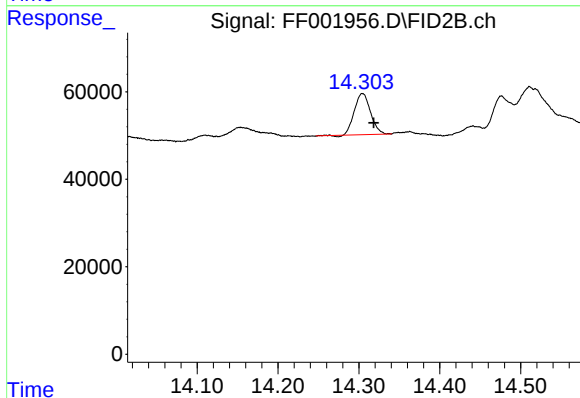


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.305 min
Delta R.T.: -0.014 min
Response: 129748
Conc: 1.03 ug/ml

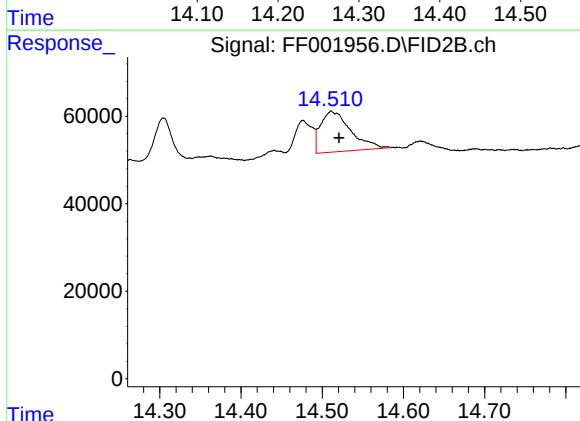


#10 N-TETRACOSANE

R.T.: 14.511 min
Delta R.T.: -0.010 min
Response: 238822
Conc: 1.67 ug/ml

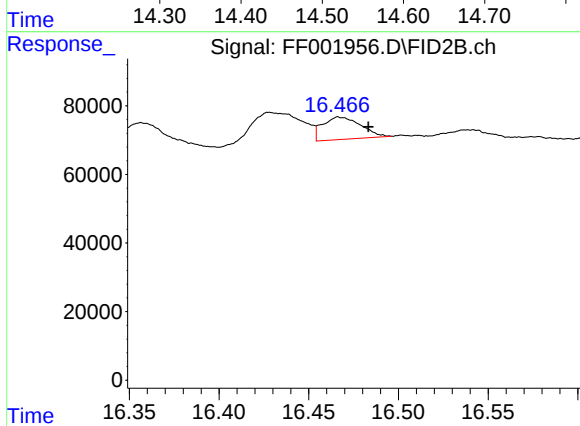


#12 N-OCTACOSANE

R.T.: 16.467 min
Delta R.T.: -0.016 min
Response: 97193
Conc: 0.69 ug/ml

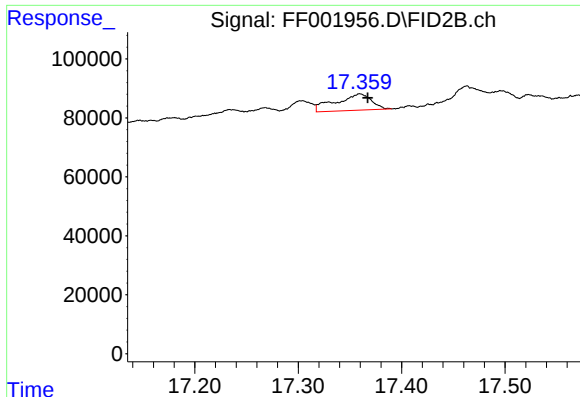


#13 N-TRIACONTANE

R.T.: 17.360 min
Delta R.T.: -0.007 min
Response: 131895
Conc: 0.95 ug/ml

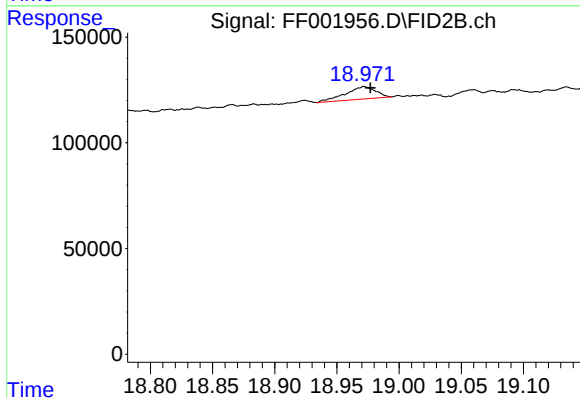

#15 N-TETRATRIACONTANE

R.T.: 18.972 min
Delta R.T.: -0.005 min
Response: 98826
Conc: 0.82 ug/ml

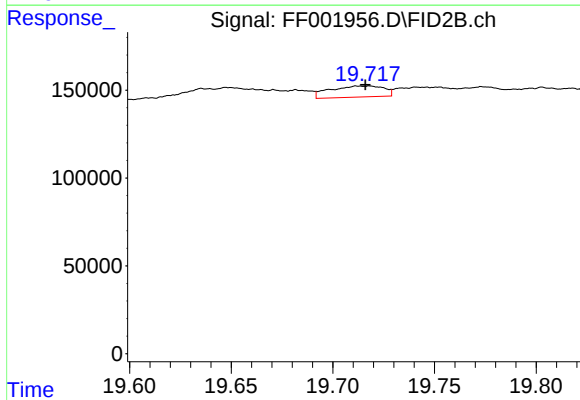

#16 N-HEXATRIACONTANE

R.T.: 19.713 min
Delta R.T.: -0.003 min
Response: 115433
Conc: 1.04 ug/ml