

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082819\
Data File : FF005375.D
Signal(s) : FID2B.ch
Acq On : 28 Aug 2019 12:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 28 14:31:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.640	2347258	21.314 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.558	96099	0.772 ug/ml
15) N-TETRATRIACONTANE	19.353	110751	0.941 ug/ml
16) N-HEXATRIACONTANE	20.099	253050	2.259 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082819\
Data File : FF005375.D
Signal(s) : FID2B.ch
Acq On : 28 Aug 2019 12:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 28 14:31:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

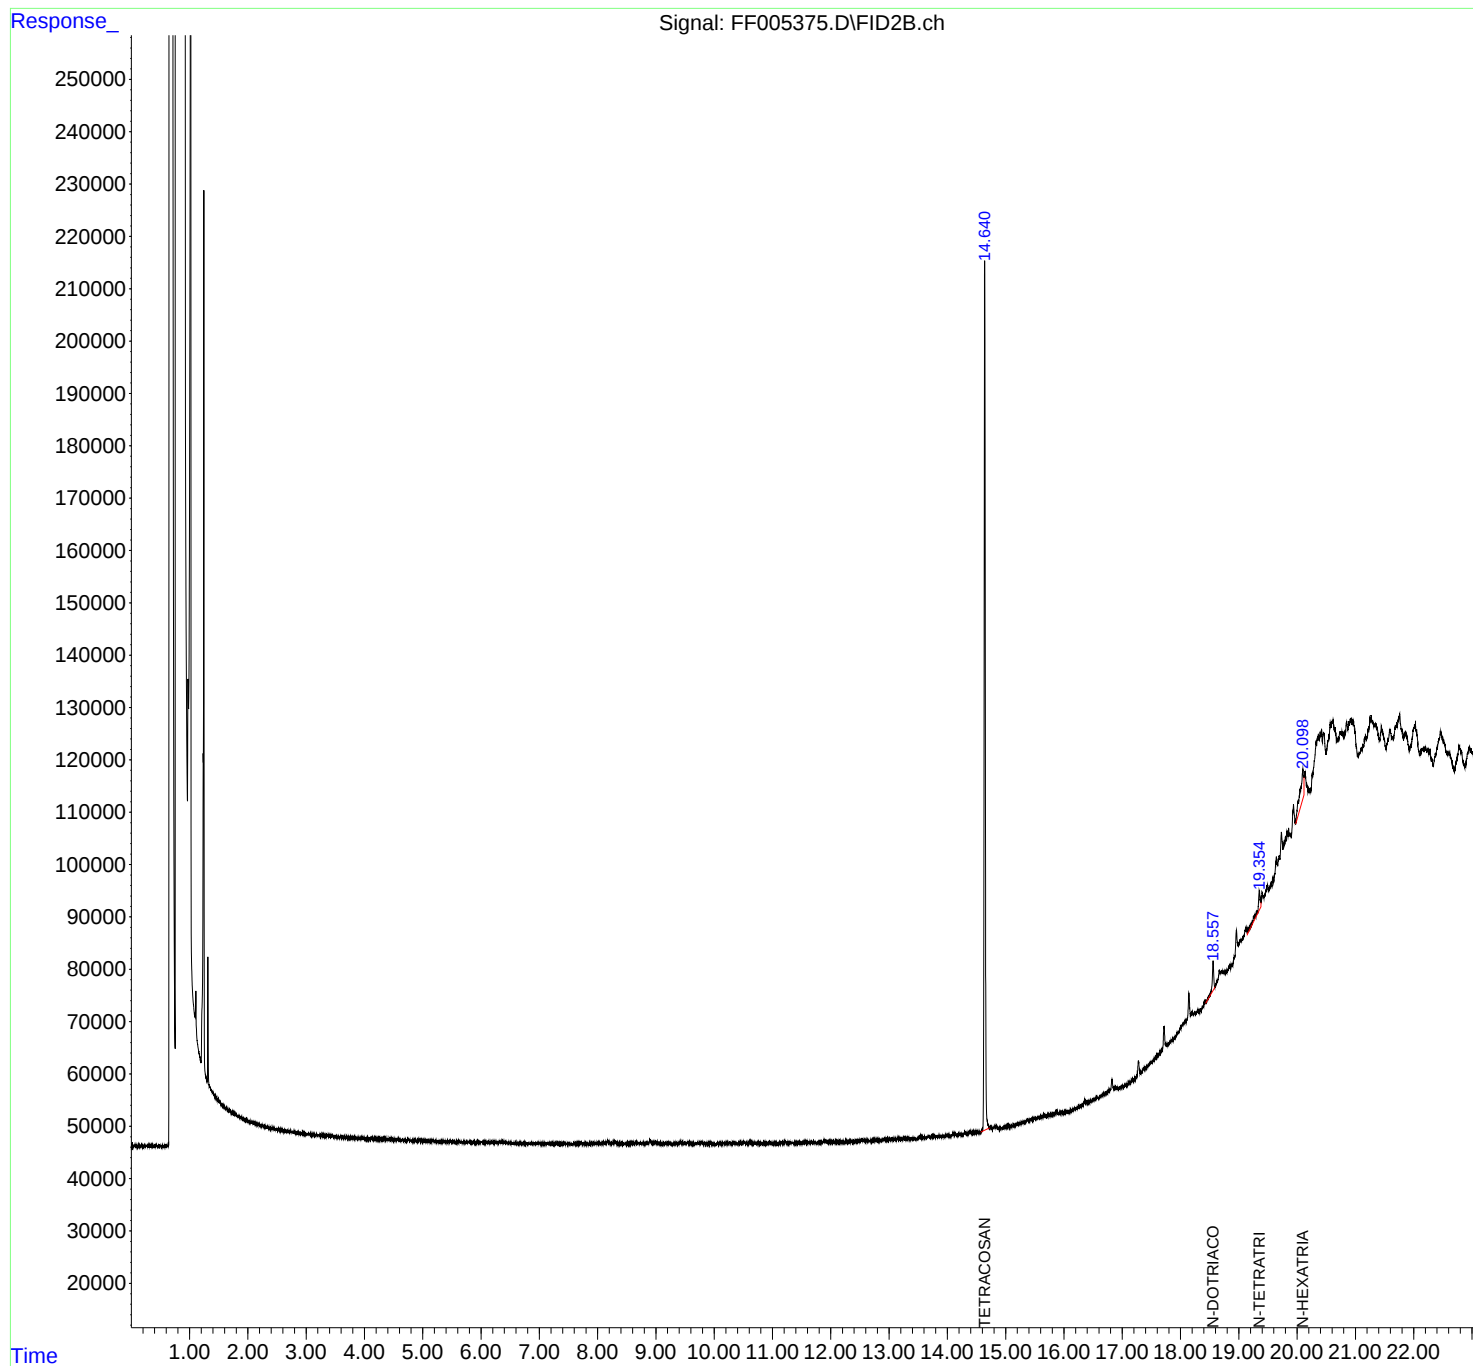


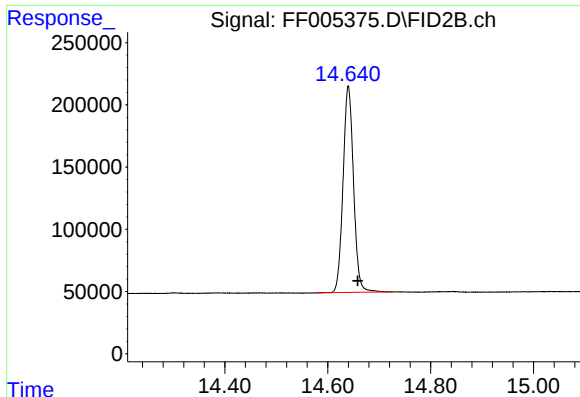

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.640 min
Delta R.T.: -0.018 min
Response: 2347258
Conc: 21.31 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

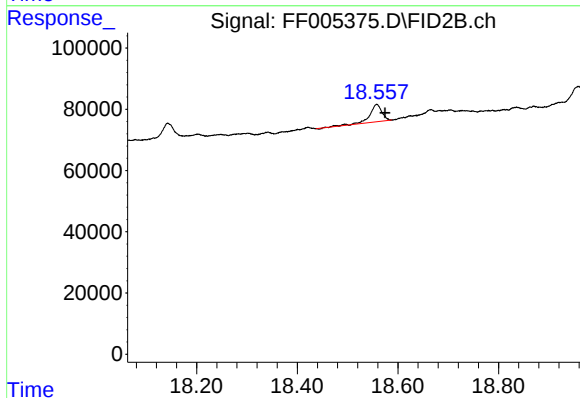


#14 N-DOTRIACONTANE

R.T.: 18.558 min
Delta R.T.: -0.017 min
Response: 96099
Conc: 0.77 ug/ml

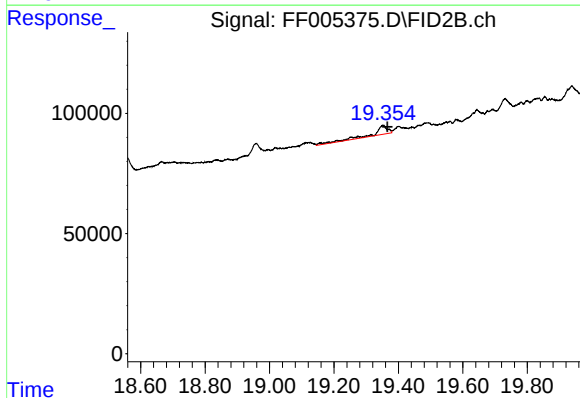

#15 N-TETRATRIACONTANE

R.T.: 19.353 min
Delta R.T.: -0.012 min
Response: 110751
Conc: 0.94 ug/ml

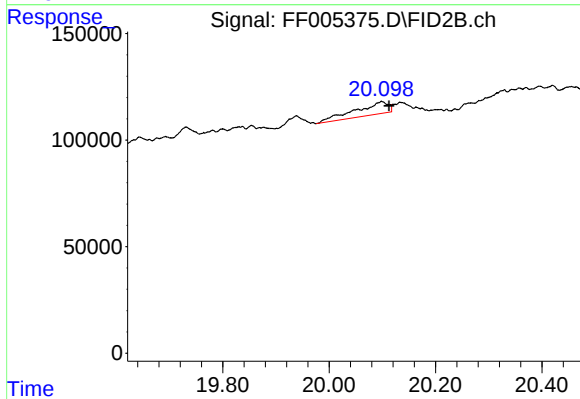

#16 N-HEXATRIACONTANE

R.T.: 20.099 min
Delta R.T.: -0.014 min
Response: 253050
Conc: 2.26 ug/ml