

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082819\
 Data File : FF005383.D
 Signal(s) : FID2B.ch
 Acq On : 28 Aug 2019 17:05
 Operator : DD\AJ
 Sample : K4568-08
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-17-COMP

Integration File: autoint1.e
 Quant Time: Aug 28 22:59:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
 Quant Title :
 QLast Update : Tue Jul 30 14:33:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.640	1531879	13.910 ug/ml
Target Compounds			
4) N-TETRADECANE	8.235	830853	5.772 ug/ml
7) N-EICOSANE	12.597	183595	1.368 ug/ml
10) N-TETRACOSANE	14.840	164143	1.303 ug/ml
11) N-HEXACOSANE	15.869	124828	1.010 ug/ml
12) N-OCTACOSANE	16.823	184583	1.478 ug/ml
13) N-TRIACONTANE	17.715	207659	1.628 ug/ml
14) N-DOTRIACONTANE	18.553	207403	1.666 ug/ml
16) N-HEXATRIACONTANE	20.096	139716	1.247 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082819\
Data File : FF005383.D
Signal(s) : FID2B.ch
Acq On : 28 Aug 2019 17:05
Operator : DD\AJ
Sample : K4568-08
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-17-COMP

Integration File: autoint1.e
Quant Time: Aug 28 22:59:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

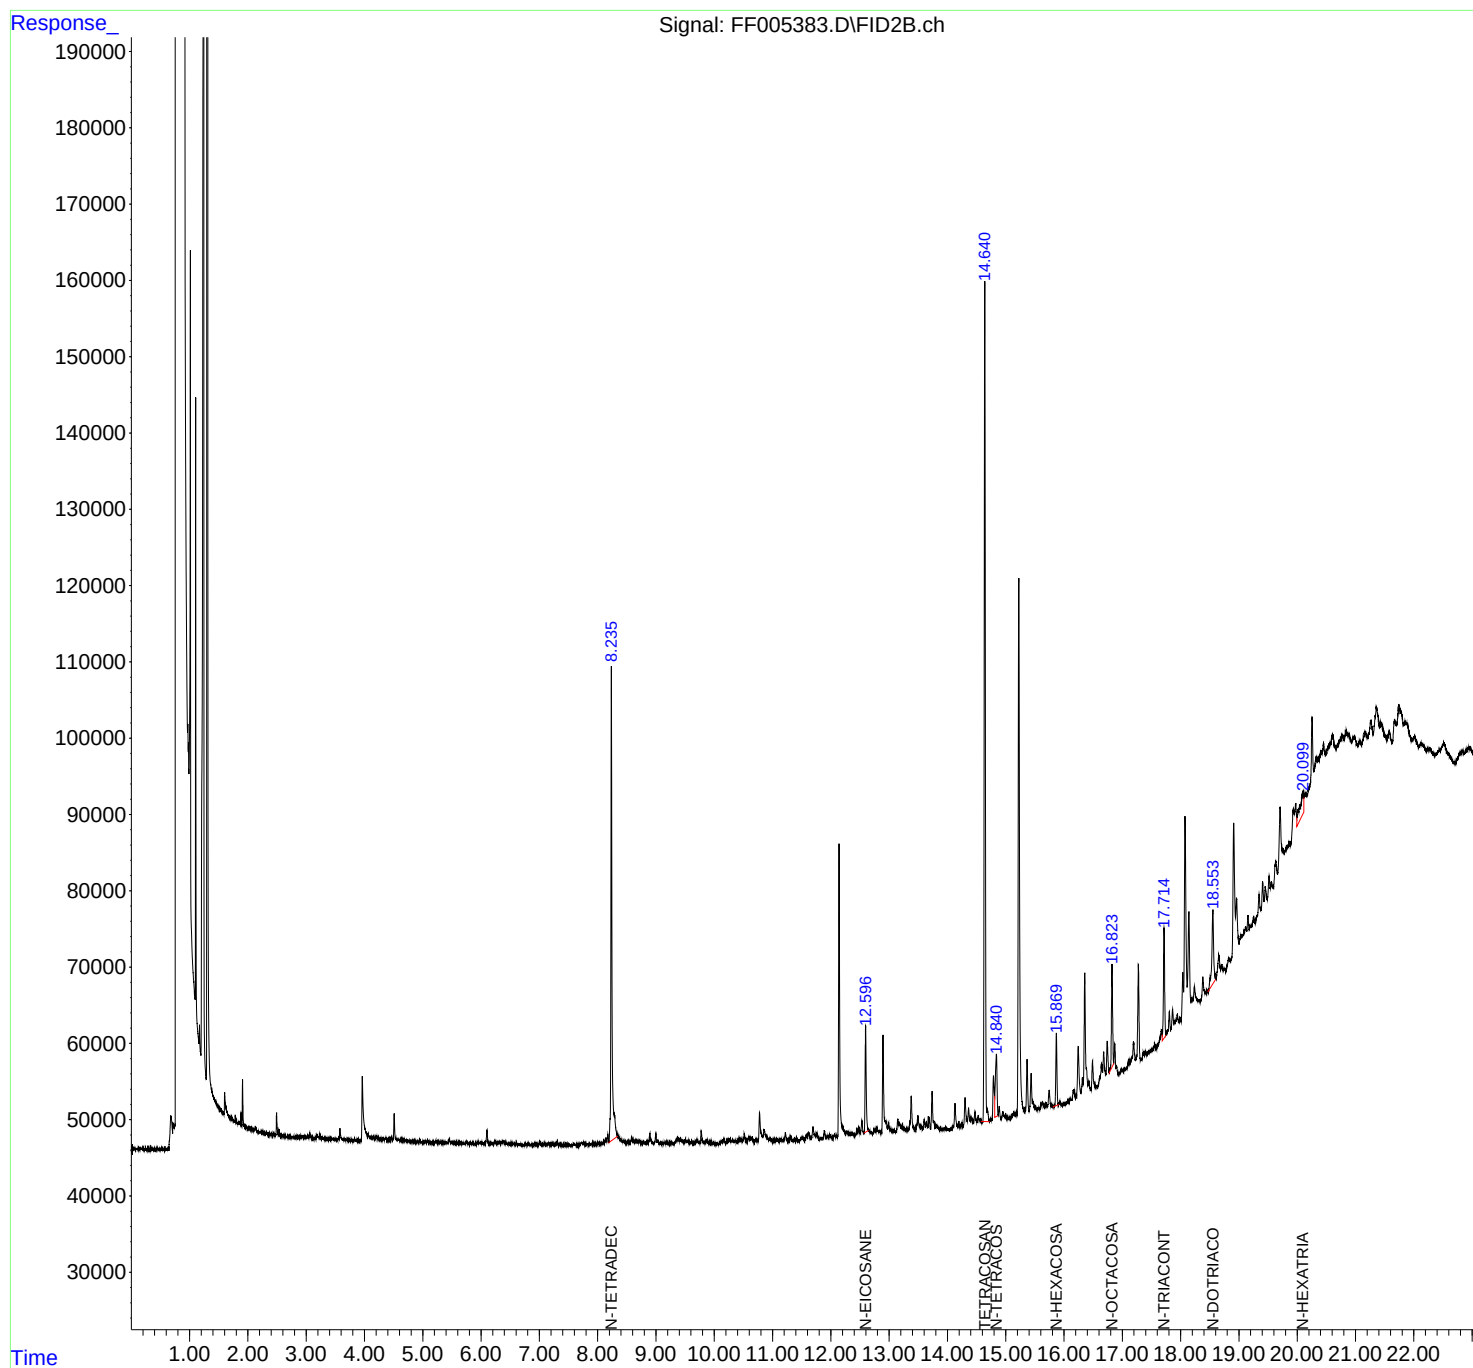


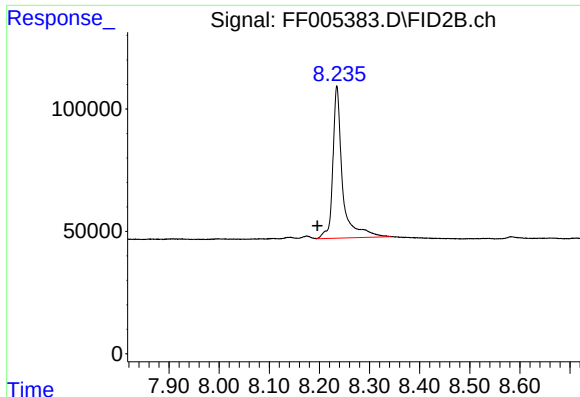

#4 N-TETRADECANE


R.T.: 8.235 min
Delta R.T.: 0.039 min
Response: 830853
Conc: 5.77 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-17-COMP

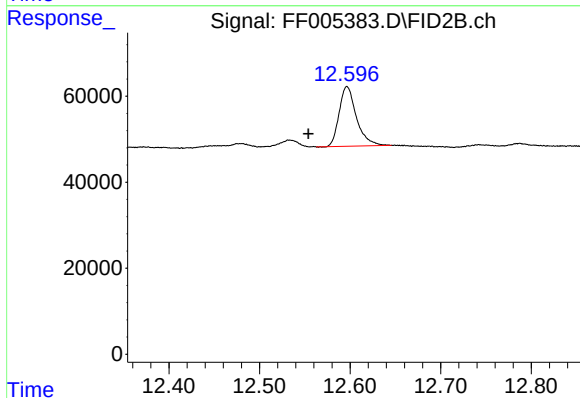


#7 N-EICOSANE

R.T.: 12.597 min
Delta R.T.: 0.043 min
Response: 183595
Conc: 1.37 ug/ml

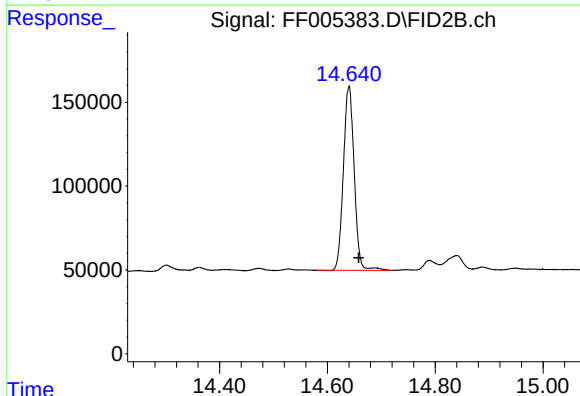


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.640 min
Delta R.T.: -0.018 min
Response: 1531879
Conc: 13.91 ug/ml

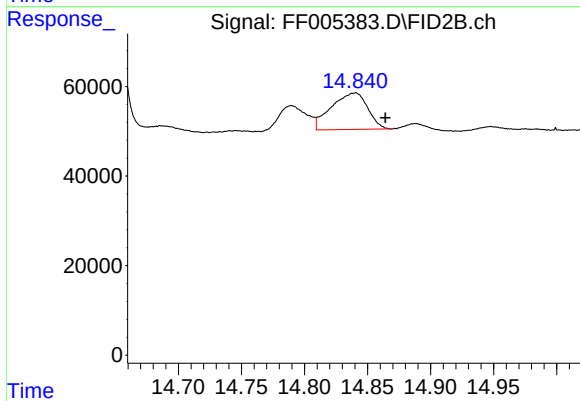

#10 N-TETRACOSANE


R.T.: 14.840 min
Delta R.T.: -0.024 min
Response: 164143
Conc: 1.30 ug/ml

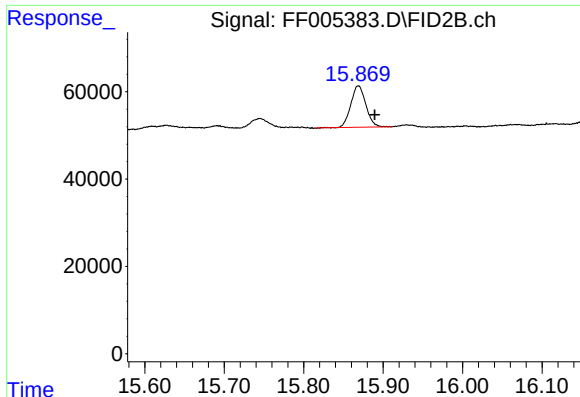

#11 N-HEXACOSANE


R.T.: 15.869 min
Delta R.T.: -0.021 min
Response: 124828
Conc: 1.01 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-17-COMP

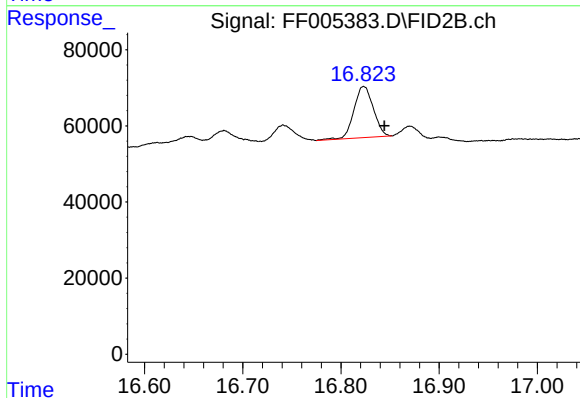


#12 N-OCTACOSANE

R.T.: 16.823 min
Delta R.T.: -0.021 min
Response: 184583
Conc: 1.48 ug/ml

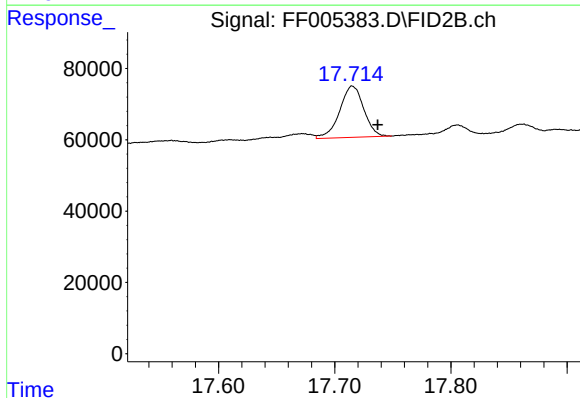


#13 N-TRIACONTANE

R.T.: 17.715 min
Delta R.T.: -0.022 min
Response: 207659
Conc: 1.63 ug/ml

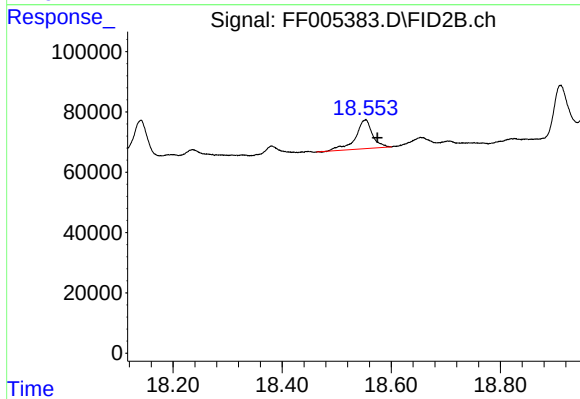

#14 N-DOTRIACONTANE

R.T.: 18.553 min
Delta R.T.: -0.022 min
Response: 207403
Conc: 1.67 ug/ml

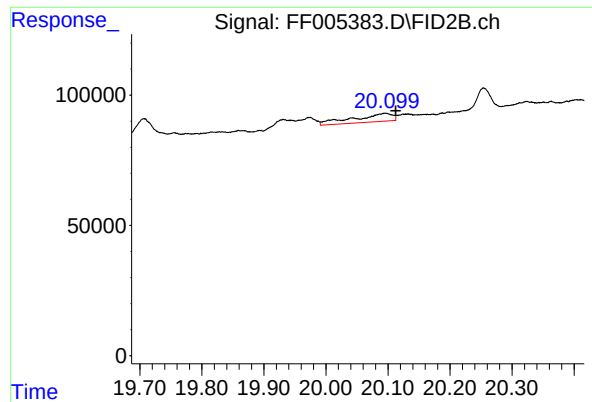

#16 N-HEXATRIACONTANE

R.T.: 20.096 min
Delta R.T.: -0.017 min
Response: 139716
Conc: 1.25 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-17-COMP