

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082819\  
Data File : FF005386.D  
Signal(s) : FID2B.ch  
Acq On : 28 Aug 2019 19:08  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Aug 28 23:00:01 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF073019.M  
Quant Title :  
QLast Update : Tue Jul 30 14:33:00 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.639 | 2264199  | 20.560 ug/ml |
| Target Compounds              |        |          |              |
| 13) N-TRIACONTANE             | 17.716 | 88340    | 0.693 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.553 | 130186   | 1.046 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082819\  
Data File : FF005386.D  
Signal(s) : FID2B.ch  
Acq On : 28 Aug 2019 19:08  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Aug 28 23:00:01 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF073019.M  
Quant Title :  
QLast Update : Tue Jul 30 14:33:00 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

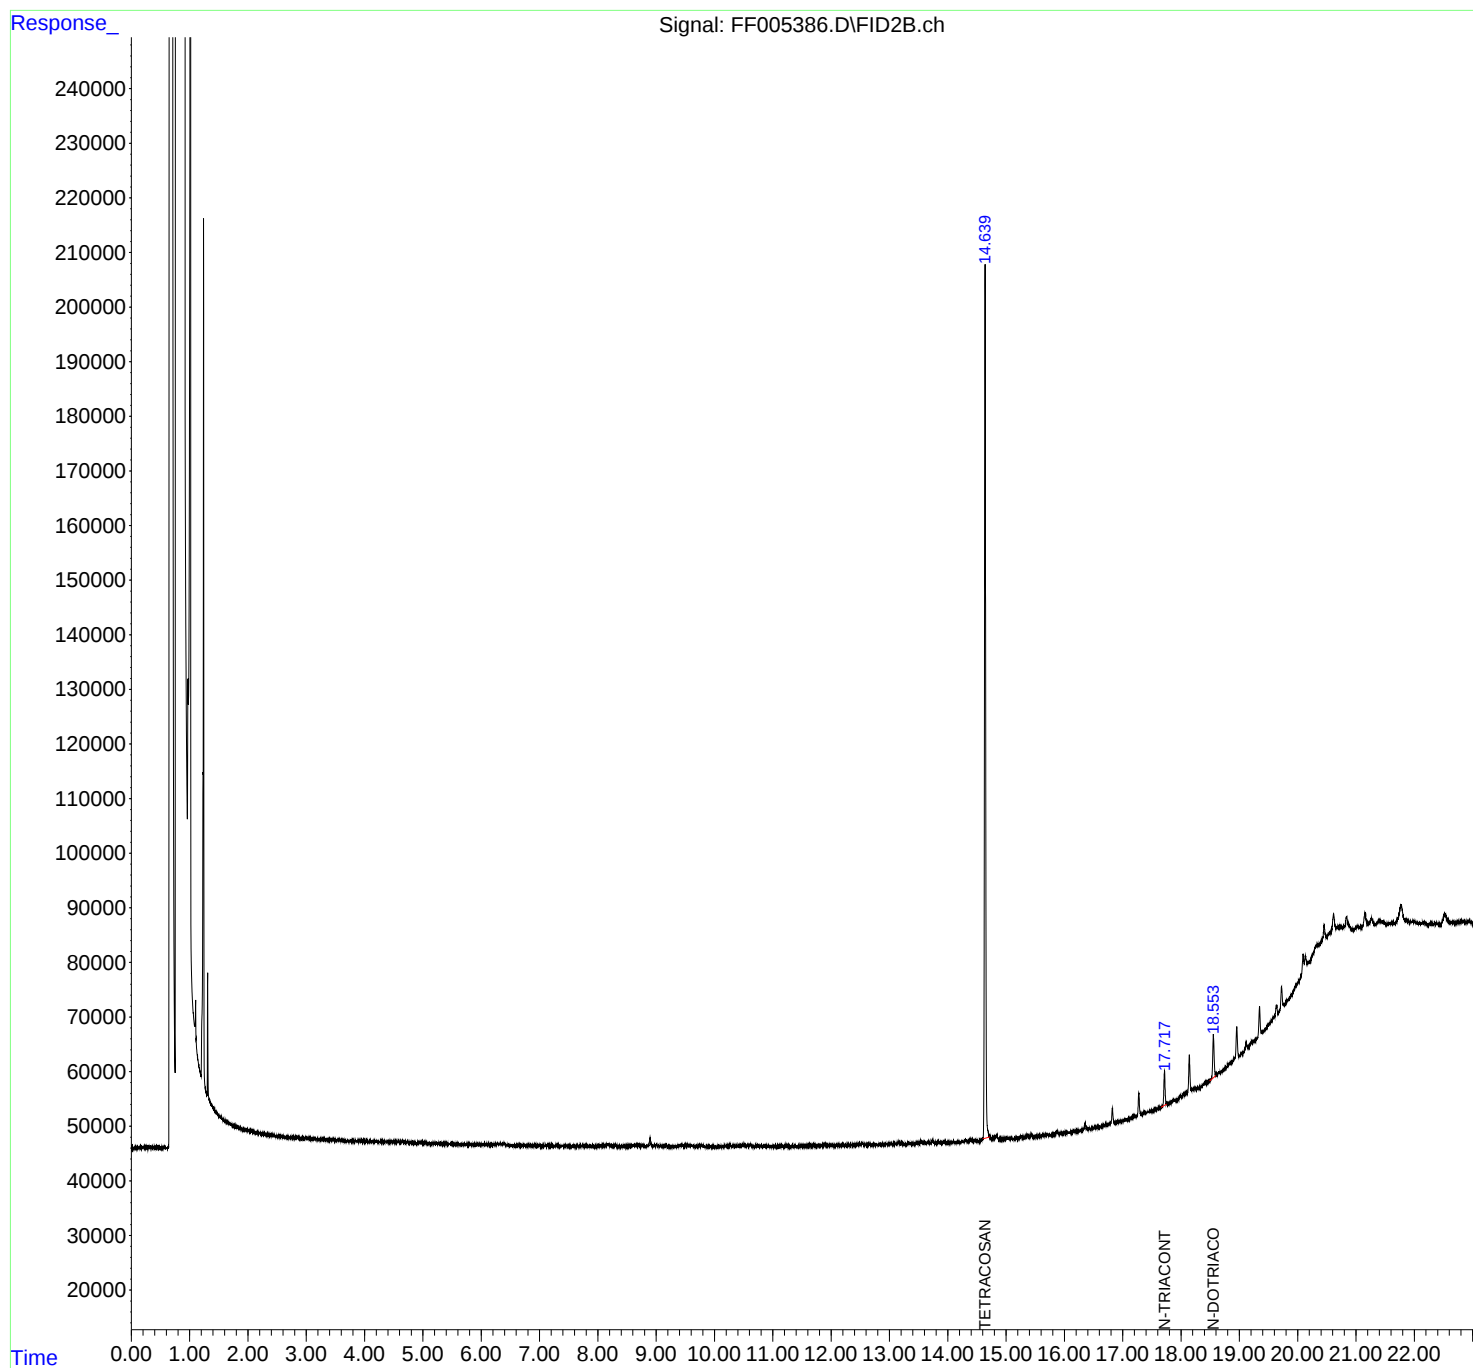


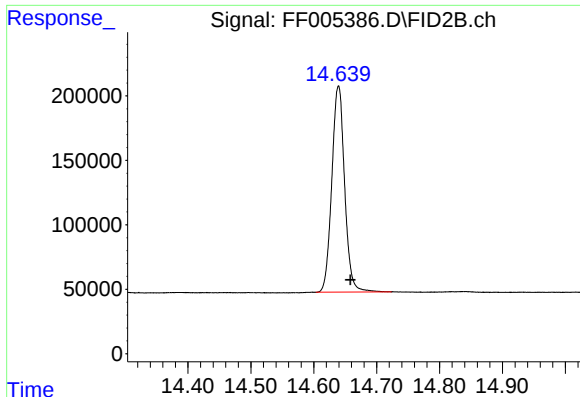

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.639 min  
Delta R.T.: -0.019 min  
Response: 2264199  
Conc: 20.56 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

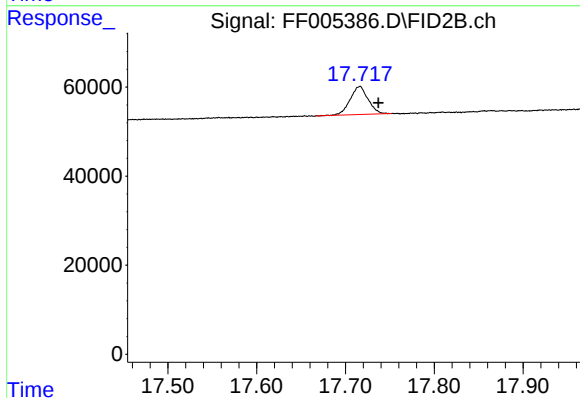

#13 N-TRIACONTANE

R.T.: 17.716 min  
Delta R.T.: -0.021 min  
Response: 88340  
Conc: 0.69 ug/ml

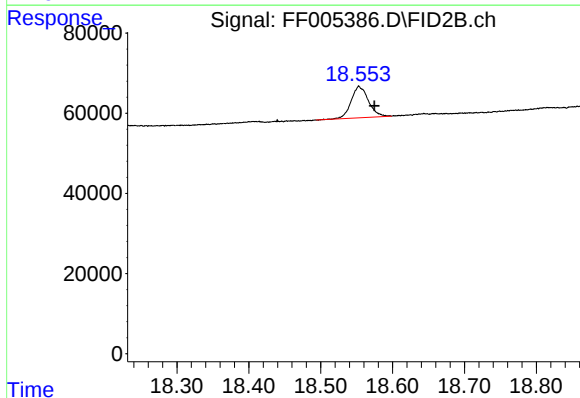

#14 N-DOTRIACONTANE

R.T.: 18.553 min  
Delta R.T.: -0.022 min  
Response: 130186  
Conc: 1.05 ug/ml