

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082919\
 Data File : FF005398.D
 Signal(s) : FID2B.ch
 Acq On : 29 Aug 2019 17:17
 Operator : DD\AJ
 Sample : K4596-11
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 EB-3-082819

Integration File: autoint1.e
 Quant Time: Aug 29 23:47:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
 Quant Title :
 QLast Update : Tue Jul 30 14:33:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.639	2290185	20.796 ug/ml
Target Compounds			
4) N-TETRADECANE	8.233	698320	4.852 ug/ml
10) N-TETRACOSANE	14.841	133407	1.059 ug/ml
11) N-HEXACOSANE	15.868	148841	1.205 ug/ml
12) N-OCTACOSANE	16.822	264390	2.117 ug/ml
13) N-TRIACONTANE	17.715	309200	2.425 ug/ml
14) N-DOTRIACONTANE	18.553	196967	1.582 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082919\
Data File : FF005398.D
Signal(s) : FID2B.ch
Acq On : 29 Aug 2019 17:17
Operator : DD\AJ
Sample : K4596-11
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EB-3-082819

Integration File: autoint1.e
Quant Time: Aug 29 23:47:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

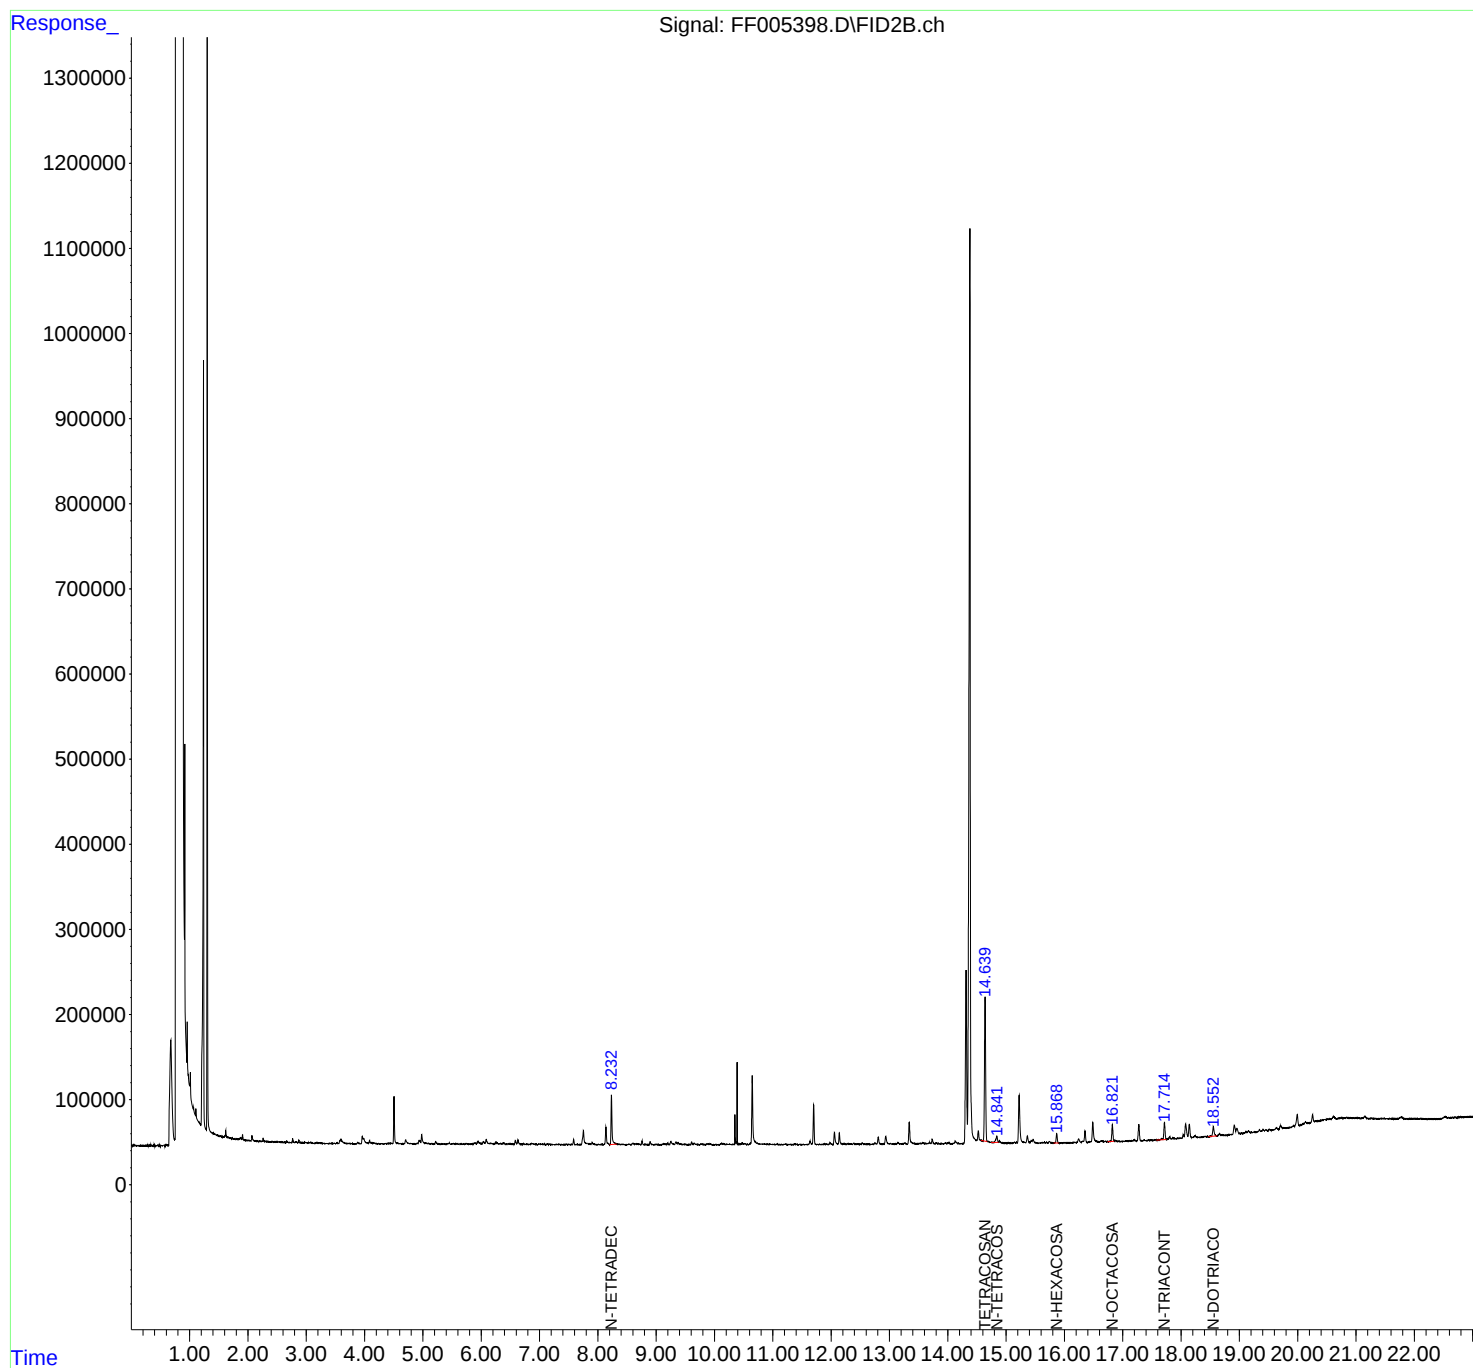


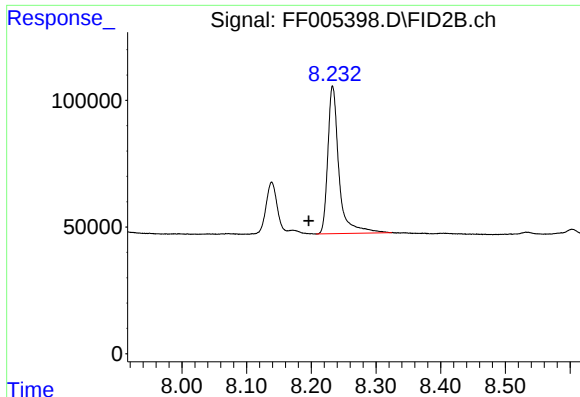

#4 N-TETRADECANE


R.T.: 8.233 min
Delta R.T.: 0.037 min
Response: 698320
Conc: 4.85 ug/ml

Instrument :
FID_F
ClientSampleId :
EB-3-082819

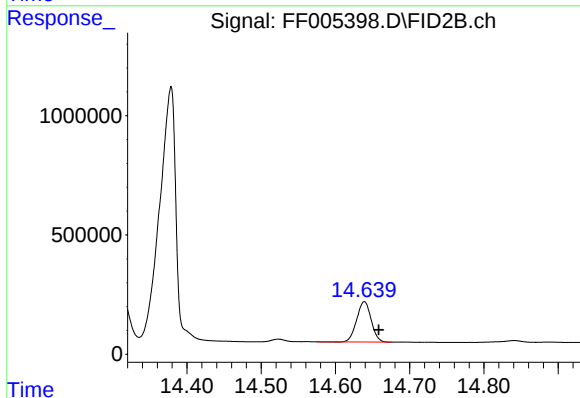


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.639 min
Delta R.T.: -0.019 min
Response: 2290185
Conc: 20.80 ug/ml

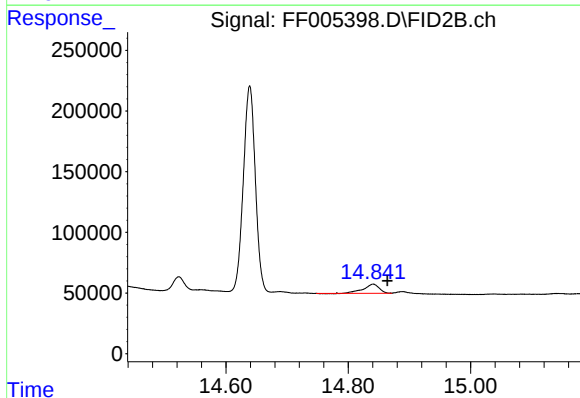


#10 N-TETRACOSANE

R.T.: 14.841 min
Delta R.T.: -0.023 min
Response: 133407
Conc: 1.06 ug/ml

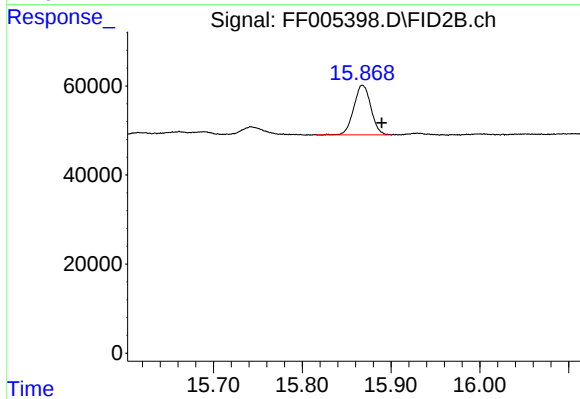

#11 N-HEXACOSANE


R.T.: 15.868 min
Delta R.T.: -0.022 min
Response: 148841
Conc: 1.20 ug/ml

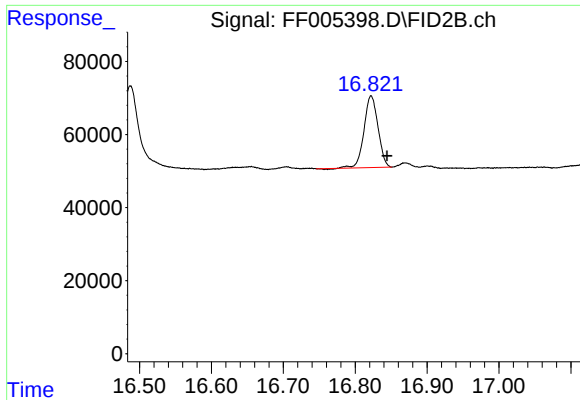

#12 N-OCTACOSANE


R.T.: 16.822 min
Delta R.T.: -0.022 min
Response: 264390
Conc: 2.12 ug/ml

Instrument :
FID_F
ClientSampleId :
EB-3-082819

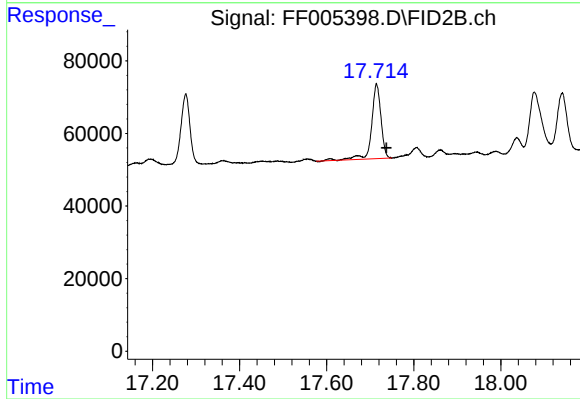

#13 N-TRIACONTANE

R.T.: 17.715 min
Delta R.T.: -0.022 min
Response: 309200
Conc: 2.42 ug/ml

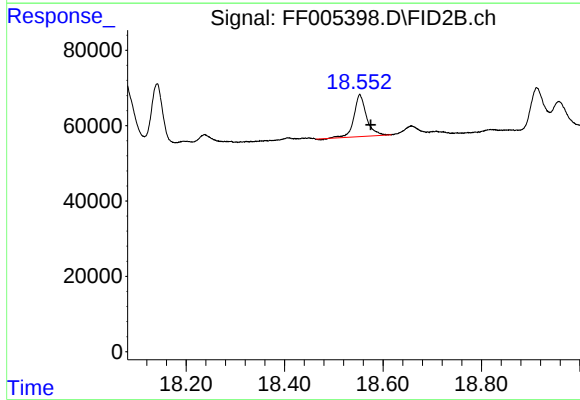

#14 N-DOTRIACONTANE

R.T.: 18.553 min
Delta R.T.: -0.022 min
Response: 196967
Conc: 1.58 ug/ml