

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082919\
 Data File : FF005401.D
 Signal(s) : FID2B.ch
 Acq On : 29 Aug 2019 18:49
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Aug 29 23:48:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
 Quant Title :
 QLast Update : Tue Jul 30 14:33:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.638	3197354	29.033 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.714	150081	1.177 ug/ml
14) N-DOTRIACONTANE	18.551	191616	1.539 ug/ml
15) N-TETRATRIACONTANE	19.343	136803	1.163 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082919\
Data File : FF005401.D
Signal(s) : FID2B.ch
Acq On : 29 Aug 2019 18:49
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 29 23:48:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

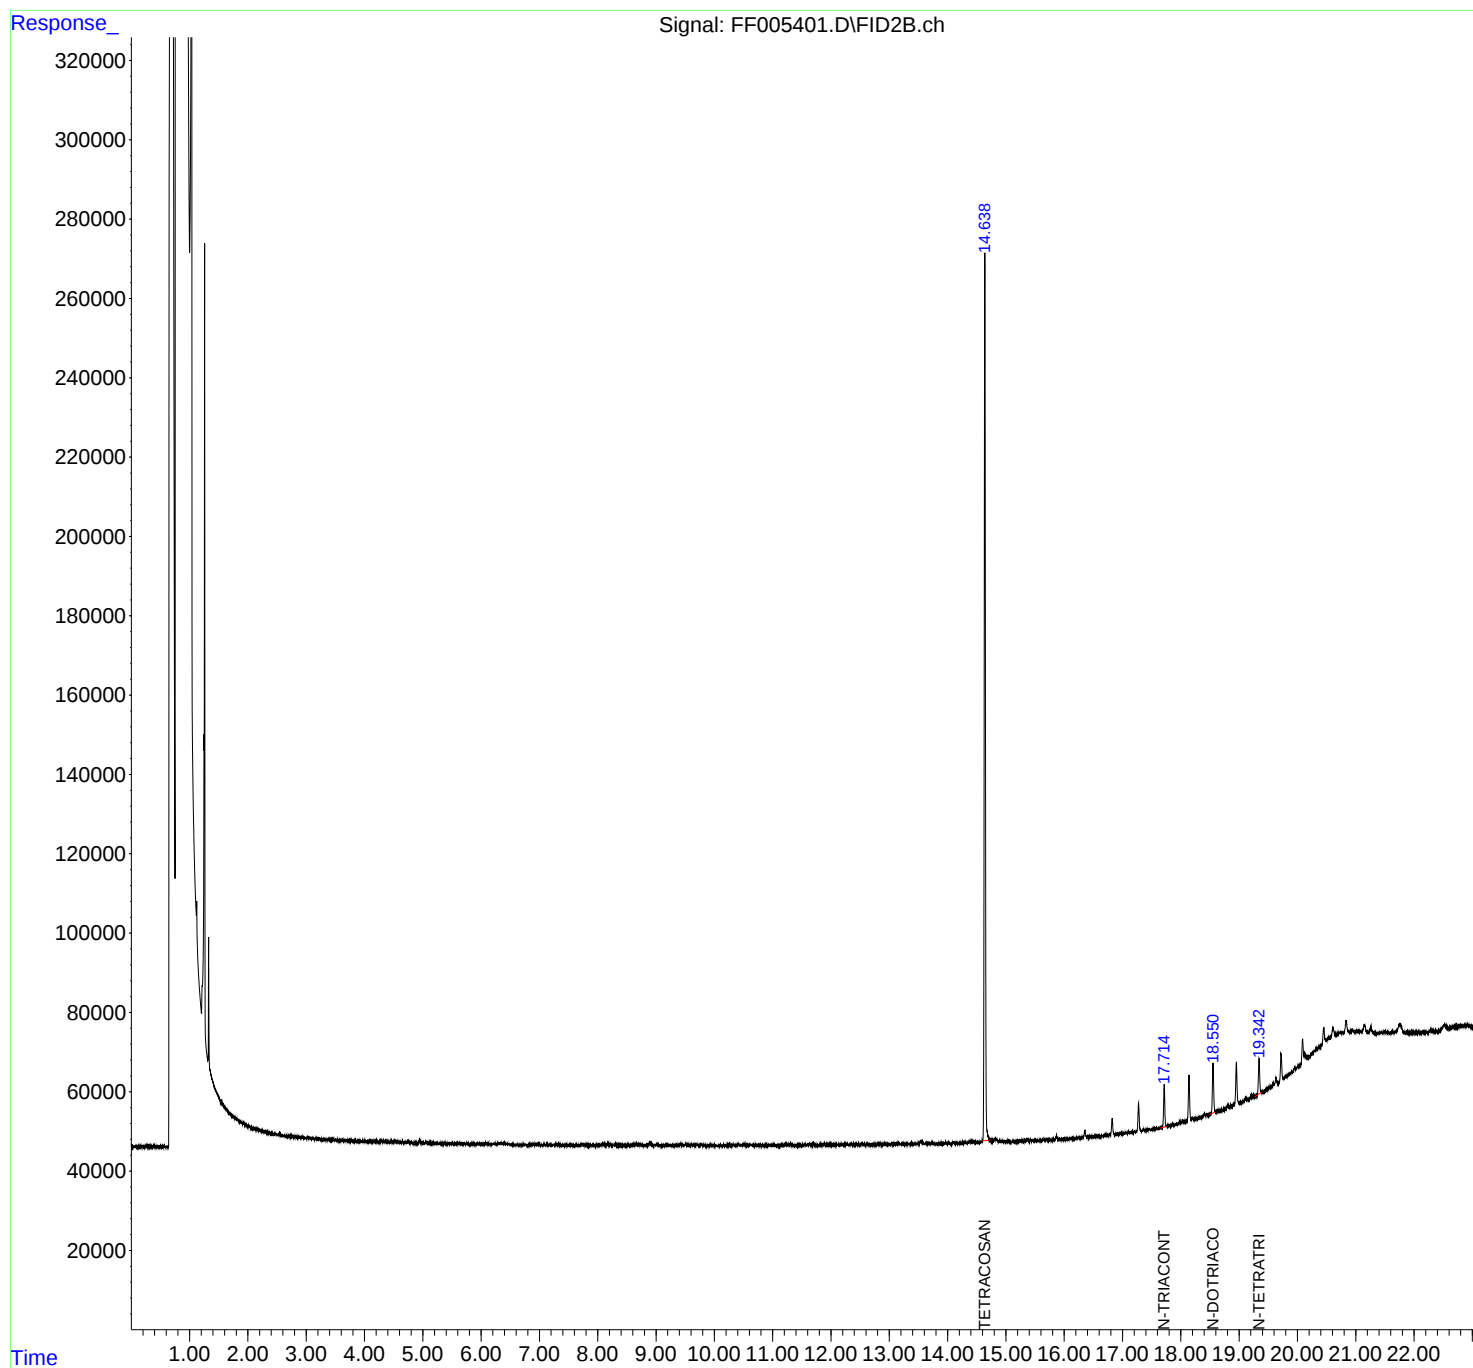


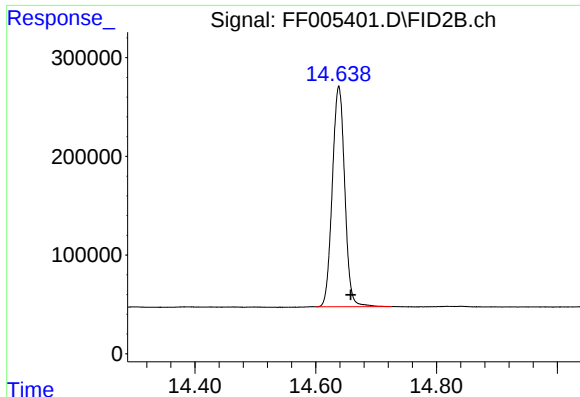

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.638 min
Delta R.T.: -0.020 min
Response: 3197354
Conc: 29.03 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

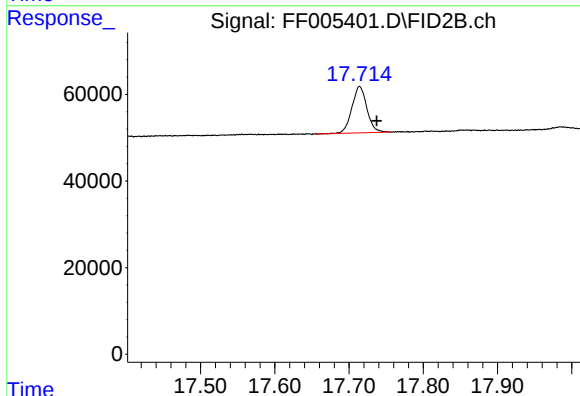


#13 N-TRIACONTANE

R.T.: 17.714 min
Delta R.T.: -0.023 min
Response: 150081
Conc: 1.18 ug/ml

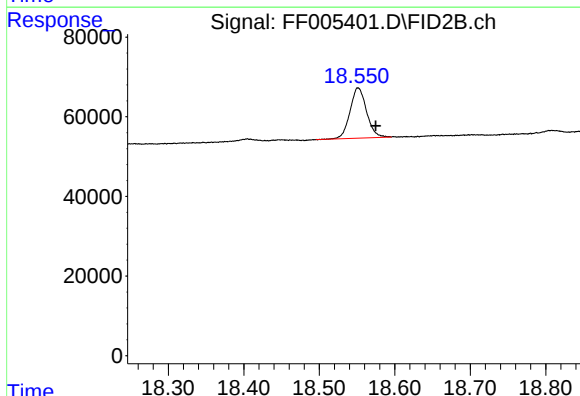

#14 N-DOTRIACONTANE

R.T.: 18.551 min
Delta R.T.: -0.024 min
Response: 191616
Conc: 1.54 ug/ml

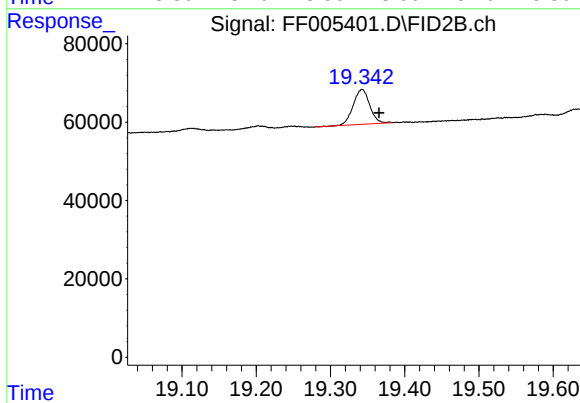

#15 N-TETRATRIACONTANE

R.T.: 19.343 min
Delta R.T.: -0.023 min
Response: 136803
Conc: 1.16 ug/ml