

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082919\
Data File : FF005392.D
Signal(s) : FID2B.ch
Acq On : 29 Aug 2019 11:23
Operator : DD\AJ
Sample : K4568-04 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-15-COMP

Integration File: autoint1.e
Quant Time: Aug 29 23:45:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	1283522	11.655 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082919\
Data File : FF005392.D
Signal(s) : FID2B.ch
Acq On : 29 Aug 2019 11:23
Operator : DD\AJ
Sample : K4568-04 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-15-COMP

Integration File: autoint1.e
Quant Time: Aug 29 23:45:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

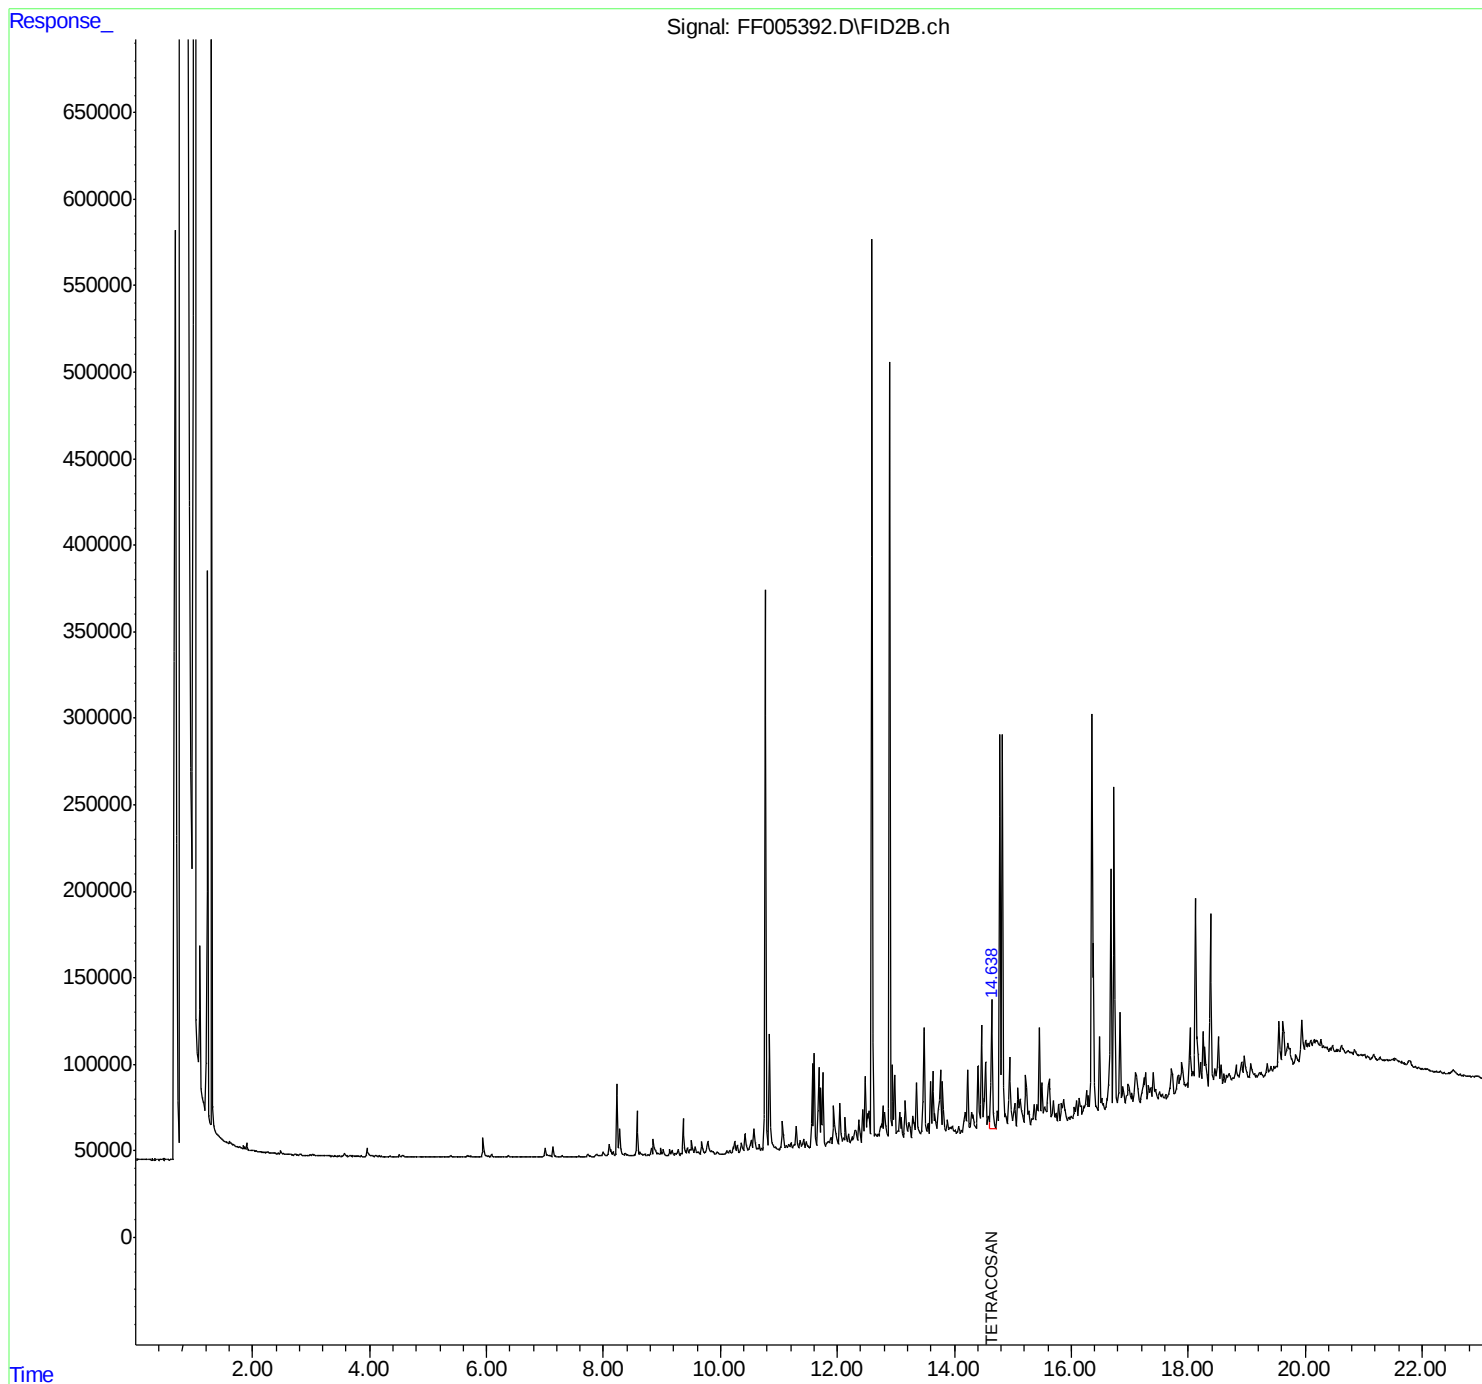

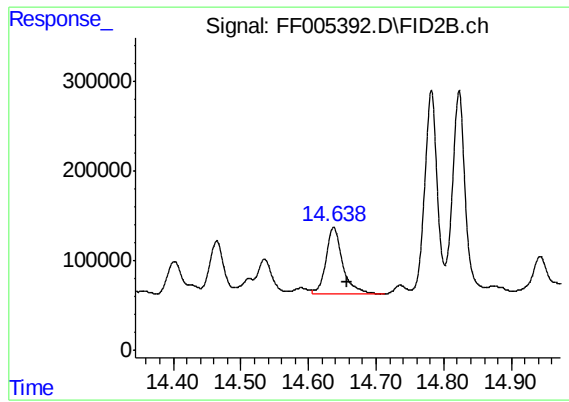

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.637 min
Delta R.T.: -0.021 min
Response: 1283522
Conc: 11.65 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-15-COMP