

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082923AL\
 Data File : FF013443.D
 Signal(s) : FID2B.ch
 Acq On : 29 Aug 2023 18:09
 Operator : YP\AJ
 Sample : 04197-19
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 OR-309-OK-370-45

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/30/2023
 Supervised By :Ankita Jodhani 08/30/2023

Integration File: autoint1.e
 Quant Time: Aug 29 23:12:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 10 16:05:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.894	6263545	45.588 ug/mlm
Spiked Amount 50.000		Recovery =	91.18%
12) S 1-chlorooctadecane (S...	13.333	4823403	46.028 ug/ml
Spiked Amount 50.000		Recovery =	92.06%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082923AL\
Data File : FF013443.D
Signal(s) : FID2B.ch
Acq On : 29 Aug 2023 18:09
Operator : YP\AJ
Sample : 04197-19
Misc :
ALS Vial : 68 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
OR-309-OK-370-45


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2023
Supervised By :Ankita Jodhani 08/30/2023

Integration File: autoint1.e
Quant Time: Aug 29 23:12:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 16:05:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

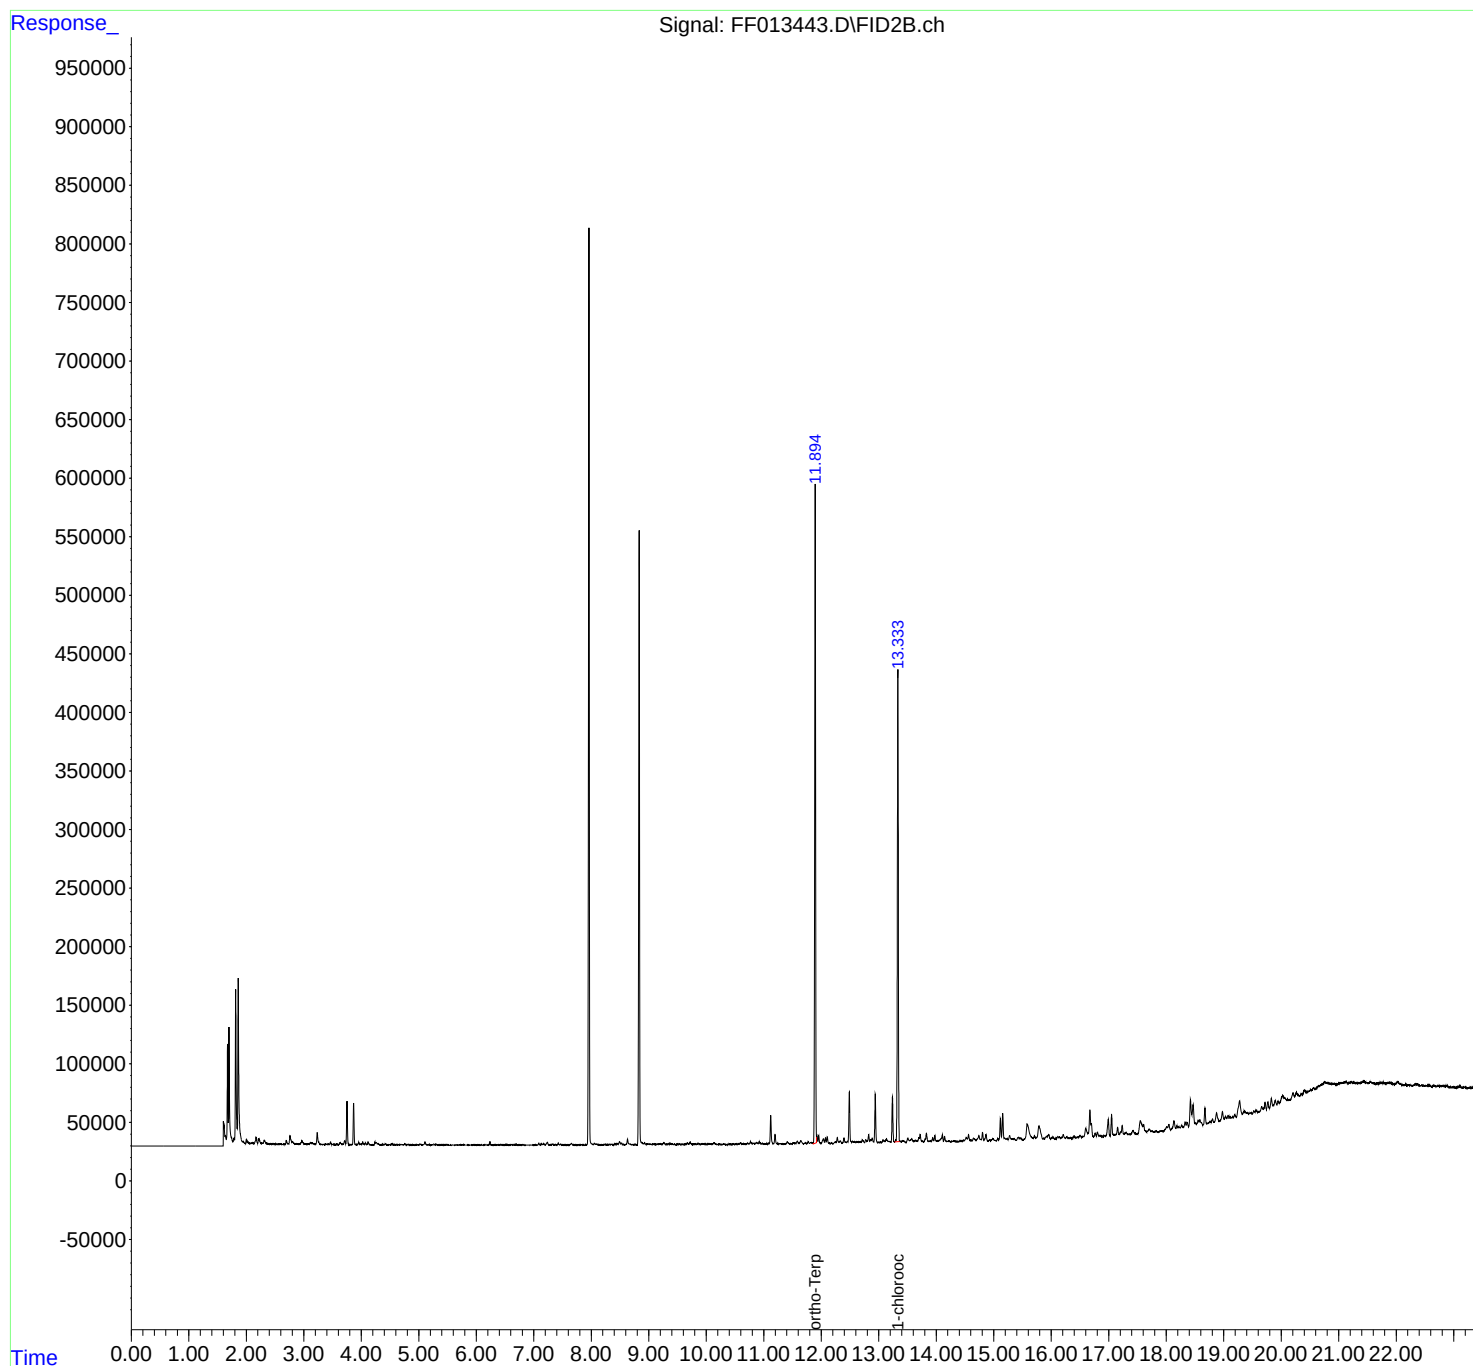

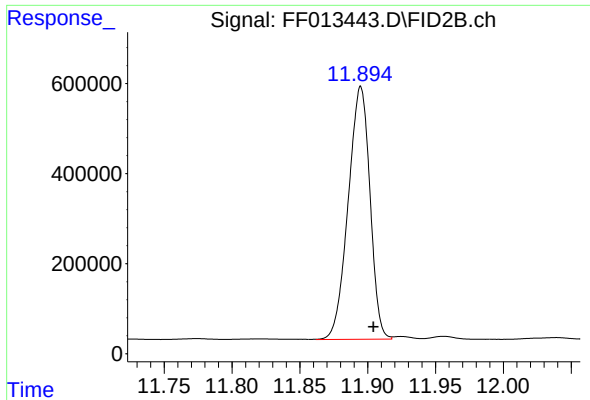


#9 ortho-Terphenyl (SURR)

R.T.: 11.894 min
Delta R.T.: -0.010 min
Response: 6263545
Conc: 45.59 ug/ml

Instrument :
FID_F
ClientSampleId :
OR-309-OK-370-45

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/30/2023
Supervised By :Ankita Jodhani 08/30/2023

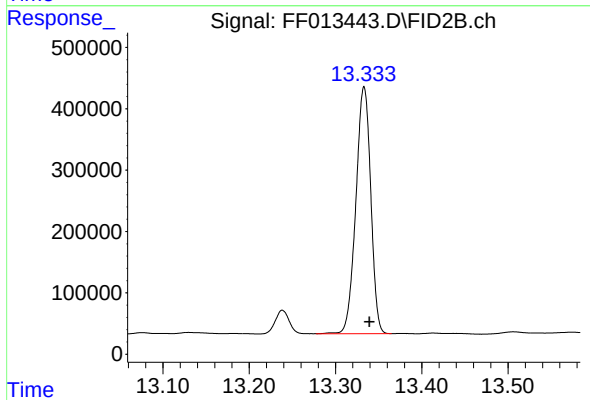

#12 1-chlorooctadecane (SURR)

R.T.: 13.333 min
Delta R.T.: -0.006 min
Response: 4823403
Conc: 46.03 ug/ml