

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF083022\
 Data File : FF011327.D
 Signal(s) : FID2B.ch
 Acq On : 30 Aug 2022 17:09
 Operator : YP\AJ
 Sample : PB147353BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB147353BS

Integration File: autoint1.e
 Quant Time: Aug 31 05:11:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.786	2047468	18.266 ug/ml
Target Compounds			
2) N-DECANE	4.349	2258055	17.403 ug/ml
3) N-DODECANE	6.518	2340946	17.877 ug/ml
4) N-TETRADECANE	8.342	2390160	18.197 ug/ml
5) N-HEXADECANE	9.946	2225057	16.775 ug/ml
6) N-OCTADECANE	11.385	2427266	18.260 ug/ml
7) N-EICOSANE	12.692	2398565	18.234 ug/ml
8) N-DOCOSANE	13.888	2343341	18.334 ug/ml
10) N-TETRACOSANE	14.989	2331049	18.307 ug/ml
11) N-HEXACOSANE	16.008	2261823	18.109 ug/ml
12) N-OCTACOSANE	16.956	2221129	18.133 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF083022\
Data File : FF011327.D
Signal(s) : FID2B.ch
Acq On : 30 Aug 2022 17:09
Operator : YP\AJ
Sample : PB147353BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB147353BS

Integration File: autoint1.e
Quant Time: Aug 31 05:11:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

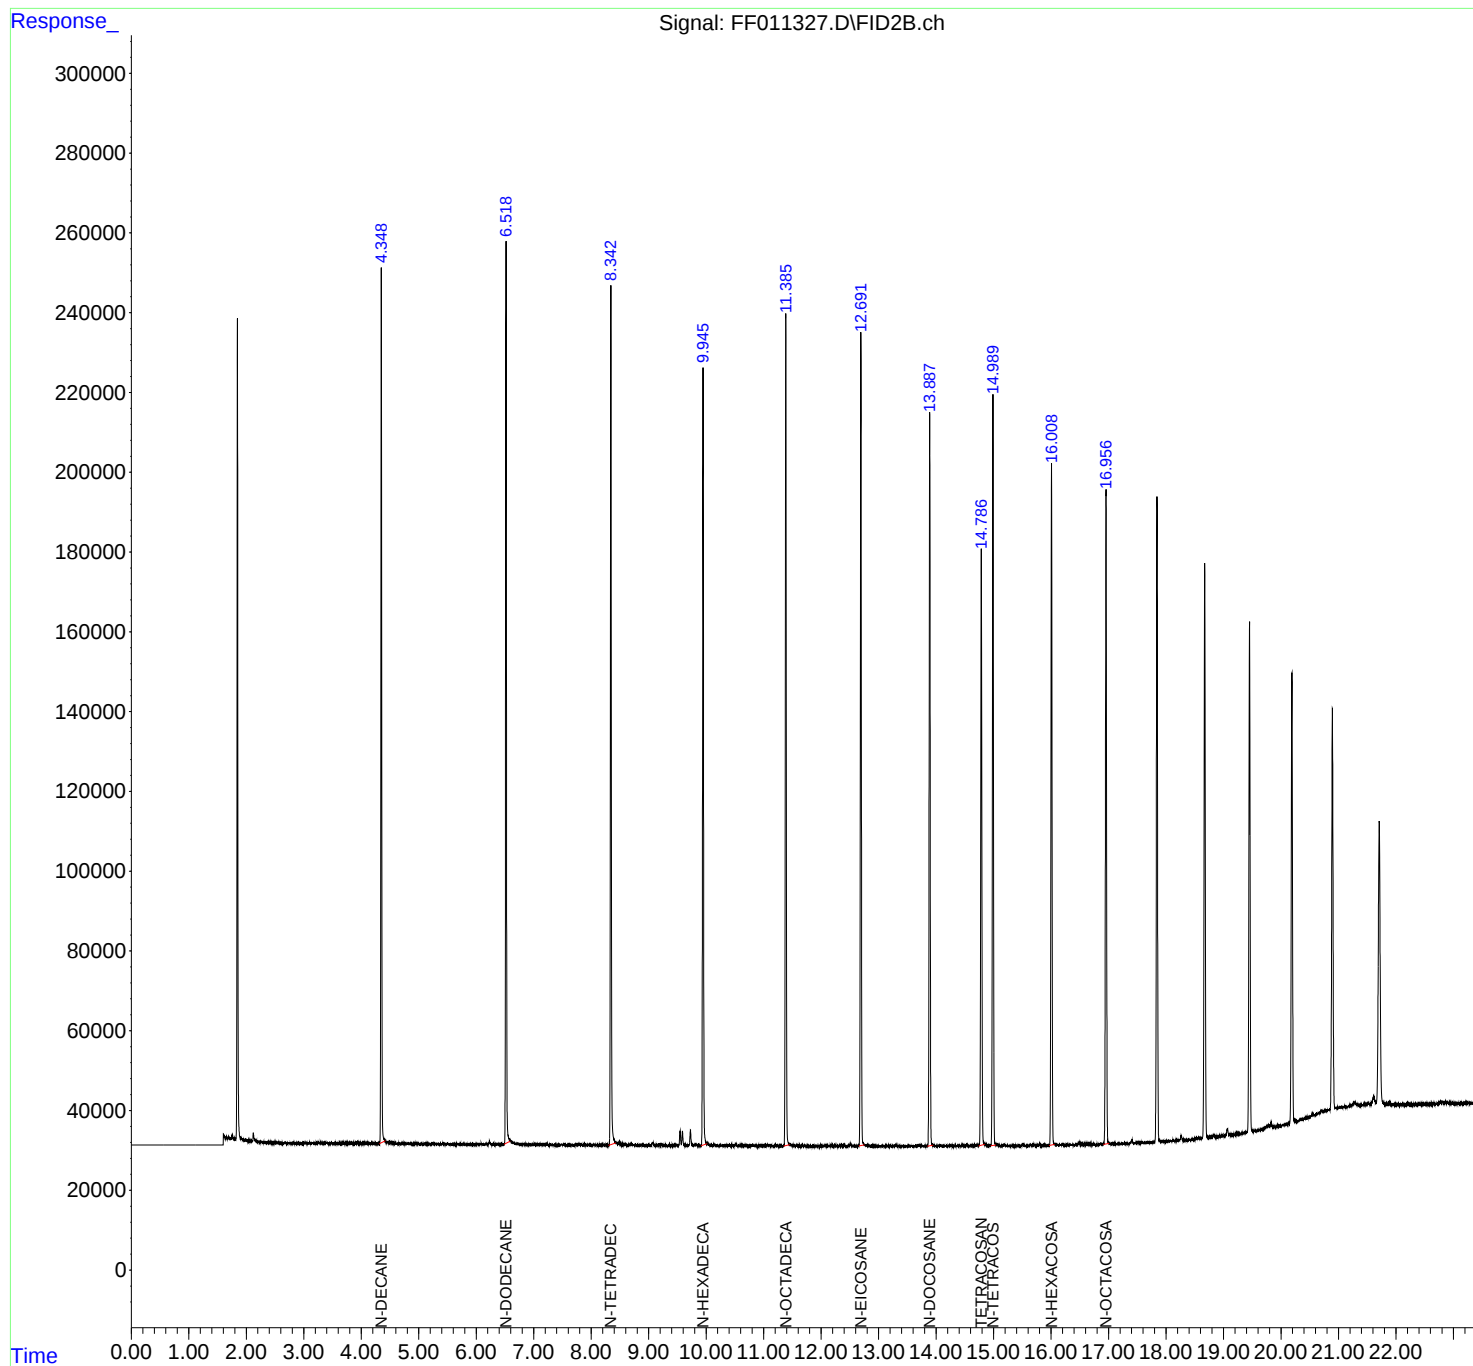


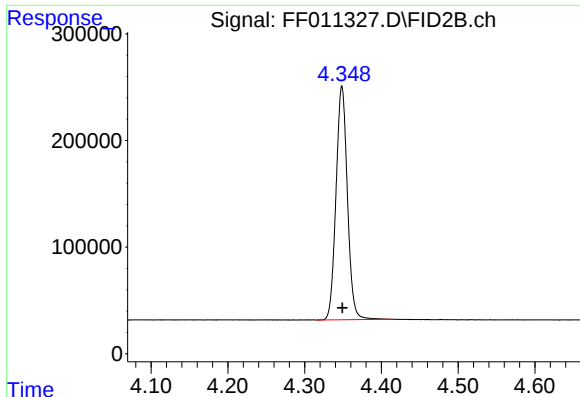

#2 N-DECANE


R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 2258055
Conc: 17.40 ug/ml

Instrument :
FID_F
ClientSampleId :
PB147353BS

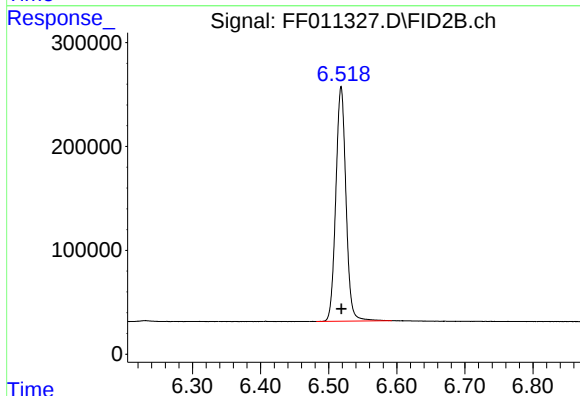


#3 N-DODECANE

R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 2340946
Conc: 17.88 ug/ml

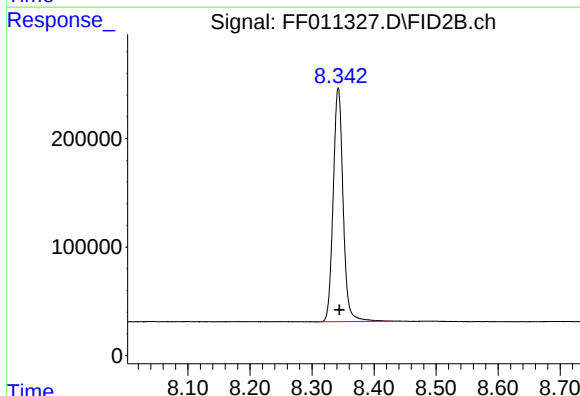


#4 N-TETRADECANE

R.T.: 8.342 min
Delta R.T.: -0.002 min
Response: 2390160
Conc: 18.20 ug/ml

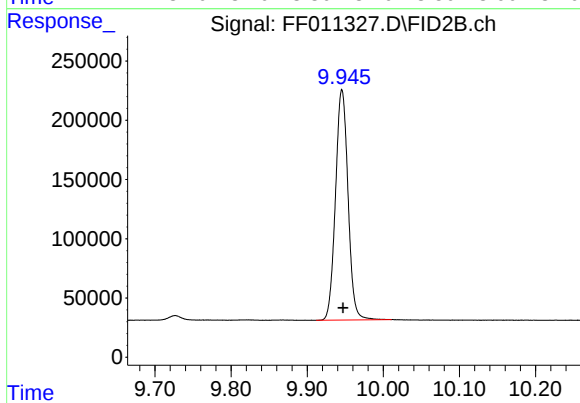

#5 N-HEXADECANE


R.T.: 9.946 min
Delta R.T.: -0.002 min
Response: 2225057
Conc: 16.77 ug/ml

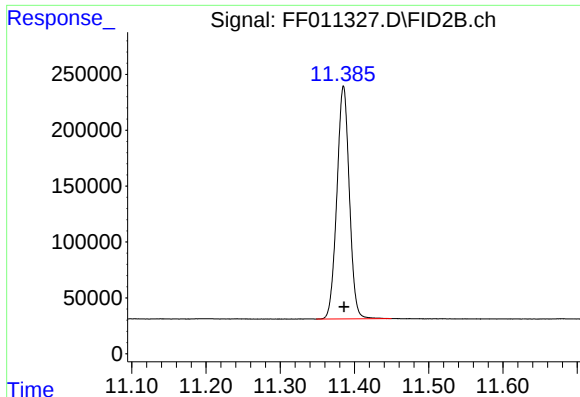

#6 N-OCTADECANE


R.T.: 11.385 min
Delta R.T.: 0.000 min
Response: 2427266
Conc: 18.26 ug/ml

Instrument :
FID_F
ClientSampleId :
PB147353BS

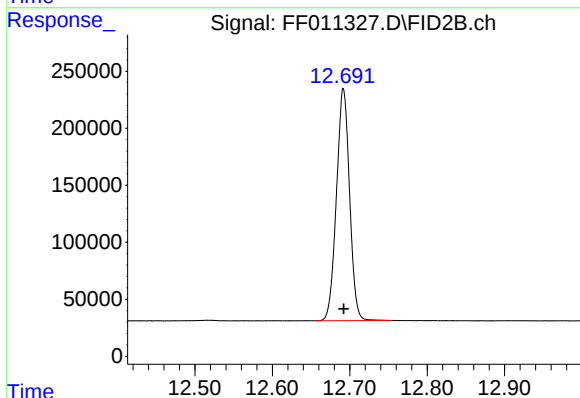


#7 N-EICOSANE

R.T.: 12.692 min
Delta R.T.: 0.000 min
Response: 2398565
Conc: 18.23 ug/ml

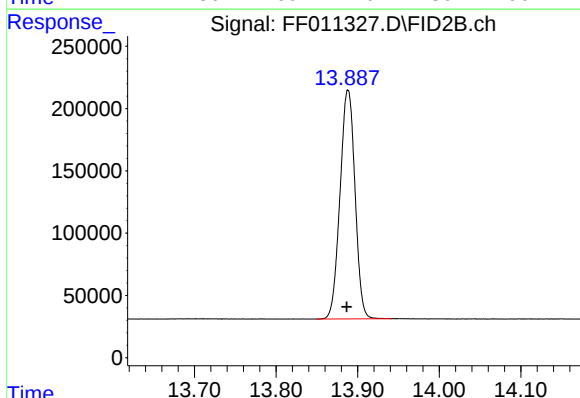


#8 N-DOCOSANE

R.T.: 13.888 min
Delta R.T.: 0.002 min
Response: 2343341
Conc: 18.33 ug/ml

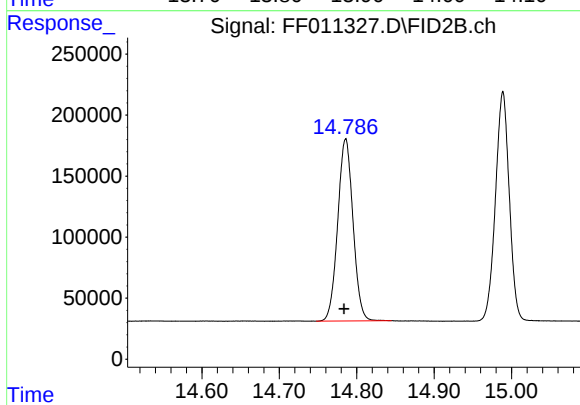

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.786 min
Delta R.T.: 0.002 min
Response: 2047468
Conc: 18.27 ug/ml

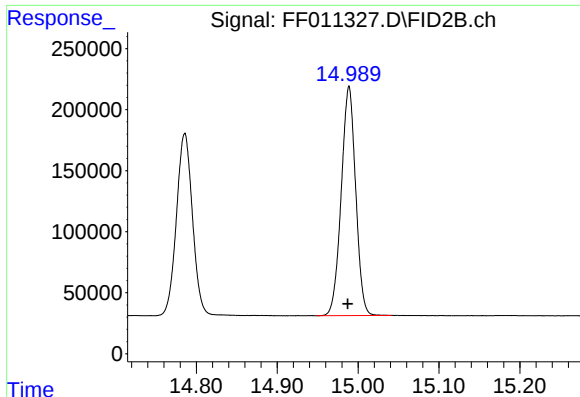

#10 N-TETRACOSANE


R.T.: 14.989 min
Delta R.T.: 0.002 min
Response: 2331049
Conc: 18.31 ug/ml

Instrument :
FID_F
ClientSampleId :
PB147353BS

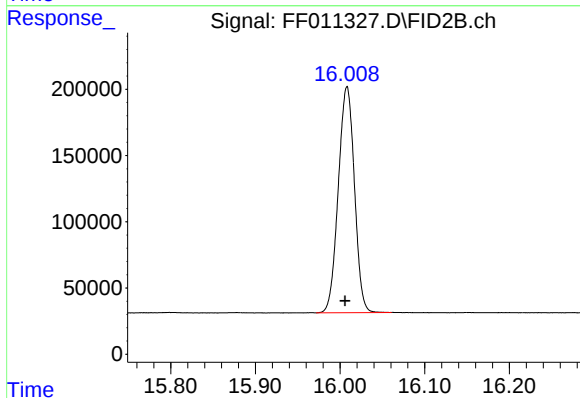

#11 N-HEXACOSANE

R.T.: 16.008 min
Delta R.T.: 0.003 min
Response: 2261823
Conc: 18.11 ug/ml

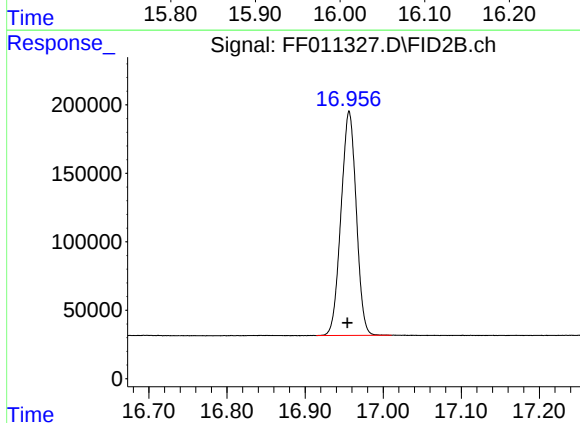

#12 N-OCTACOSANE

R.T.: 16.956 min
Delta R.T.: 0.002 min
Response: 2221129
Conc: 18.13 ug/ml