

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
 Data File : FF011346.D
 Signal(s) : FID2B.ch
 Acq On : 01 Sep 2022 12:00
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 02 02:45:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.786	1931101	17.228 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.842	57834	0.479 ug/ml
14) N-DOTRIACONTANE	18.672	82934	0.701 ug/ml
15) N-TETRATRIACONTANE	19.454	69941	0.613 ug/ml
16) N-HEXATRIACONTANE	20.191	46807	0.440 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
Data File : FF011346.D
Signal(s) : FID2B.ch
Acq On : 01 Sep 2022 12:00
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 02:45:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

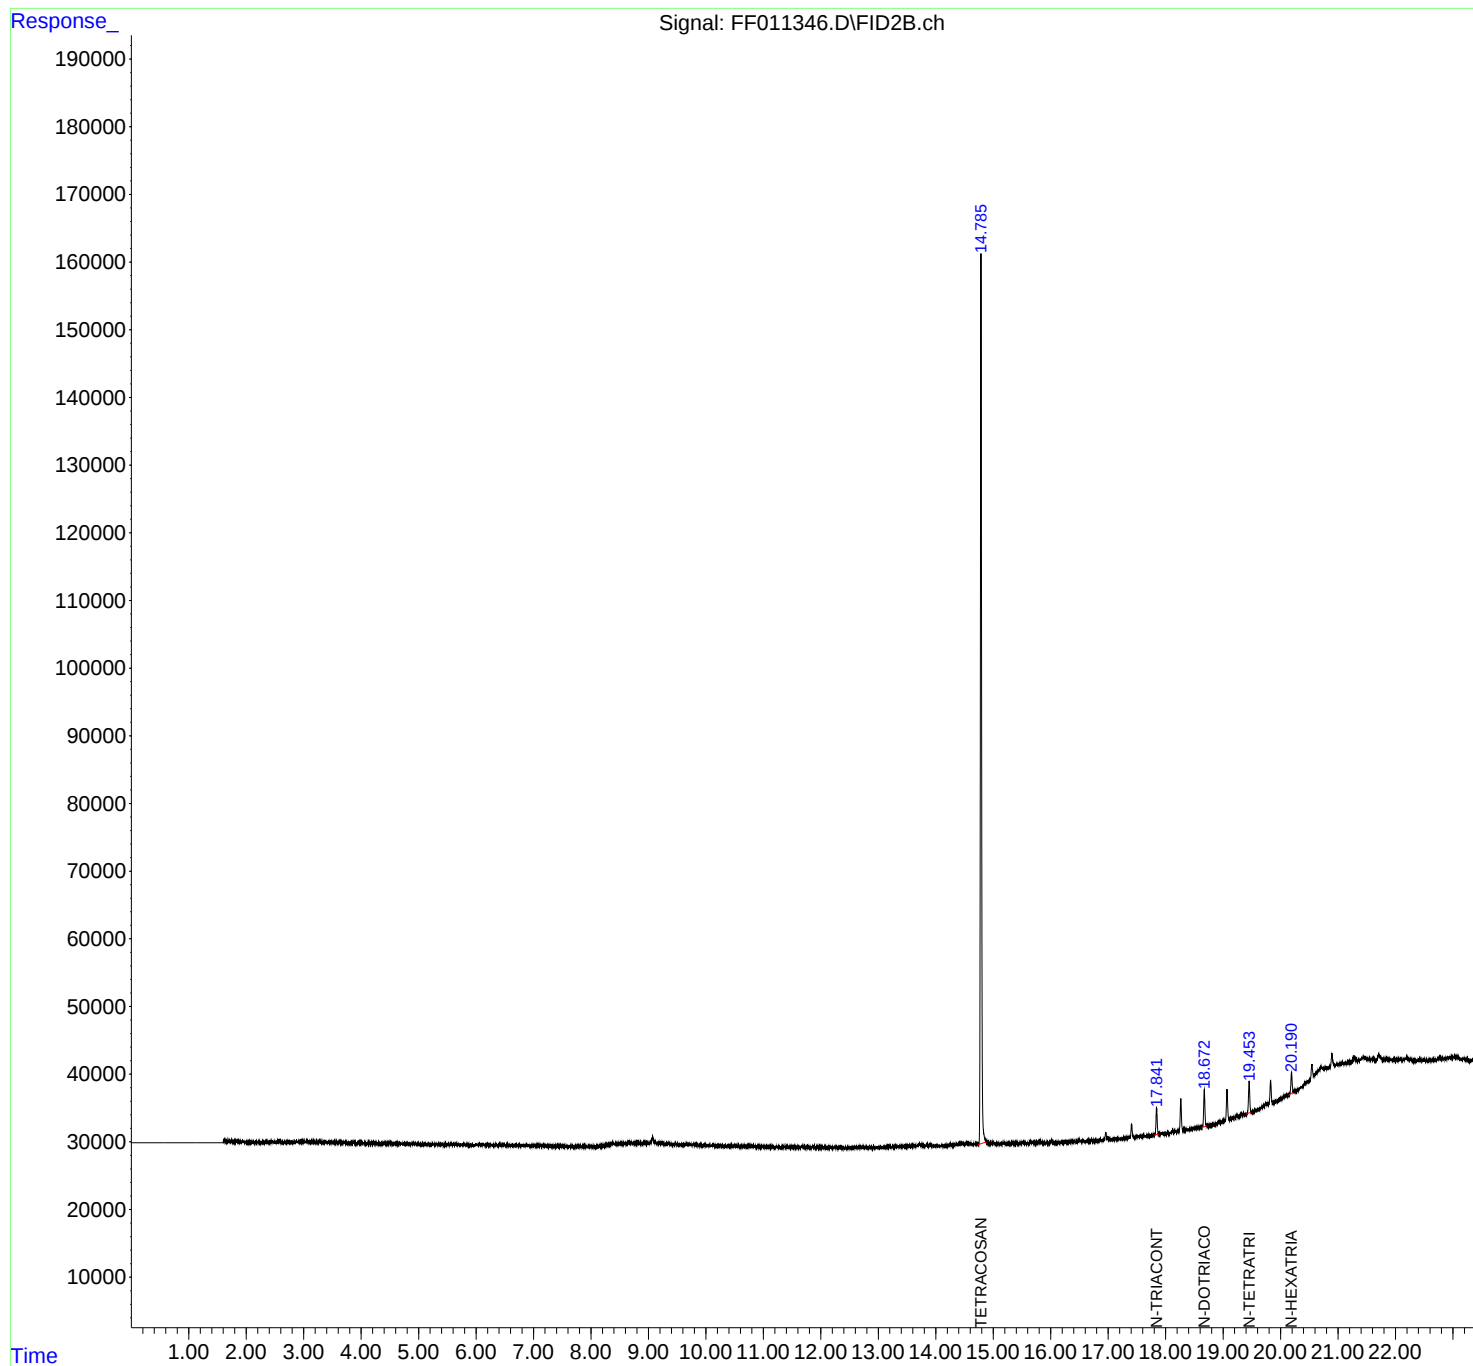


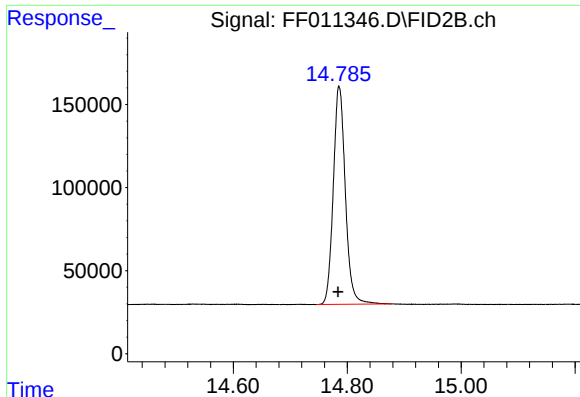

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.786 min
Delta R.T.: 0.002 min
Response: 1931101
Conc: 17.23 ug/ml

Instrument :
FID_F
ClientSampleId :

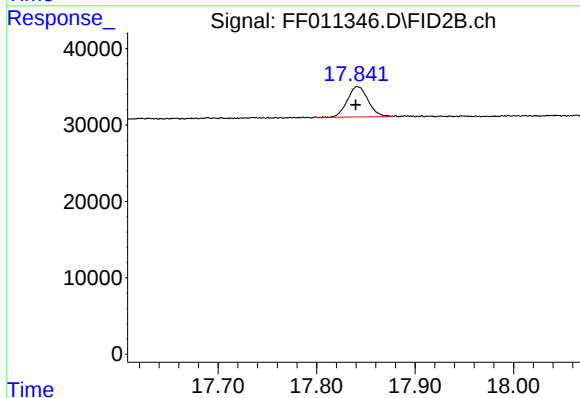


#13 N-TRIACONTANE

R.T.: 17.842 min
Delta R.T.: 0.002 min
Response: 57834
Conc: 0.48 ug/ml

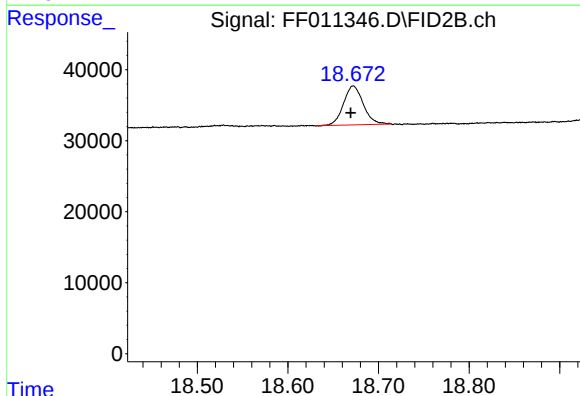


#14 N-DOTRIACONTANE

R.T.: 18.672 min
Delta R.T.: 0.003 min
Response: 82934
Conc: 0.70 ug/ml

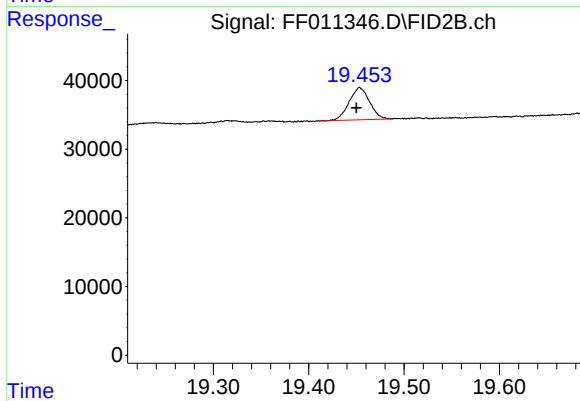

#15 N-TETRATRIACONTANE

R.T.: 19.454 min
Delta R.T.: 0.004 min
Response: 69941
Conc: 0.61 ug/ml

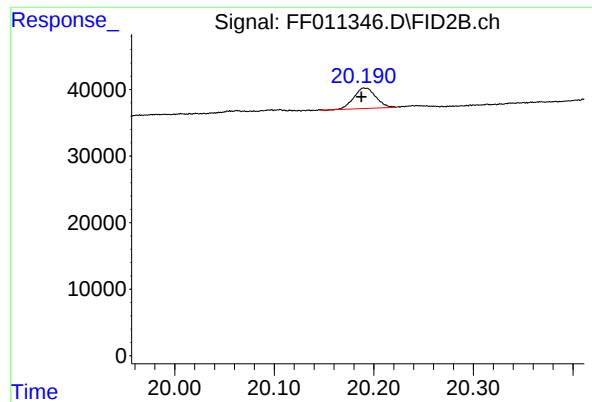

#16 N-HEXATRIACONTANE

R.T.: 20.191 min
Delta R.T.: 0.003 min
Response: 46807
Conc: 0.44 ug/ml

Instrument :

FID_F

ClientSampleId :