

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
 Data File : FF011348.D
 Signal(s) : FID2B.ch
 Acq On : 01 Sep 2022 12:59
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 02 02:45:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
3) N-DODECANE	6.518	2645512	20.202	ug/ml
12) N-OCTACOSANE	16.956	2627750	21.453	ug/ml
13) N-TRIACONTANE	17.841	130171	1.079	ug/ml
14) N-DOTRIACONTANE	18.671	192077	1.624	ug/ml
15) N-TETRATRIACONTANE	19.452	188933	1.655	ug/ml
16) N-HEXATRIACONTANE	20.189	141289	1.327	ug/ml
17) N-OCTATRIACONTANE	20.894	101928	0.980	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
Data File : FF011348.D
Signal(s) : FID2B.ch
Acq On : 01 Sep 2022 12:59
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 02:45:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

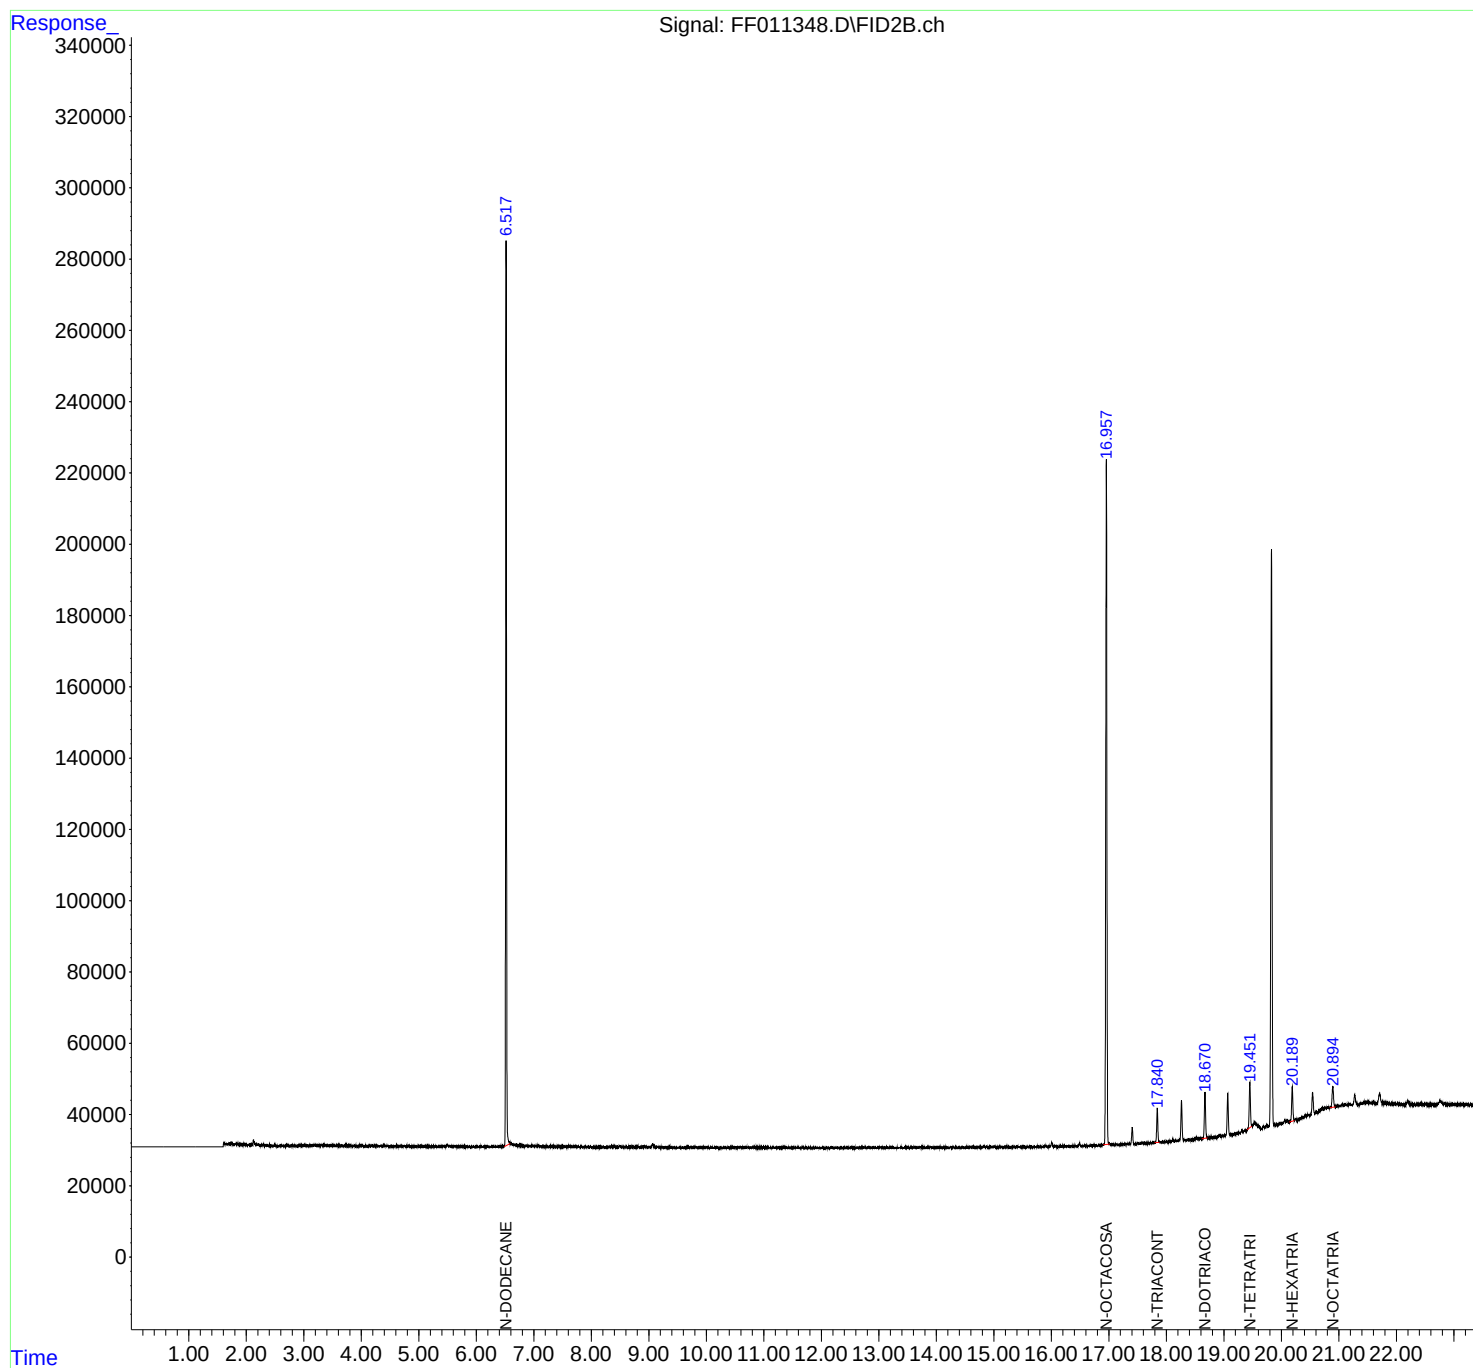


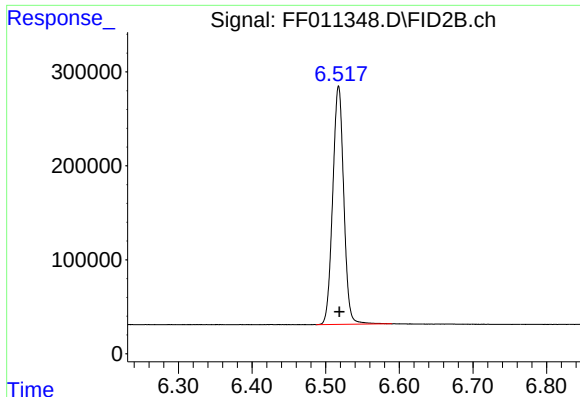

#3 N-DODECANE


R.T.: 6.518 min
Delta R.T.: -0.001 min
Response: 2645512
Conc: 20.20 ug/ml

Instrument :
FID_F
ClientSampleId :

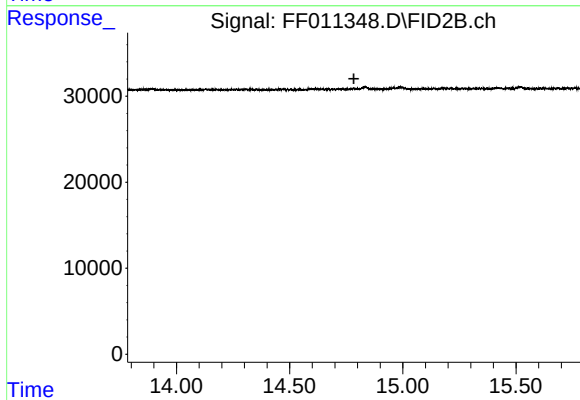


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

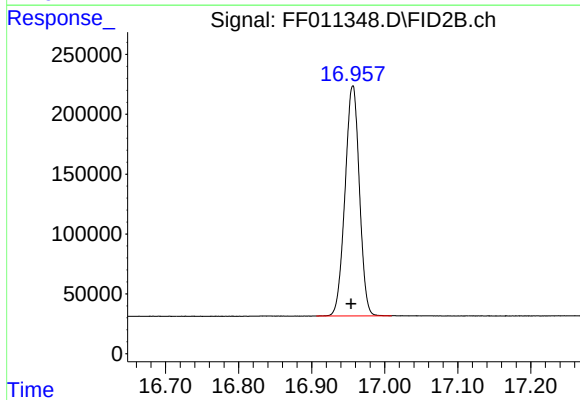


#12 N-OCTACOSANE

R.T.: 16.956 min
Delta R.T.: 0.002 min
Response: 2627750
Conc: 21.45 ug/ml

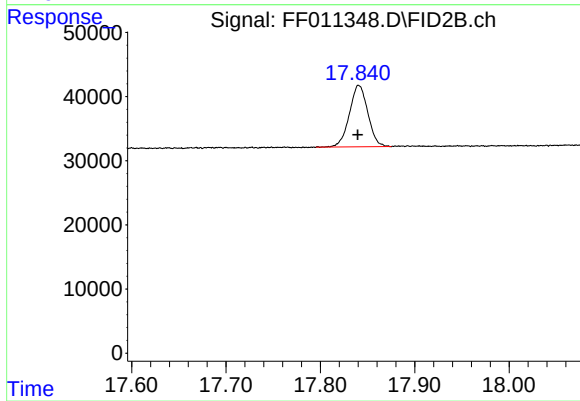

#13 N-TRIACONTANE


R.T.: 17.841 min
Delta R.T.: 0.000 min
Response: 130171
Conc: 1.08 ug/ml

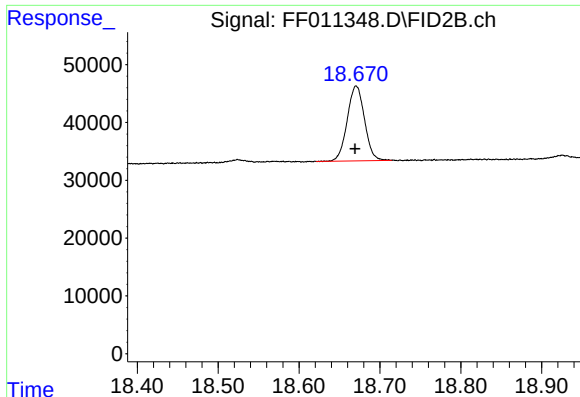

#14 N-DOTRIACONTANE


R.T.: 18.671 min
Delta R.T.: 0.001 min
Response: 192077
Conc: 1.62 ug/ml

Instrument :
FID_F
ClientSampleId :

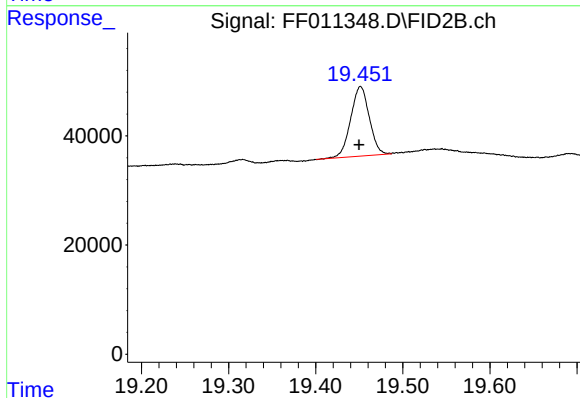


#15 N-TETRATRIACONTANE

R.T.: 19.452 min
Delta R.T.: 0.002 min
Response: 188933
Conc: 1.66 ug/ml

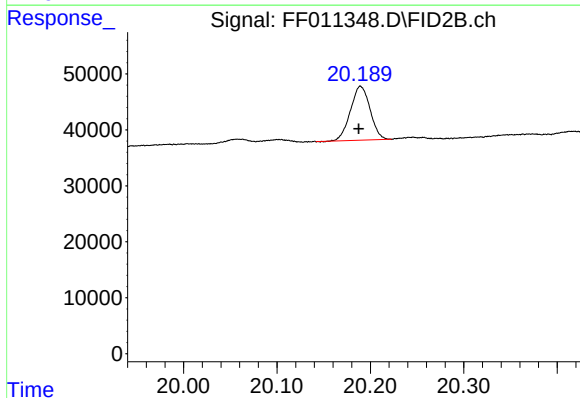

#16 N-HEXATRIACONTANE

R.T.: 20.189 min
Delta R.T.: 0.002 min
Response: 141289
Conc: 1.33 ug/ml

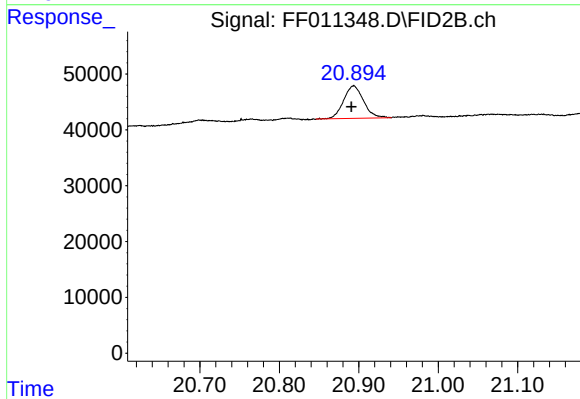

#17 N-OCTATRIACONTANE

R.T.: 20.894 min
Delta R.T.: 0.003 min
Response: 101928
Conc: 0.98 ug/ml