

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
 Data File : FF011352.D
 Signal(s) : FID2B.ch
 Acq On : 01 Sep 2022 15:55
 Operator : YP\AJ
 Sample : N4455-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 02 02:46:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	814708	7.268 ug/ml
Target Compounds			
4) N-TETRADECANE	8.392	544340	4.144 ug/ml
5) N-HEXADECANE	9.933	598765	4.514 ug/ml
7) N-EICOSANE	12.748f	107472	0.817 ug/ml
11) N-HEXACOSANE	16.006	92723	0.742 ug/ml
12) N-OCTACOSANE	16.954	289129	2.360 ug/ml
13) N-TRIACONTANE	17.839	382820	3.173 ug/ml
14) N-DOTRIACONTANE	18.669	555501	4.696 ug/ml
15) N-TETRATRIACONTANE	19.390f	83499	0.731 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
Data File : FF011352.D
Signal(s) : FID2B.ch
Acq On : 01 Sep 2022 15:55
Operator : YP\AJ
Sample : N4455-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 02:46:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

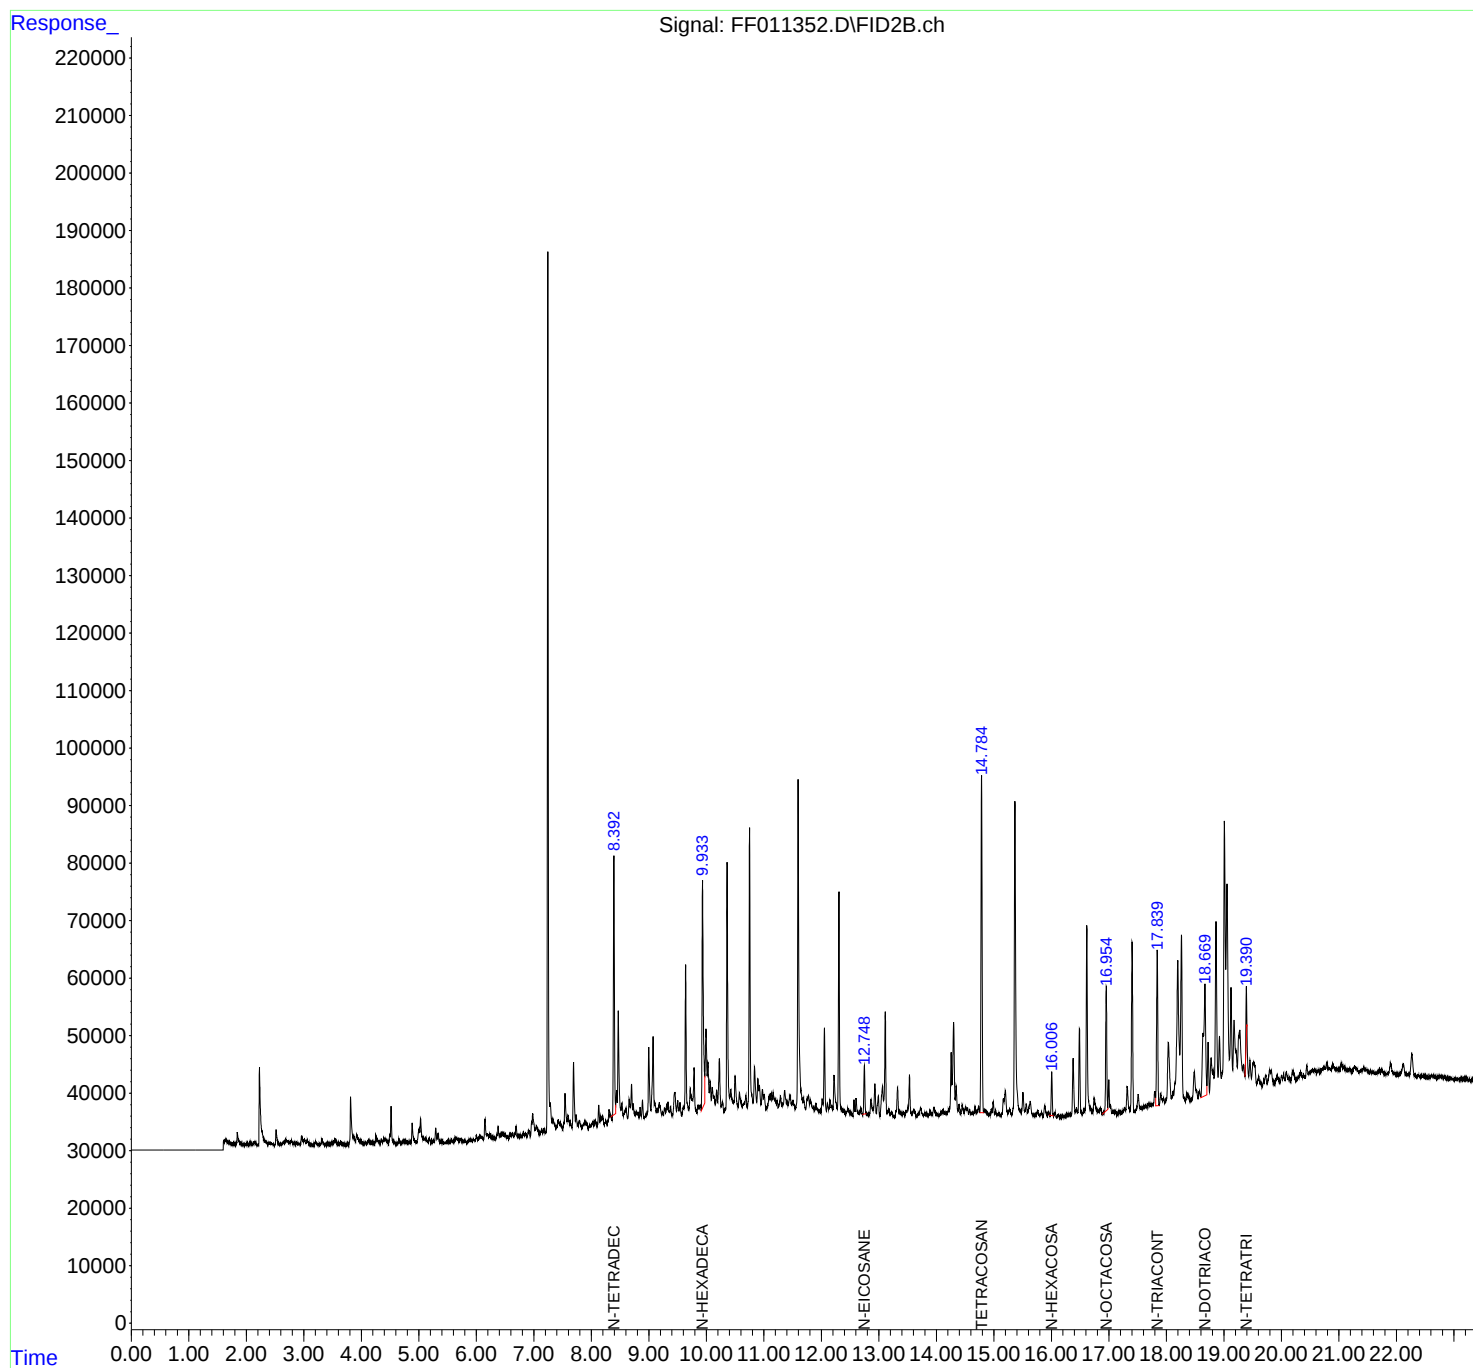


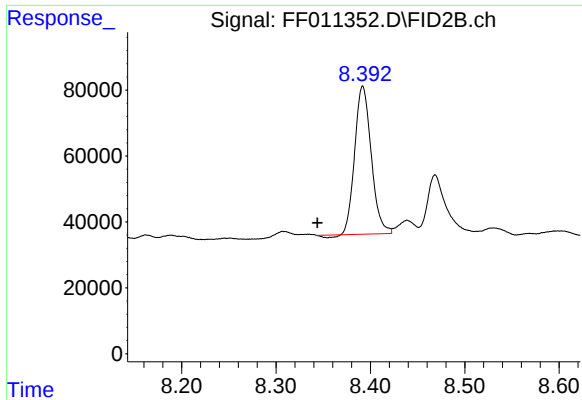

#4 N-TETRADECANE


R.T.: 8.392 min
Delta R.T.: 0.048 min
Response: 544340
Conc: 4.14 ug/ml

Instrument :
FID_F
ClientSampleId :

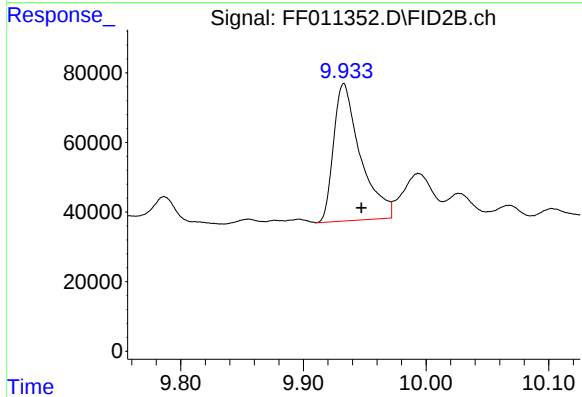


#5 N-HEXADECANE

R.T.: 9.933 min
Delta R.T.: -0.014 min
Response: 598765
Conc: 4.51 ug/ml

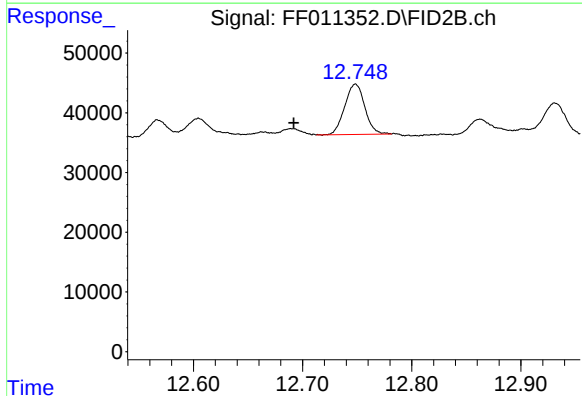


#7 N-EICOSANE

R.T.: 12.748 min
Delta R.T.: 0.056 min
Response: 107472
Conc: 0.82 ug/ml

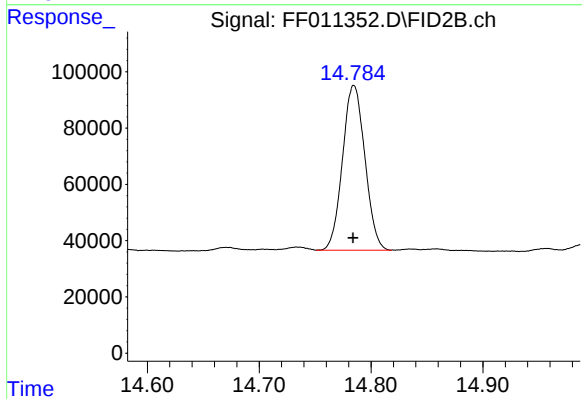

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.785 min
Delta R.T.: 0.000 min
Response: 814708
Conc: 7.27 ug/ml

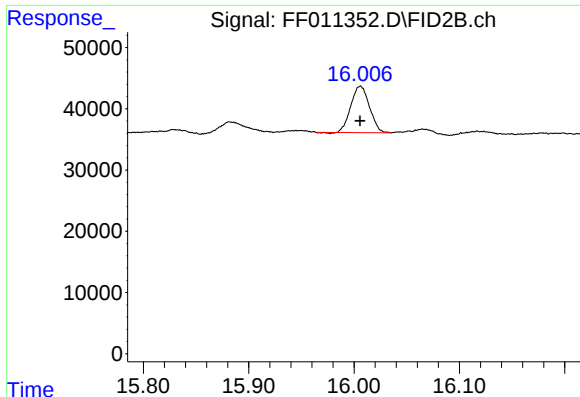

#11 N-HEXACOSANE


R.T.: 16.006 min
Delta R.T.: 0.000 min
Response: 92723
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

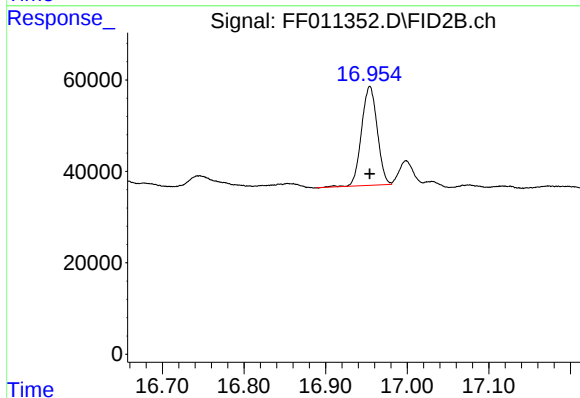


#12 N-OCTACOSANE

R.T.: 16.954 min
Delta R.T.: 0.000 min
Response: 289129
Conc: 2.36 ug/ml

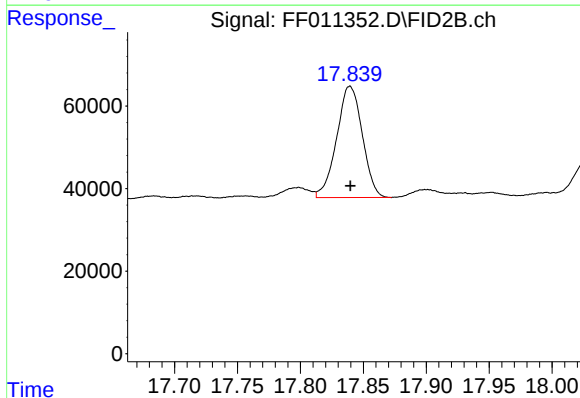


#13 N-TRIACONTANE

R.T.: 17.839 min
Delta R.T.: 0.000 min
Response: 382820
Conc: 3.17 ug/ml

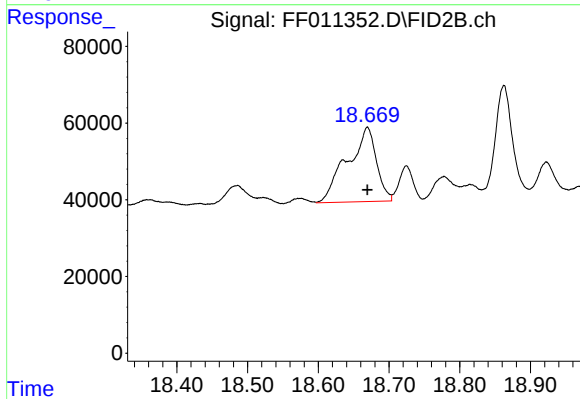

#14 N-DOTRIACONTANE

R.T.: 18.669 min
Delta R.T.: 0.000 min
Response: 555501
Conc: 4.70 ug/ml

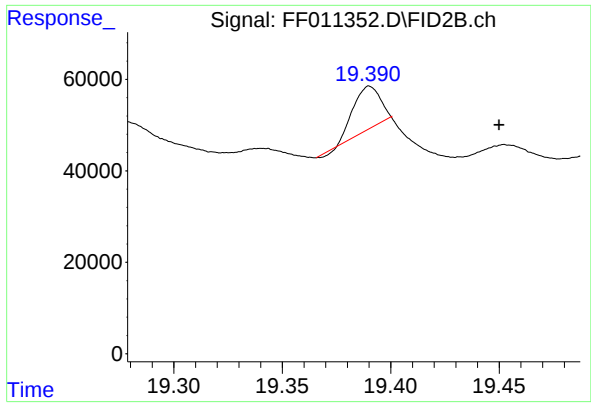

#15 N-TETRATRIACONTANE

R.T.: 19.390 min
Delta R.T.: -0.060 min
Response: 83499
Conc: 0.73 ug/ml

Instrument :
FID_F
ClientSampleId :