

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
 Data File : FF011354.D
 Signal(s) : FID2B.ch
 Acq On : 01 Sep 2022 16:55
 Operator : YP\AJ
 Sample : N4455-01RE
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 02 02:47:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.784	820550	7.321 ug/ml
Target Compounds			
4) N-TETRADECANE	8.393	567064	4.317 ug/ml
5) N-HEXADECANE	9.933	712507	5.372 ug/ml
7) N-EICOSANE	12.748f	120969	0.920 ug/ml
11) N-HEXACOSANE	16.007	96802	0.775 ug/ml
12) N-OCTACOSANE	16.954	295896	2.416 ug/ml
13) N-TRIACONTANE	17.839	362737	3.007 ug/ml
14) N-DOTRIACONTANE	18.670	664817	5.620 ug/ml
15) N-TETRATRIACONTANE	19.395f	60767	0.532 ug/ml
16) N-HEXATRIACONTANE	20.197	120770	1.135 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
Data File : FF011354.D
Signal(s) : FID2B.ch
Acq On : 01 Sep 2022 16:55
Operator : YP\AJ
Sample : N4455-01RE
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 02:47:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

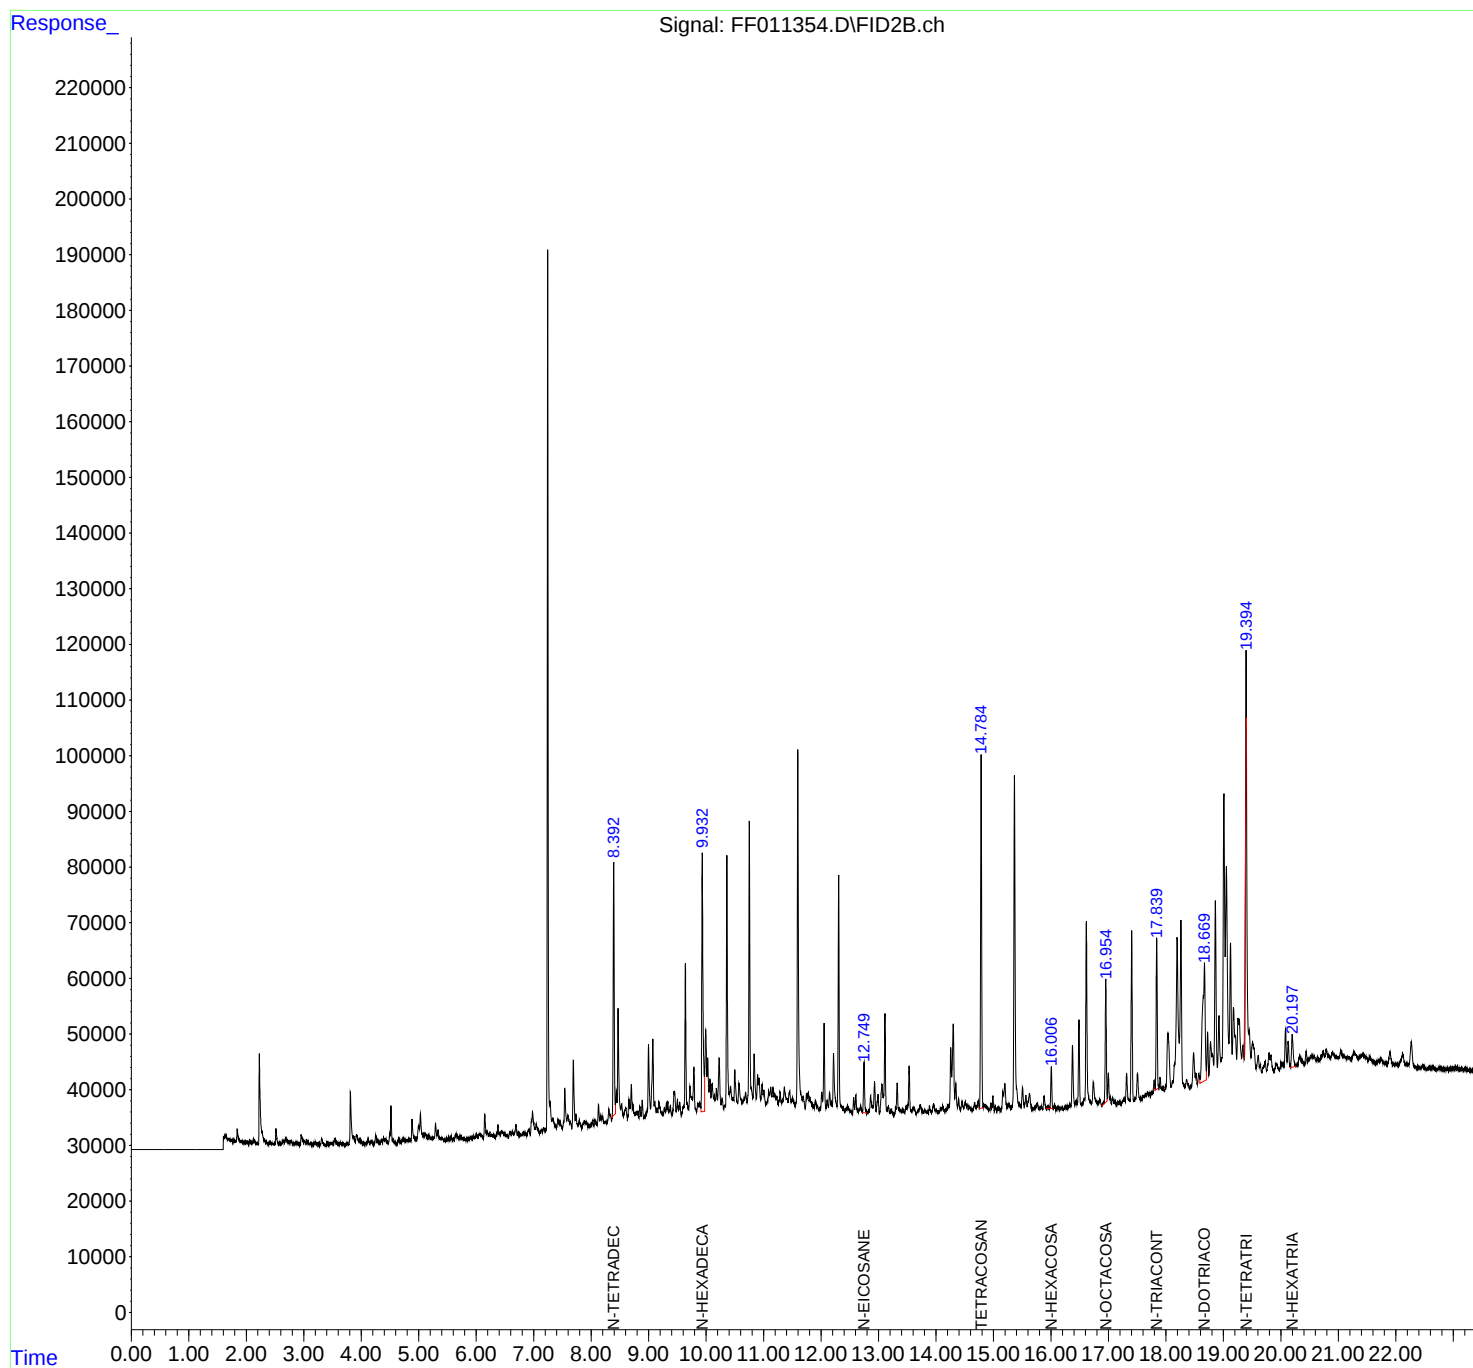


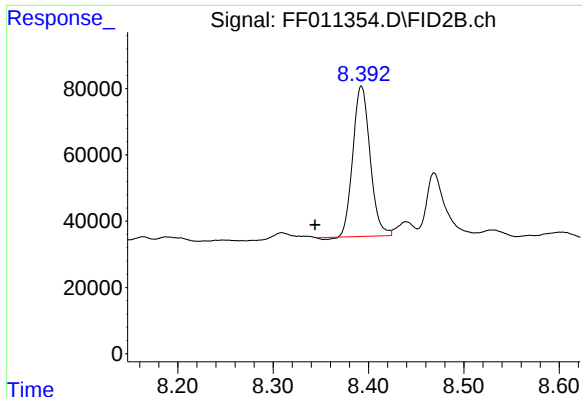

#4 N-TETRADECANE


R.T.: 8.393 min
Delta R.T.: 0.049 min
Response: 567064
Conc: 4.32 ug/ml

Instrument :
FID_F
ClientSampleId :

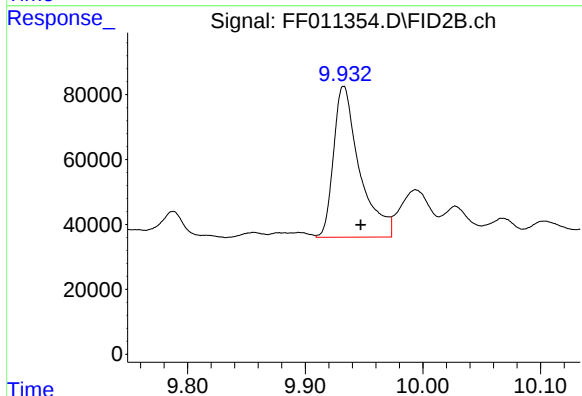


#5 N-HEXADECANE

R.T.: 9.933 min
Delta R.T.: -0.015 min
Response: 712507
Conc: 5.37 ug/ml

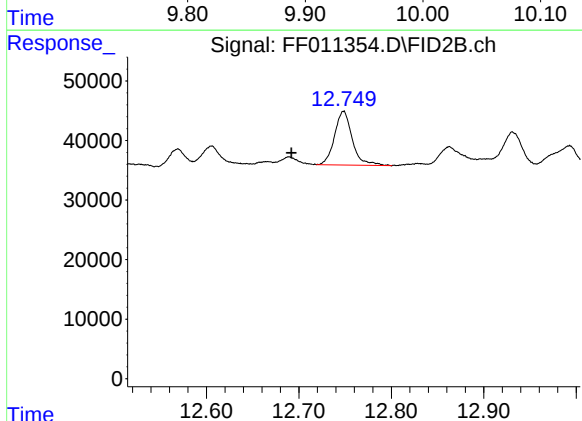


#7 N-EICOSANE

R.T.: 12.748 min
Delta R.T.: 0.056 min
Response: 120969
Conc: 0.92 ug/ml

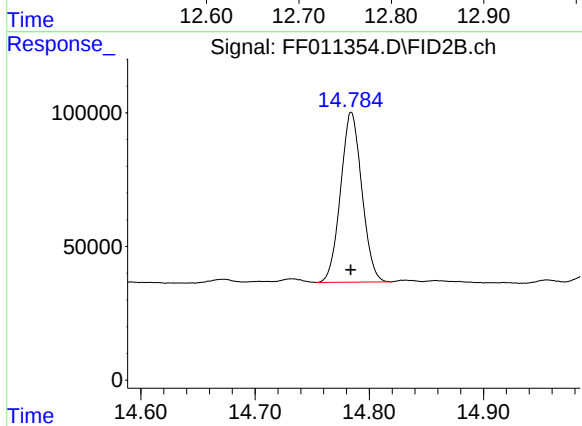

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.784 min
Delta R.T.: 0.000 min
Response: 820550
Conc: 7.32 ug/ml

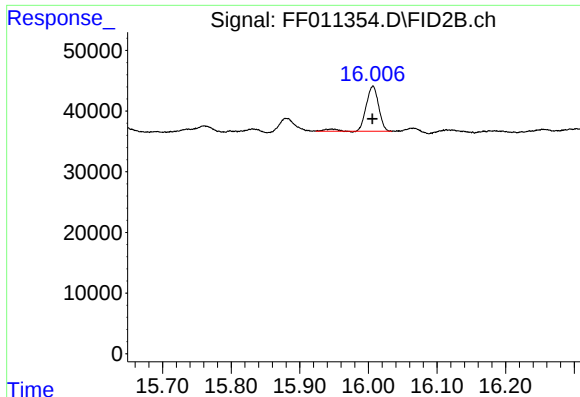

#11 N-HEXACOSANE


R.T.: 16.007 min
Delta R.T.: 0.000 min
Response: 96802
Conc: 0.78 ug/ml

Instrument :
FID_F
ClientSampleId :

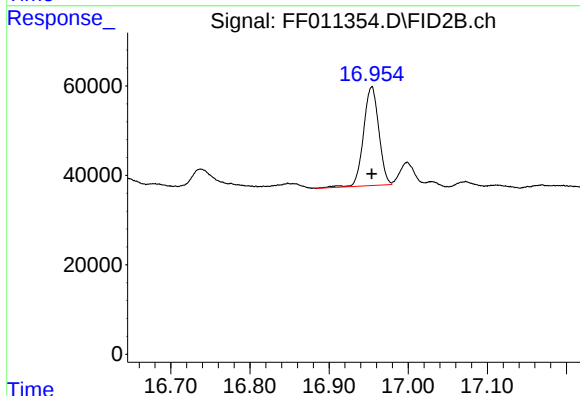


#12 N-OCTACOSANE

R.T.: 16.954 min
Delta R.T.: 0.000 min
Response: 295896
Conc: 2.42 ug/ml

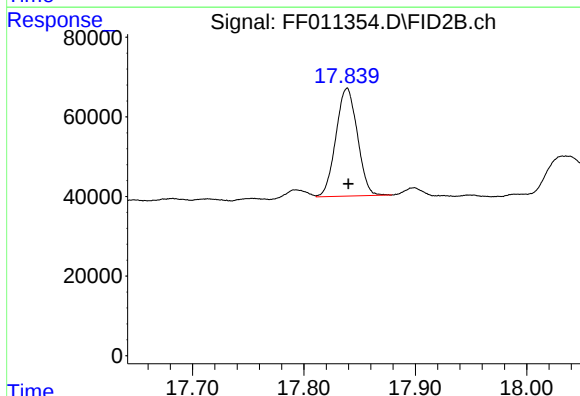


#13 N-TRIACONTANE

R.T.: 17.839 min
Delta R.T.: -0.001 min
Response: 362737
Conc: 3.01 ug/ml

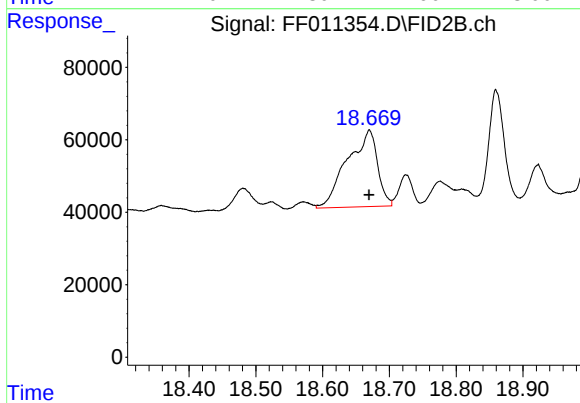

#14 N-DOTRIACONTANE


R.T.: 18.670 min
Delta R.T.: 0.000 min
Response: 664817
Conc: 5.62 ug/ml

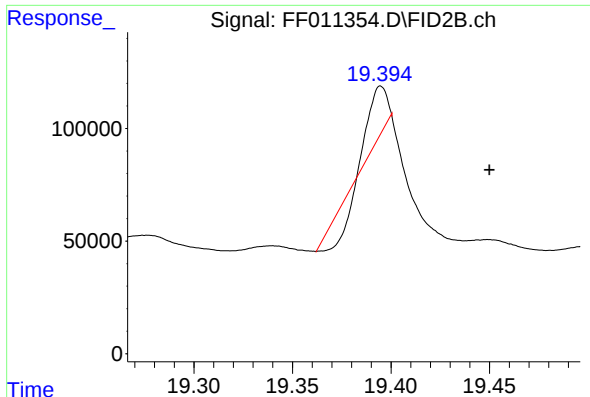

#15 N-TETRATRIACONTANE

R.T.: 19.395 min
Delta R.T.: -0.055 min
Response: 60767
Conc: 0.53 ug/ml

Instrument :
FID_F
ClientSampleId :

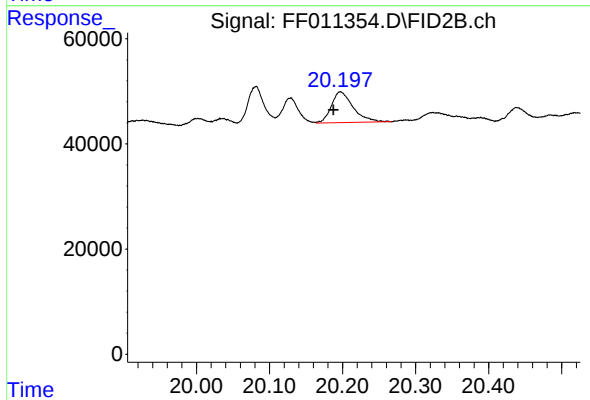

#16 N-HEXATRIACONTANE

R.T.: 20.197 min
Delta R.T.: 0.010 min
Response: 120770
Conc: 1.13 ug/ml