

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
 Data File : FF011355.D
 Signal(s) : FID2B.ch
 Acq On : 01 Sep 2022 17:25
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 02 02:47:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.787	2022255	18.042 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.841	75219	0.623 ug/ml
14) N-DOTRIACONTANE	18.670	113685	0.961 ug/ml
15) N-TETRATRIACONTANE	19.452	88247	0.773 ug/ml
16) N-HEXATRIACONTANE	20.190	60199	0.566 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
Data File : FF011355.D
Signal(s) : FID2B.ch
Acq On : 01 Sep 2022 17:25
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 02:47:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

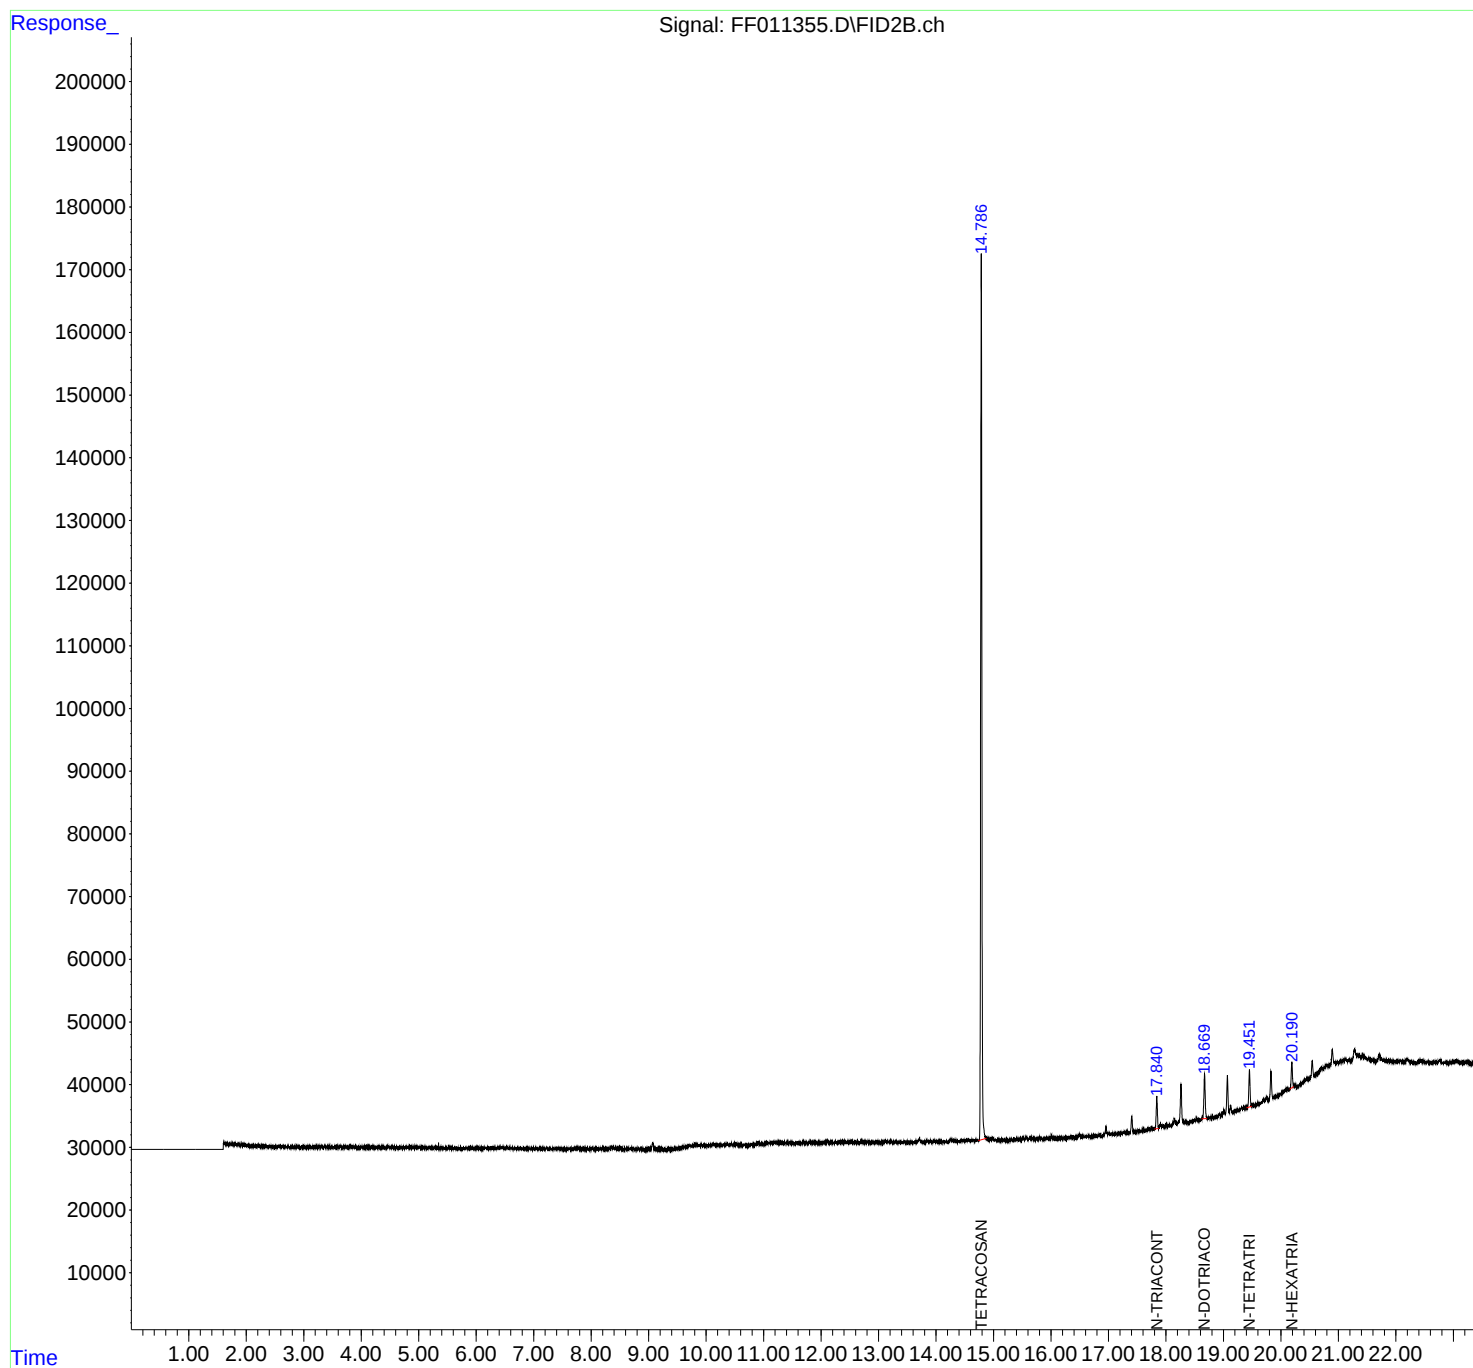


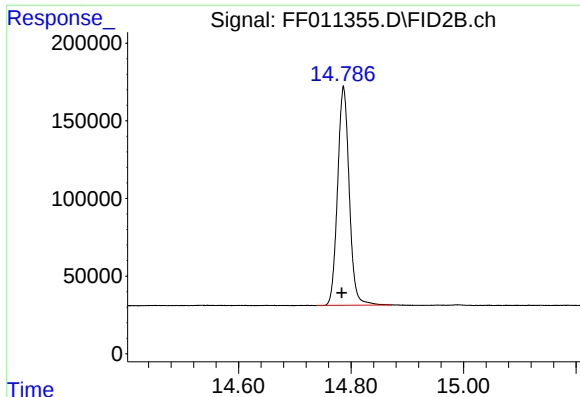

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.787 min
Delta R.T.: 0.003 min
Response: 2022255
Conc: 18.04 ug/ml

Instrument :
FID_F
ClientSampleId :

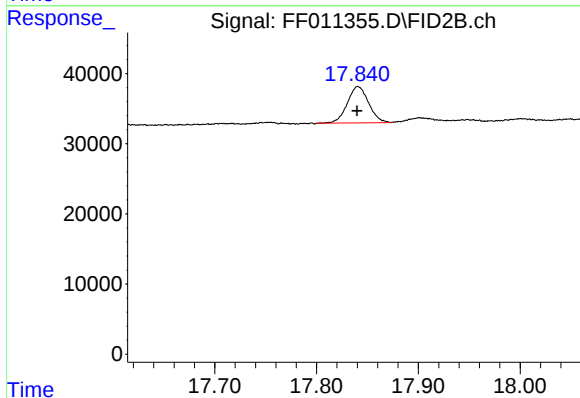


#13 N-TRIACONTANE

R.T.: 17.841 min
Delta R.T.: 0.000 min
Response: 75219
Conc: 0.62 ug/ml

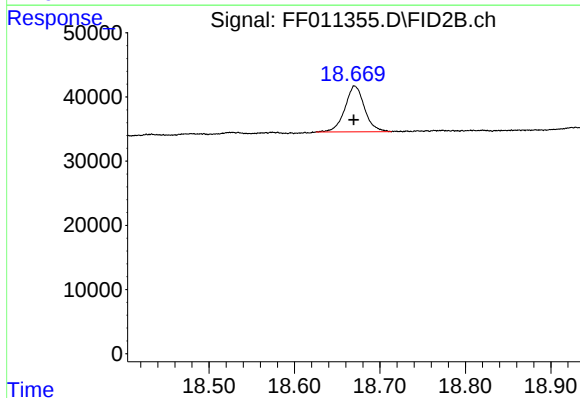


#14 N-DOTRIACONTANE

R.T.: 18.670 min
Delta R.T.: 0.001 min
Response: 113685
Conc: 0.96 ug/ml

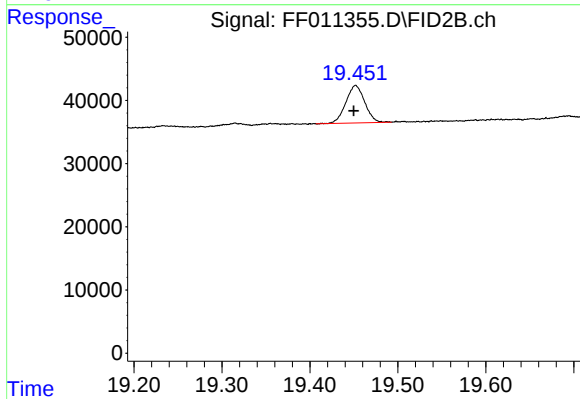

#15 N-TETRATRIACONTANE

R.T.: 19.452 min
Delta R.T.: 0.002 min
Response: 88247
Conc: 0.77 ug/ml

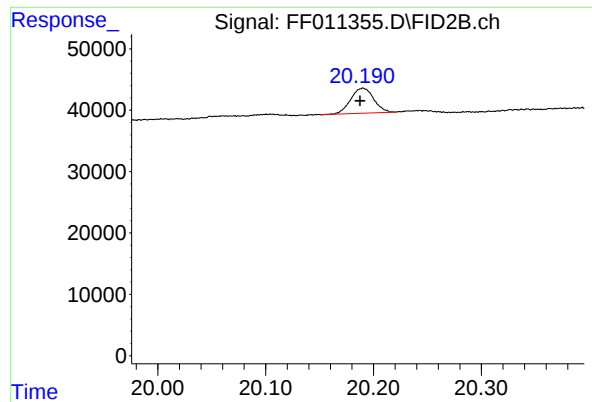

#16 N-HEXATRIACONTANE

R.T.: 20.190 min
Delta R.T.: 0.003 min
Response: 60199
Conc: 0.57 ug/ml

Instrument :

FID_F

ClientSampleId :