

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
Data File : FF011354.D
Signal(s) : FID2B.ch
Acq On : 01 Sep 2022 16:55
Operator : YP\AJ
Sample : N4455-01RE
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS2-WC-L-MH-02RE

Integration File: autoint1.e
Quant Time: Sep 02 02:47:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.784	820550	7.321 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090122\
Data File : FF011354.D
Signal(s) : FID2B.ch
Acq On : 01 Sep 2022 16:55
Operator : YP\AJ
Sample : N4455-01RE
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS2-WC-L-MH-02RE

Integration File: autoint1.e
Quant Time: Sep 02 02:47:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

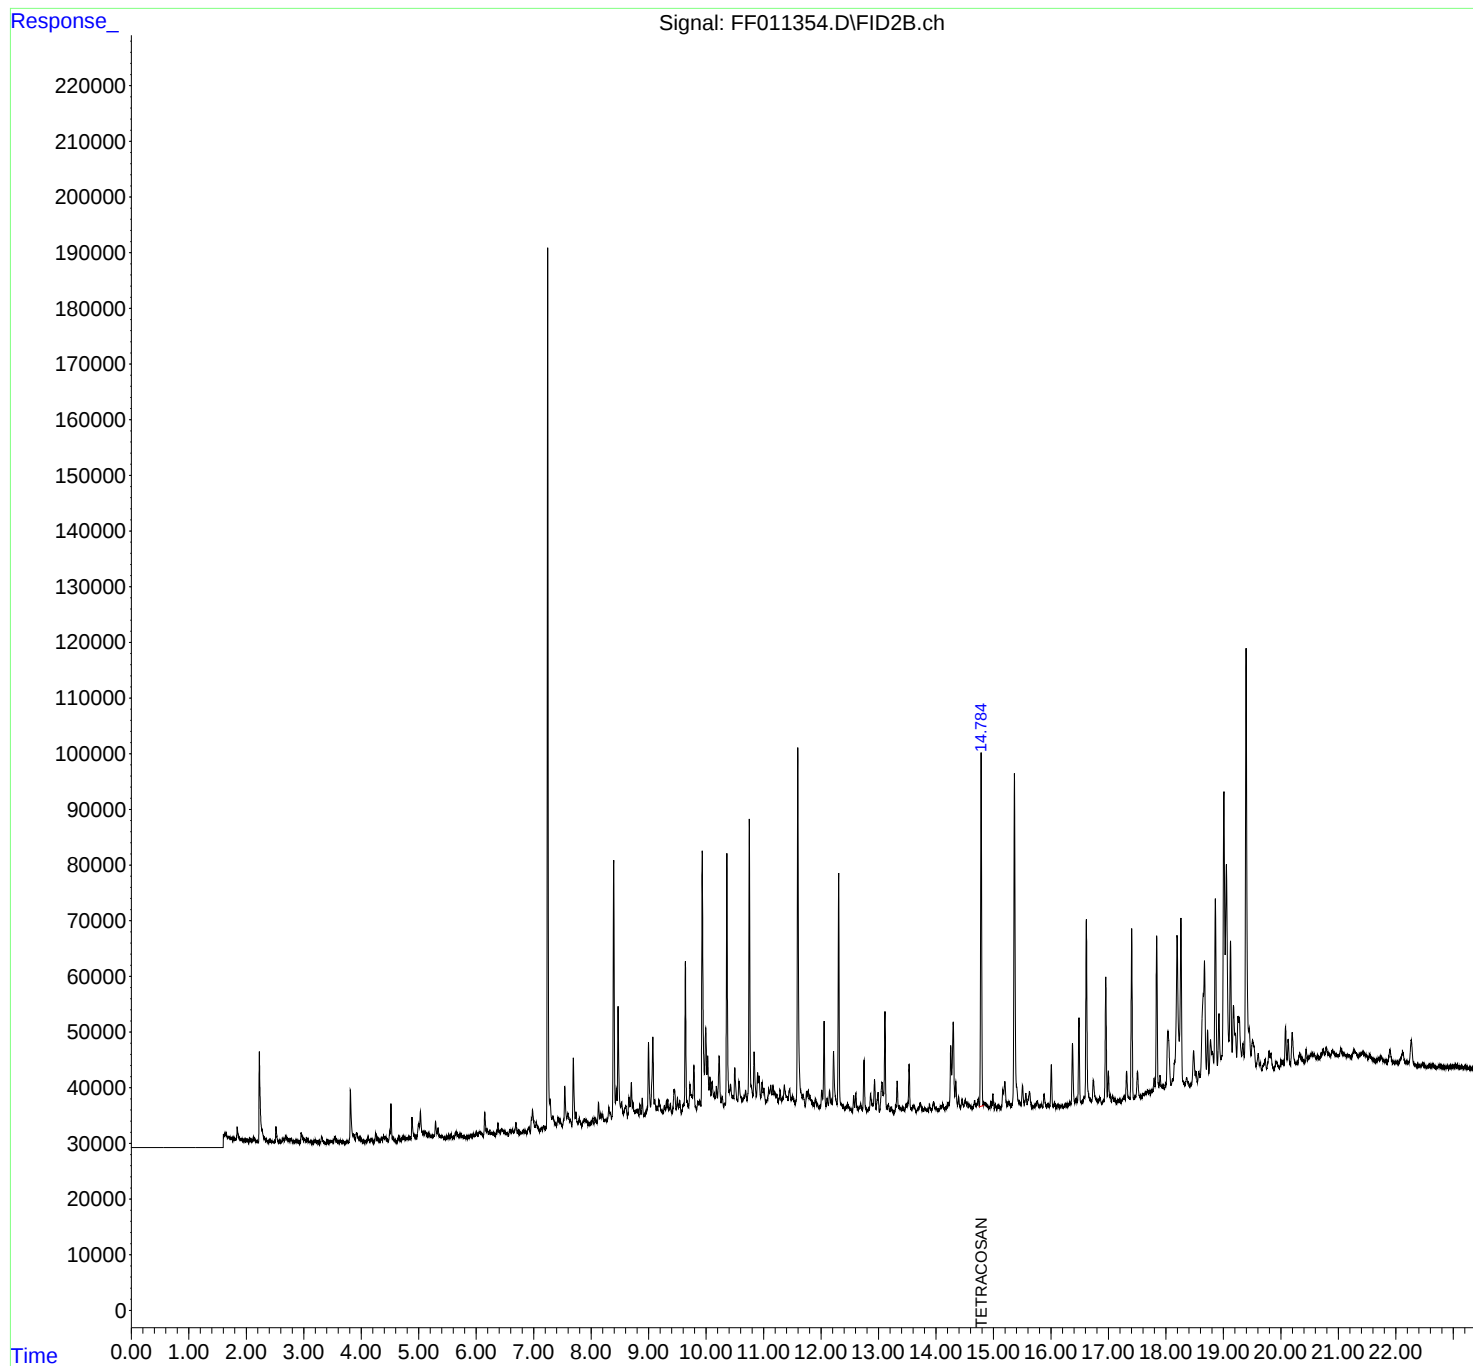

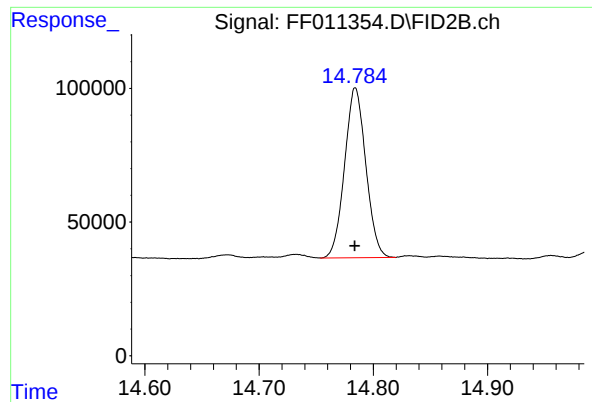

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.784 min
Delta R.T.: 0.000 min
Response: 820550
Conc: 7.32 ug/ml

Instrument :
FID_F
ClientSampleId :
KTS2-WC-L-MH-02RE