

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090220\
 Data File : FF007445.D
 Signal(s) : FID2B.ch
 Acq On : 02 Sep 2020 14:37
 Operator : DD\AJ
 Sample : L3858-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 03 02:03:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.767	41678370	283.382 ug/ml
Target Compounds			
2) N-DECANE	4.450	299966	1.881 ug/ml
3) N-DODECANE	6.477	1578307	9.702 ug/ml
4) N-TETRADECANE	8.277	1867892	11.351 ug/ml
5) N-HEXADECANE	9.882	1648152	9.766 ug/ml
6) N-OCTADECANE	11.330	3535490	20.748 ug/ml
7) N-EICOSANE	12.674	27771935	165.184 ug/ml
8) N-DOCOSANE	13.824	23756372	144.188 ug/ml
10) N-TETRACOSANE	14.959	14836204	90.965 ug/ml
11) N-HEXACOSANE	15.977	5837456	36.927 ug/ml
12) N-OCTACOSANE	16.927	16735674	109.051 ug/ml
13) N-TRIACONTANE	17.809	10214543	69.110 ug/ml
15) N-TETRATRIACONTANE	19.473	2507310	19.868 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090220\
Data File : FF007445.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2020 14:37
Operator : DD\AJ
Sample : L3858-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 03 02:03:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

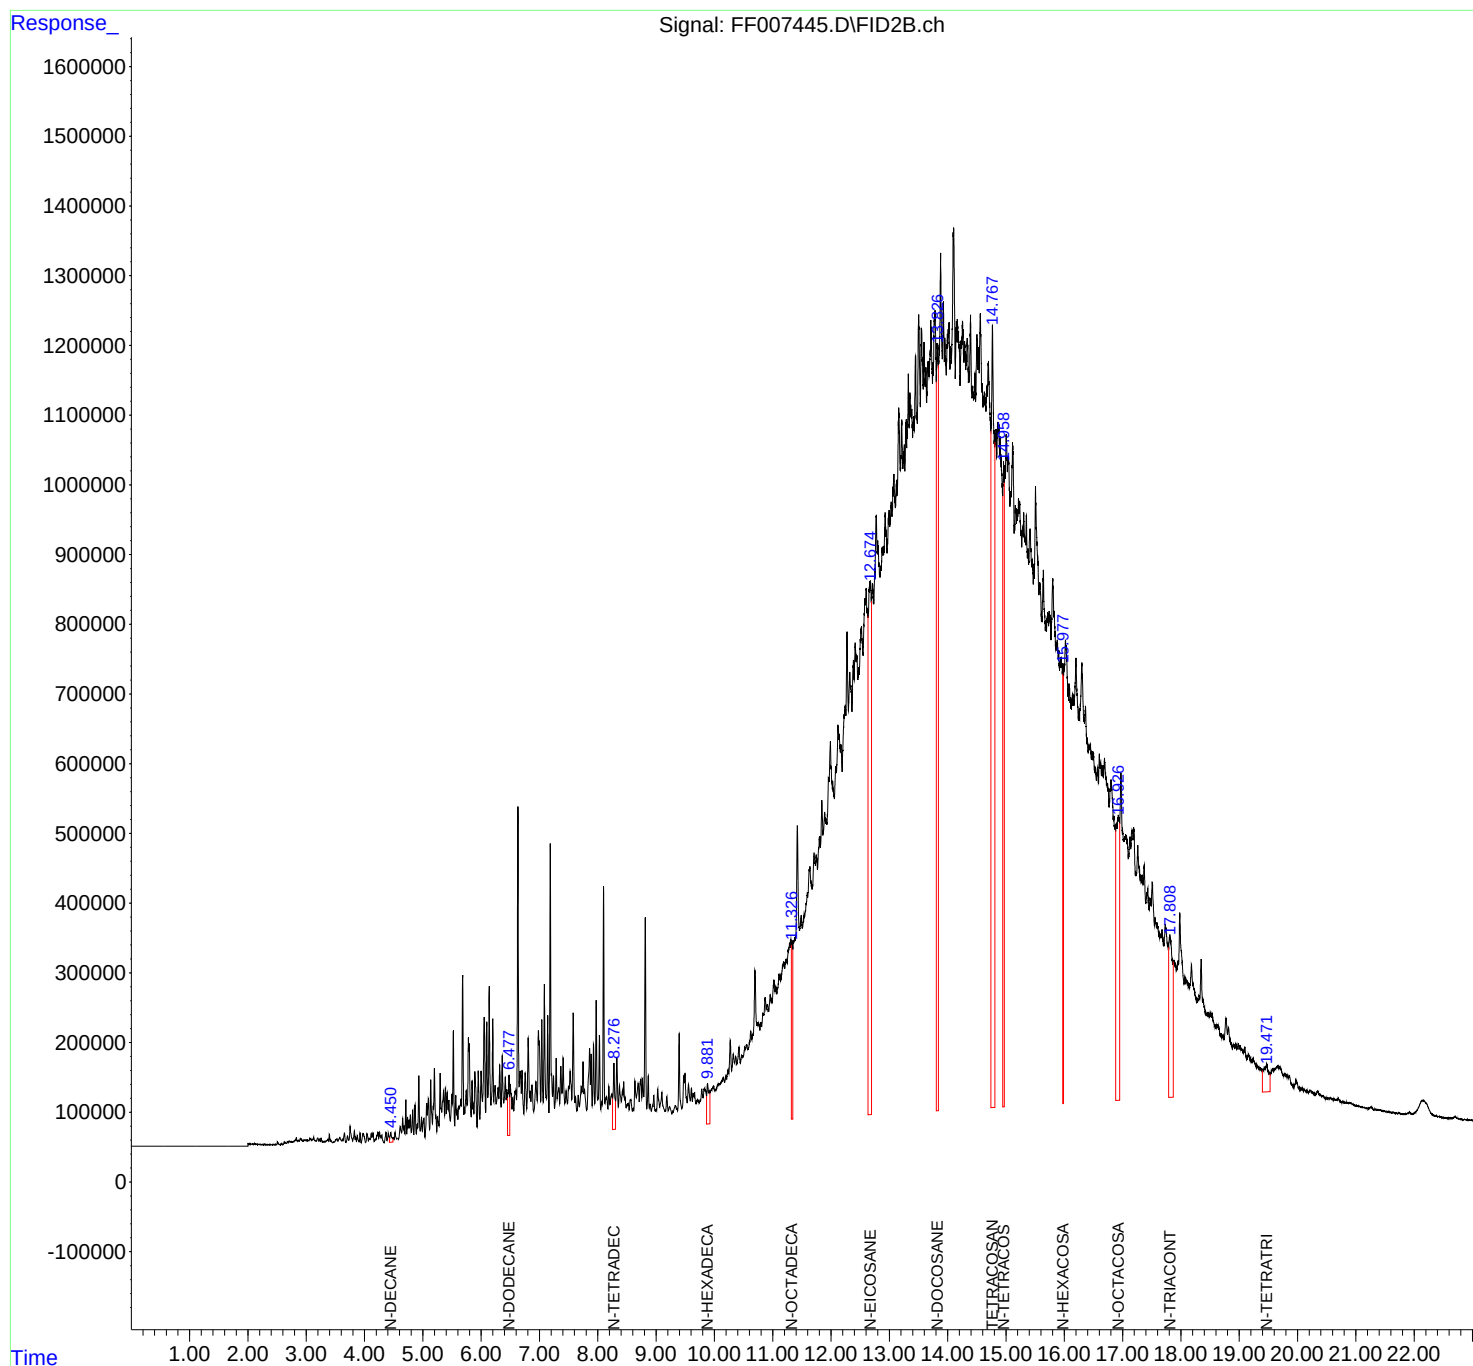


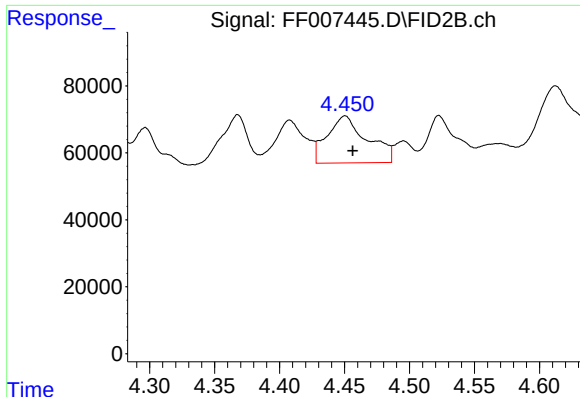

#2 N-DECANE


R.T.: 4.450 min
Delta R.T.: -0.006 min
Response: 299966
Conc: 1.88 ug/ml

Instrument :
FID_F
ClientSampleId :

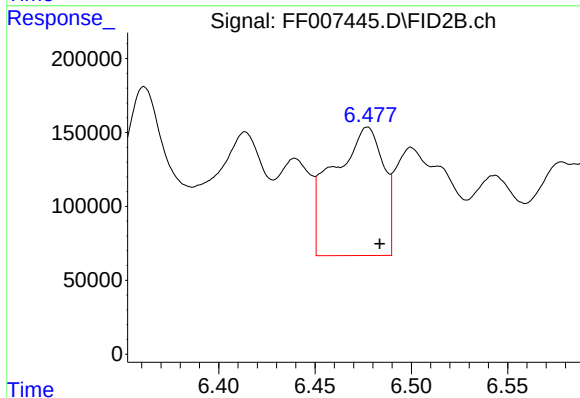


#3 N-DODECANE

R.T.: 6.477 min
Delta R.T.: -0.006 min
Response: 1578307
Conc: 9.70 ug/ml

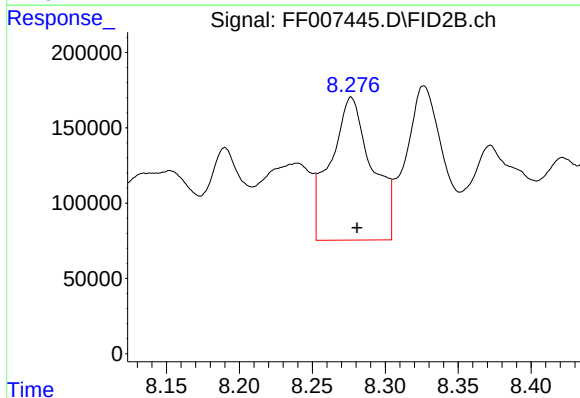


#4 N-TETRADECANE

R.T.: 8.277 min
Delta R.T.: -0.004 min
Response: 1867892
Conc: 11.35 ug/ml

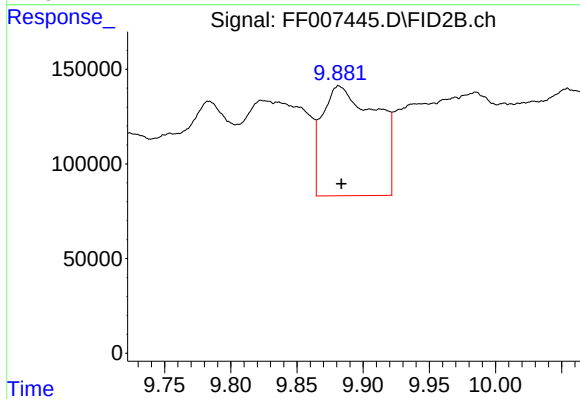

#5 N-HEXADECANE


R.T.: 9.882 min
Delta R.T.: -0.001 min
Response: 1648152
Conc: 9.77 ug/ml

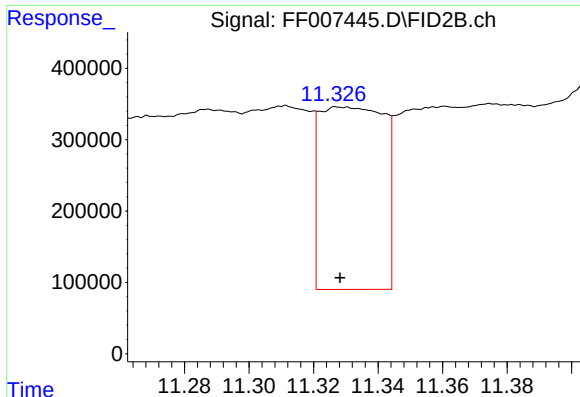

#6 N-OCTADECANE


R.T.: 11.330 min
Delta R.T.: 0.002 min
Response: 3535490
Conc: 20.75 ug/ml

Instrument :
FID_F
ClientSampleId :

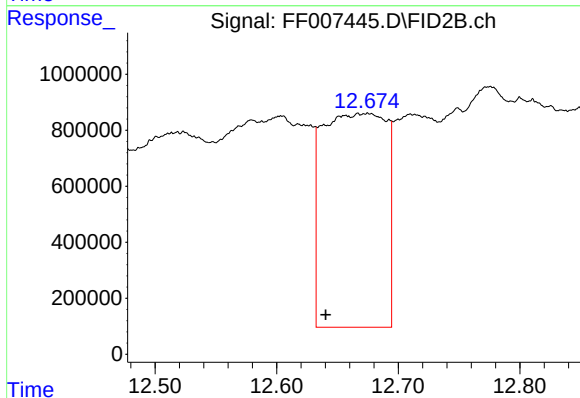


#7 N-EICOSANE

R.T.: 12.674 min
Delta R.T.: 0.034 min
Response: 27771935
Conc: 165.18 ug/ml

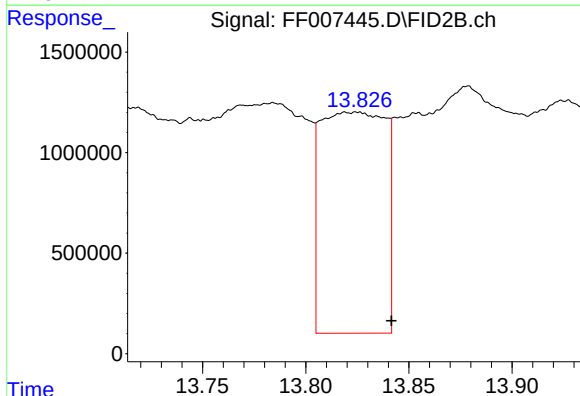


#8 N-DOCOSANE

R.T.: 13.824 min
Delta R.T.: -0.018 min
Response: 23756372
Conc: 144.19 ug/ml

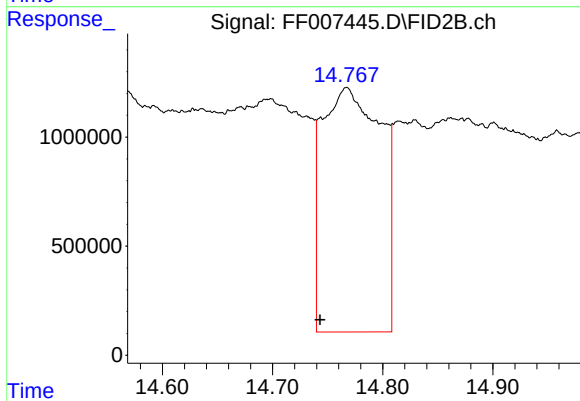

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.767 min
Delta R.T.: 0.024 min
Response: 41678370
Conc: 283.38 ug/ml

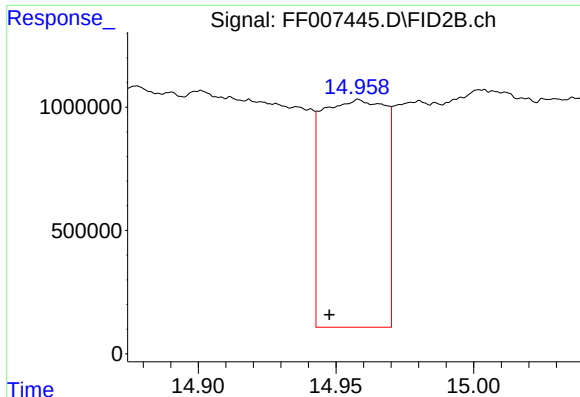

#10 N-TETRACOSANE


R.T.: 14.959 min
Delta R.T.: 0.011 min
Response: 14836204
Conc: 90.97 ug/ml

Instrument :
FID_F
ClientSampleId :

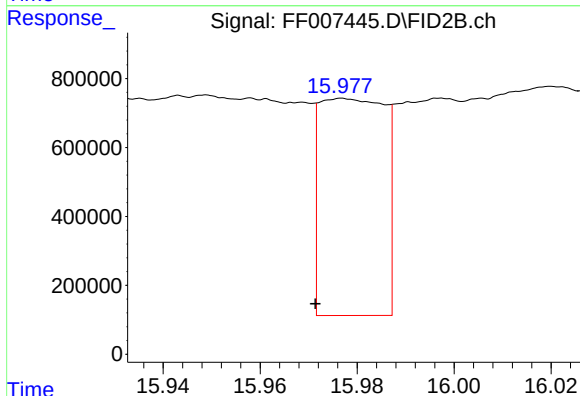


#11 N-HEXACOSANE

R.T.: 15.977 min
Delta R.T.: 0.006 min
Response: 5837456
Conc: 36.93 ug/ml

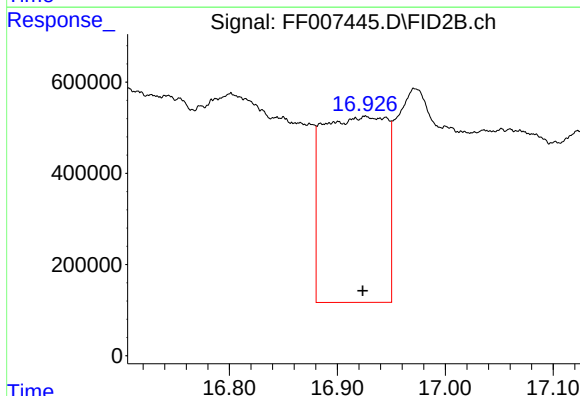


#12 N-OCTACOSANE

R.T.: 16.927 min
Delta R.T.: 0.003 min
Response: 16735674
Conc: 109.05 ug/ml

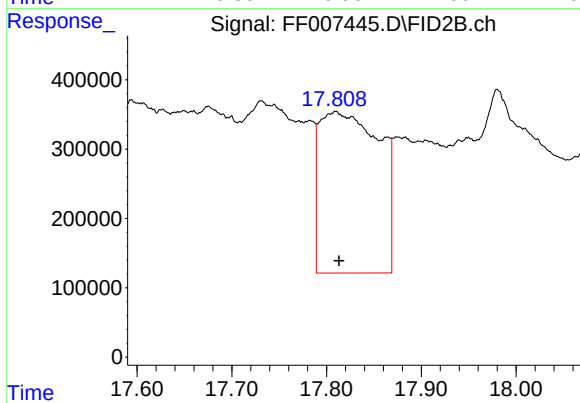

#13 N-TRIACONTANE

R.T.: 17.809 min
Delta R.T.: -0.004 min
Response: 10214543
Conc: 69.11 ug/ml

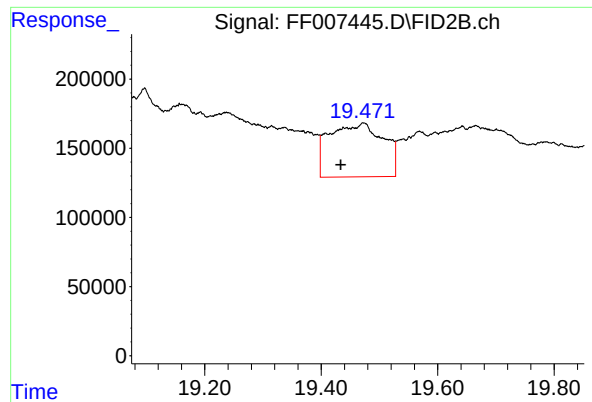

#15 N-TETRATRIACONTANE

R.T.: 19.473 min

Delta R.T.: 0.040 min

Response: 2507310

Conc: 19.87 ug/ml

Instrument :
FID_F
ClientSampleId :