

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090220\
 Data File : FF007447.D
 Signal(s) : FID2B.ch
 Acq On : 02 Sep 2020 15:39
 Operator : DD\AJ
 Sample : L3828-05 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 03 02:04:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	231769	1.576 ug/ml
Target Compounds			
2) N-DECANE	4.453	349120	2.189 ug/ml
3) N-DODECANE	6.479	1538449	9.457 ug/ml
4) N-TETRADECANE	8.277	2026287	12.314 ug/ml
5) N-HEXADECANE	9.880	1991955	11.804 ug/ml
6) N-OCTADECANE	11.323	310925	1.825 ug/ml
14) N-DOTRIACONTANE	18.647	269426	1.942 ug/ml
16) N-HEXATRIACONTANE	20.213	234047	1.958 ug/ml
18) N-TETRACONTANE	21.917	298916	2.694 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090220\
Data File : FF007447.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2020 15:39
Operator : DD\AJ
Sample : L3828-05 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 03 02:04:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

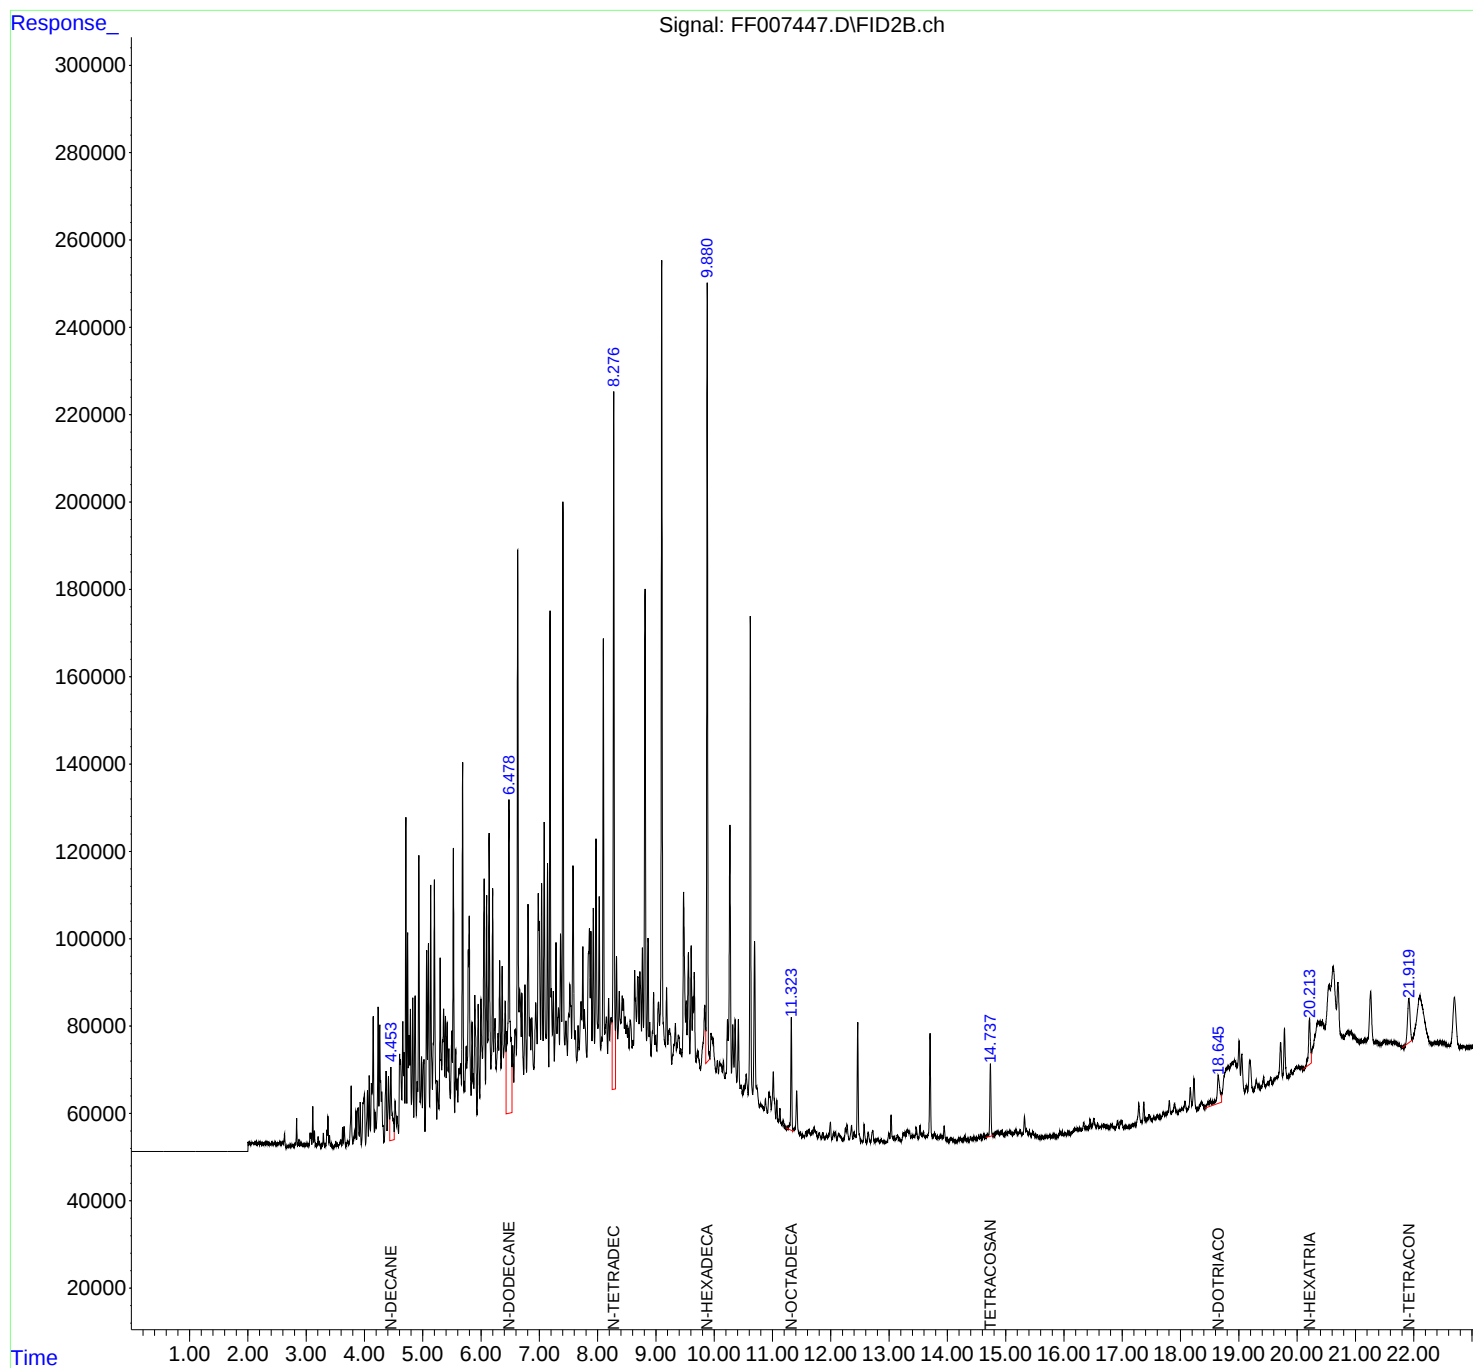


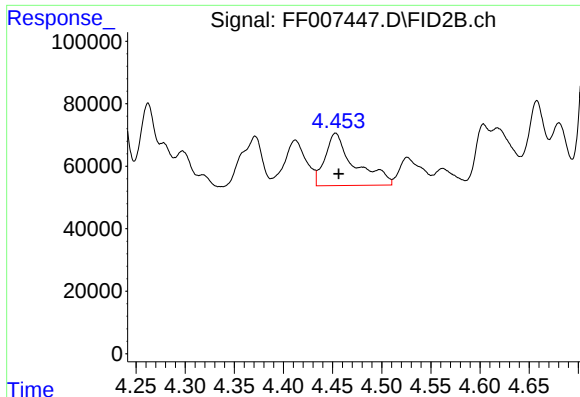

#2 N-DECANE


R.T.: 4.453 min
Delta R.T.: -0.003 min
Response: 349120
Conc: 2.19 ug/ml

Instrument :
FID_F
ClientSampleId :

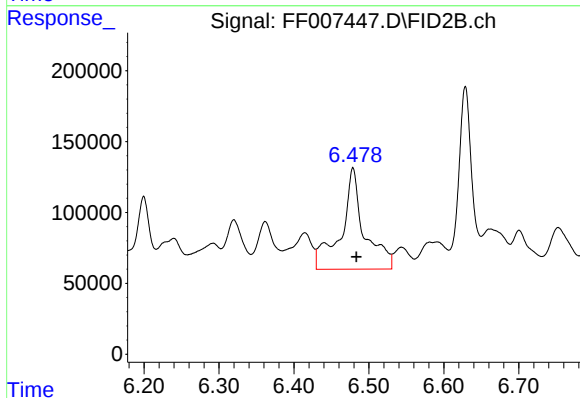


#3 N-DODECANE

R.T.: 6.479 min
Delta R.T.: -0.005 min
Response: 1538449
Conc: 9.46 ug/ml

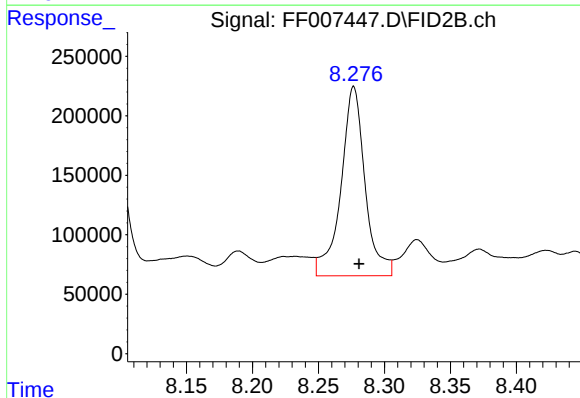


#4 N-TETRADECANE

R.T.: 8.277 min
Delta R.T.: -0.004 min
Response: 2026287
Conc: 12.31 ug/ml

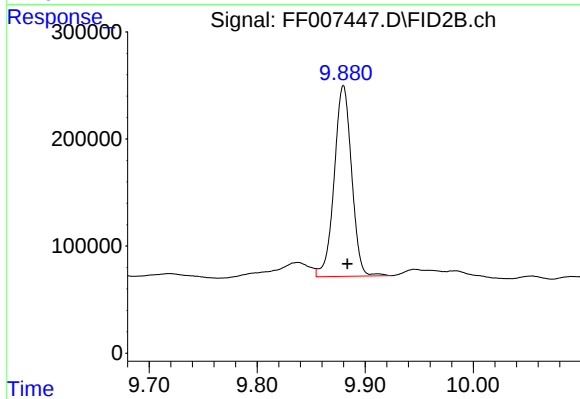

#5 N-HEXADECANE


R.T.: 9.880 min
Delta R.T.: -0.004 min
Response: 1991955
Conc: 11.80 ug/ml

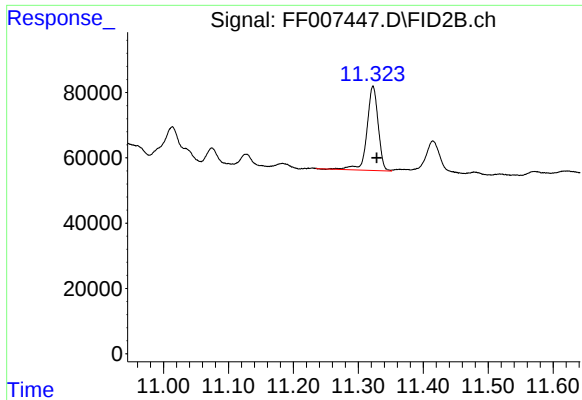

#6 N-OCTADECANE


R.T.: 11.323 min
Delta R.T.: -0.006 min
Response: 310925
Conc: 1.82 ug/ml

Instrument :
FID_F
ClientSampleId :

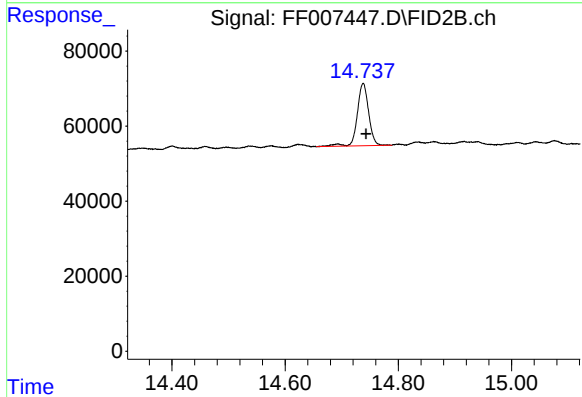


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.738 min
Delta R.T.: -0.005 min
Response: 231769
Conc: 1.58 ug/ml

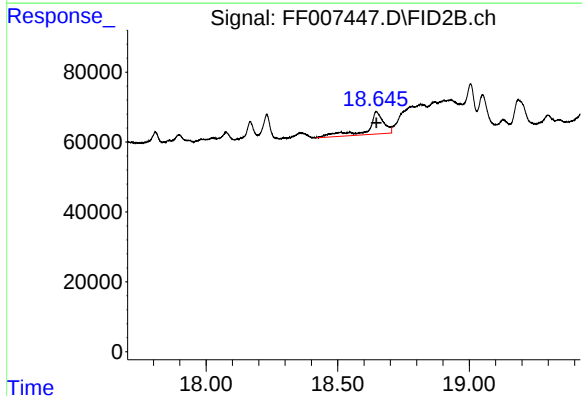


#14 N-DOTRIACONTANE

R.T.: 18.647 min
Delta R.T.: 0.000 min
Response: 269426
Conc: 1.94 ug/ml

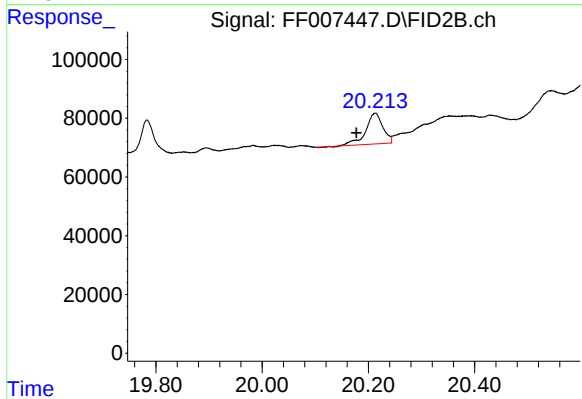

#16 N-HEXATRIACONTANE

R.T.: 20.213 min
Delta R.T.: 0.036 min
Response: 234047
Conc: 1.96 ug/ml

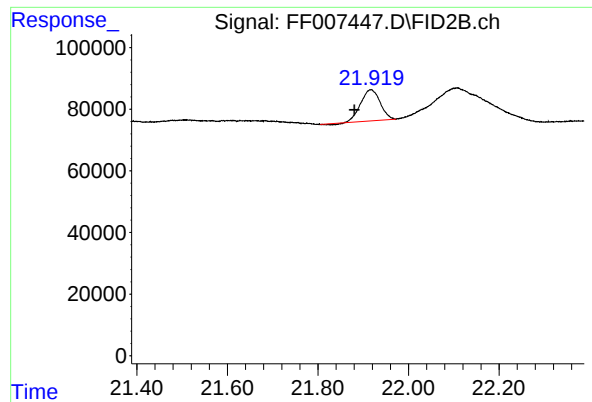

#18 N-TETRACONTANE

R.T.: 21.917 min
Delta R.T.: 0.036 min
Response: 298916
Conc: 2.69 ug/ml

Instrument :
FID_F
ClientSampleId :