

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090220\
 Data File : FF007451.D
 Signal(s) : FID2B.ch
 Acq On : 02 Sep 2020 17:45
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 03 02:05:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	3156208	21.460 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.645	111252	0.802 ug/ml
16) N-HEXATRIACONTANE	20.212	223268	1.868 ug/ml
18) N-TETRACONTANE	21.918	355621	3.205 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090220\
Data File : FF007451.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2020 17:45
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 03 02:05:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

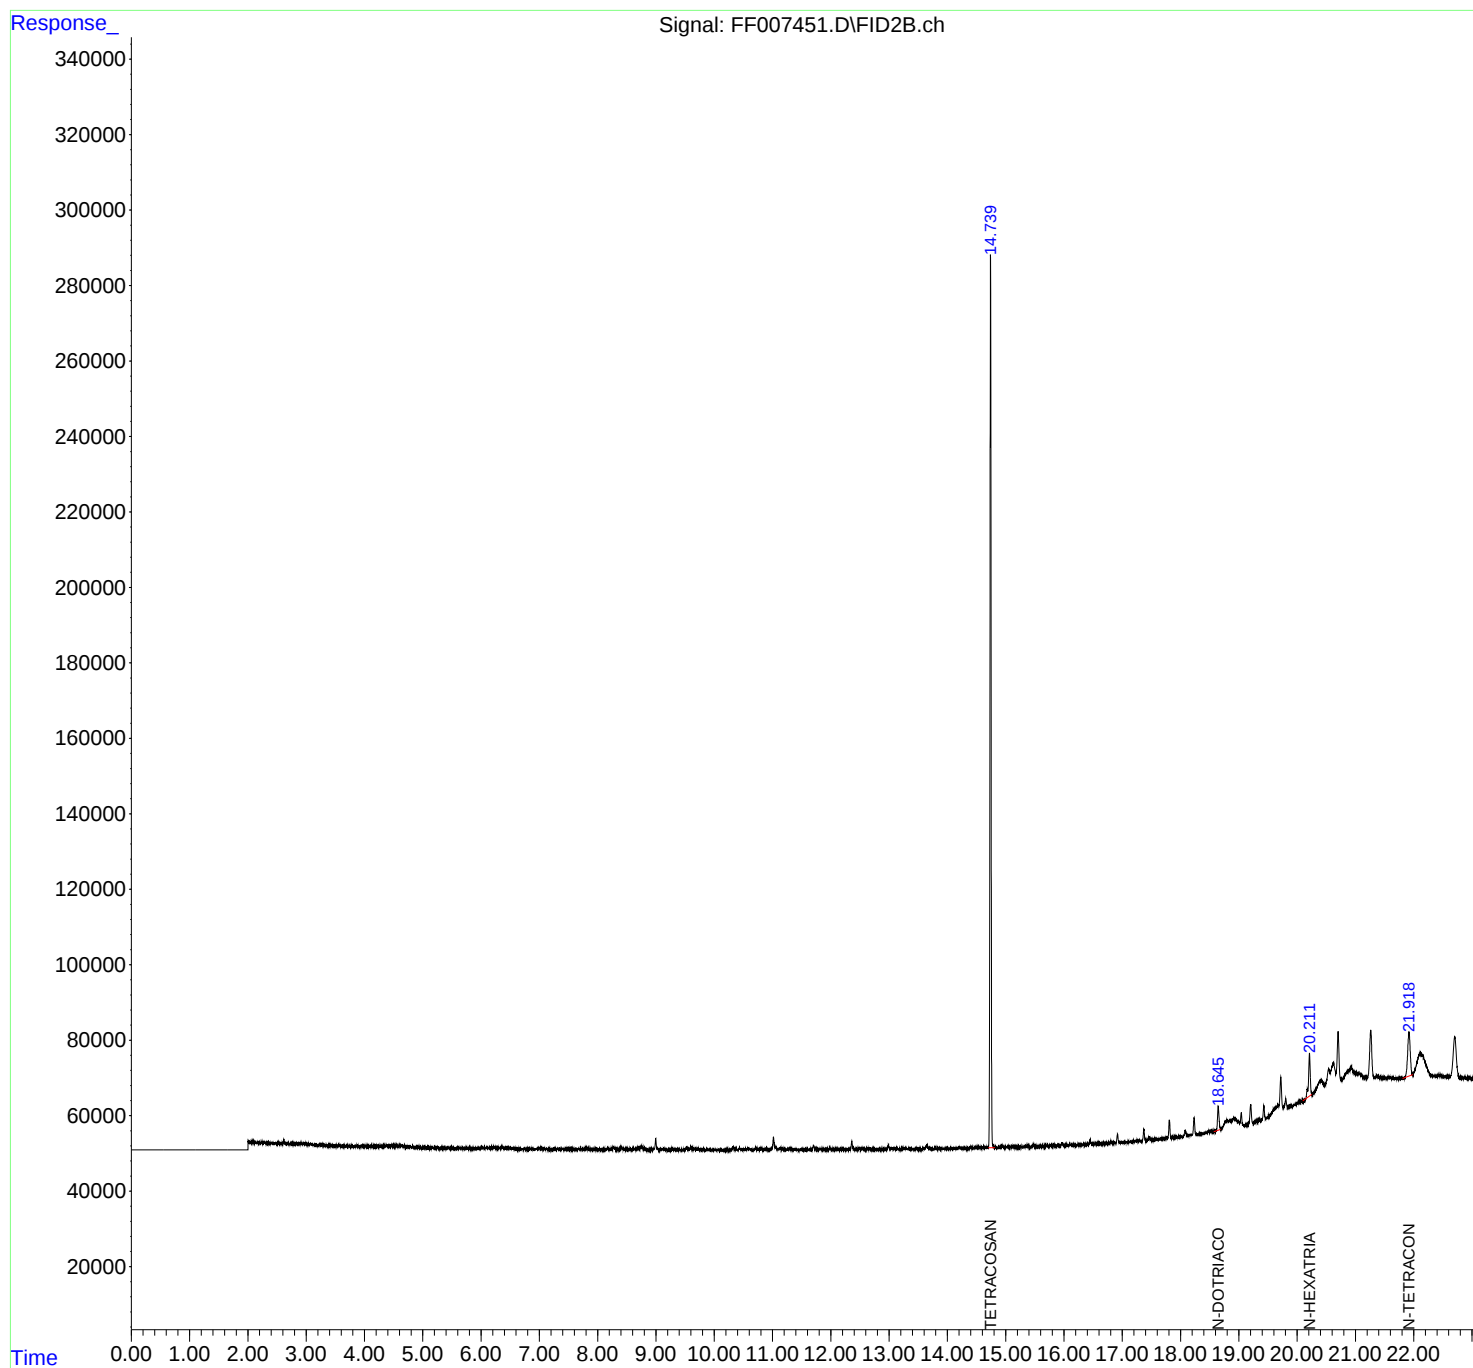


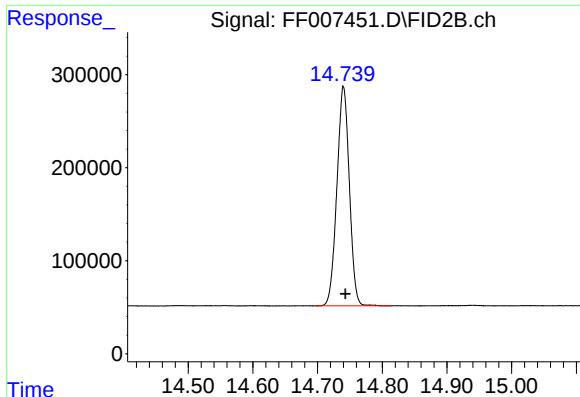

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.740 min
Delta R.T.: -0.003 min
Response: 3156208
Conc: 21.46 ug/ml

Instrument :
FID_F
ClientSampleId :

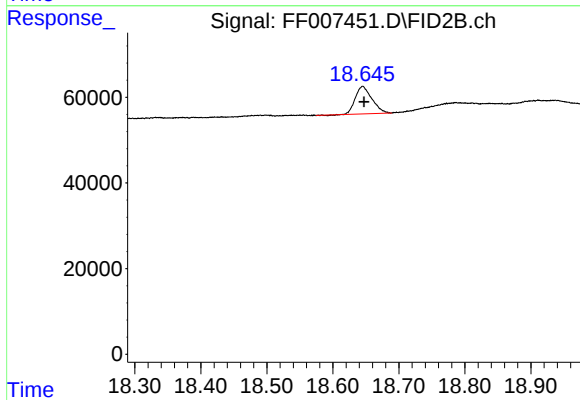


#14 N-DOTRIACONTANE

R.T.: 18.645 min
Delta R.T.: -0.002 min
Response: 111252
Conc: 0.80 ug/ml

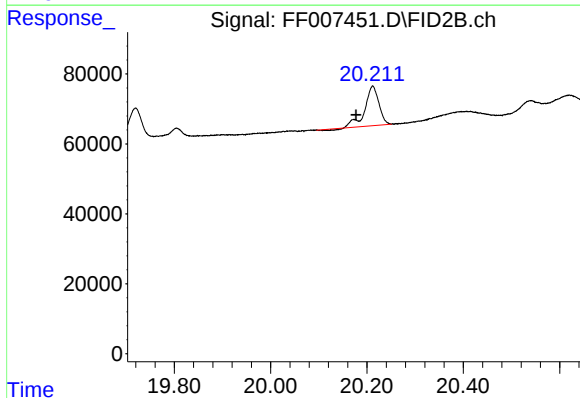

#16 N-HEXATRIACONTANE

R.T.: 20.212 min
Delta R.T.: 0.035 min
Response: 223268
Conc: 1.87 ug/ml

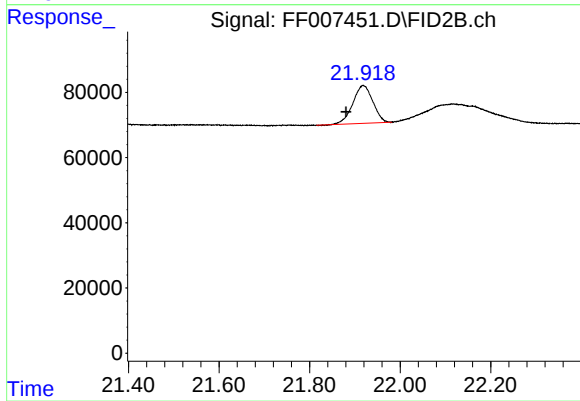

#18 N-TETRACONTANE

R.T.: 21.918 min
Delta R.T.: 0.038 min
Response: 355621
Conc: 3.21 ug/ml