

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
Data File : FF011357.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2022 11:49
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 02:05:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.675	51067	0.388 ug/ml
10)	N-TETRACOSANE	14.947	39477	0.310 ug/ml
14)	N-DOTRIACONTANE	18.689	85725	0.725 ug/ml
16)	N-HEXATRIACONTANE	20.236	64157	0.603 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
Data File : FF011357.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2022 11:49
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 02:05:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

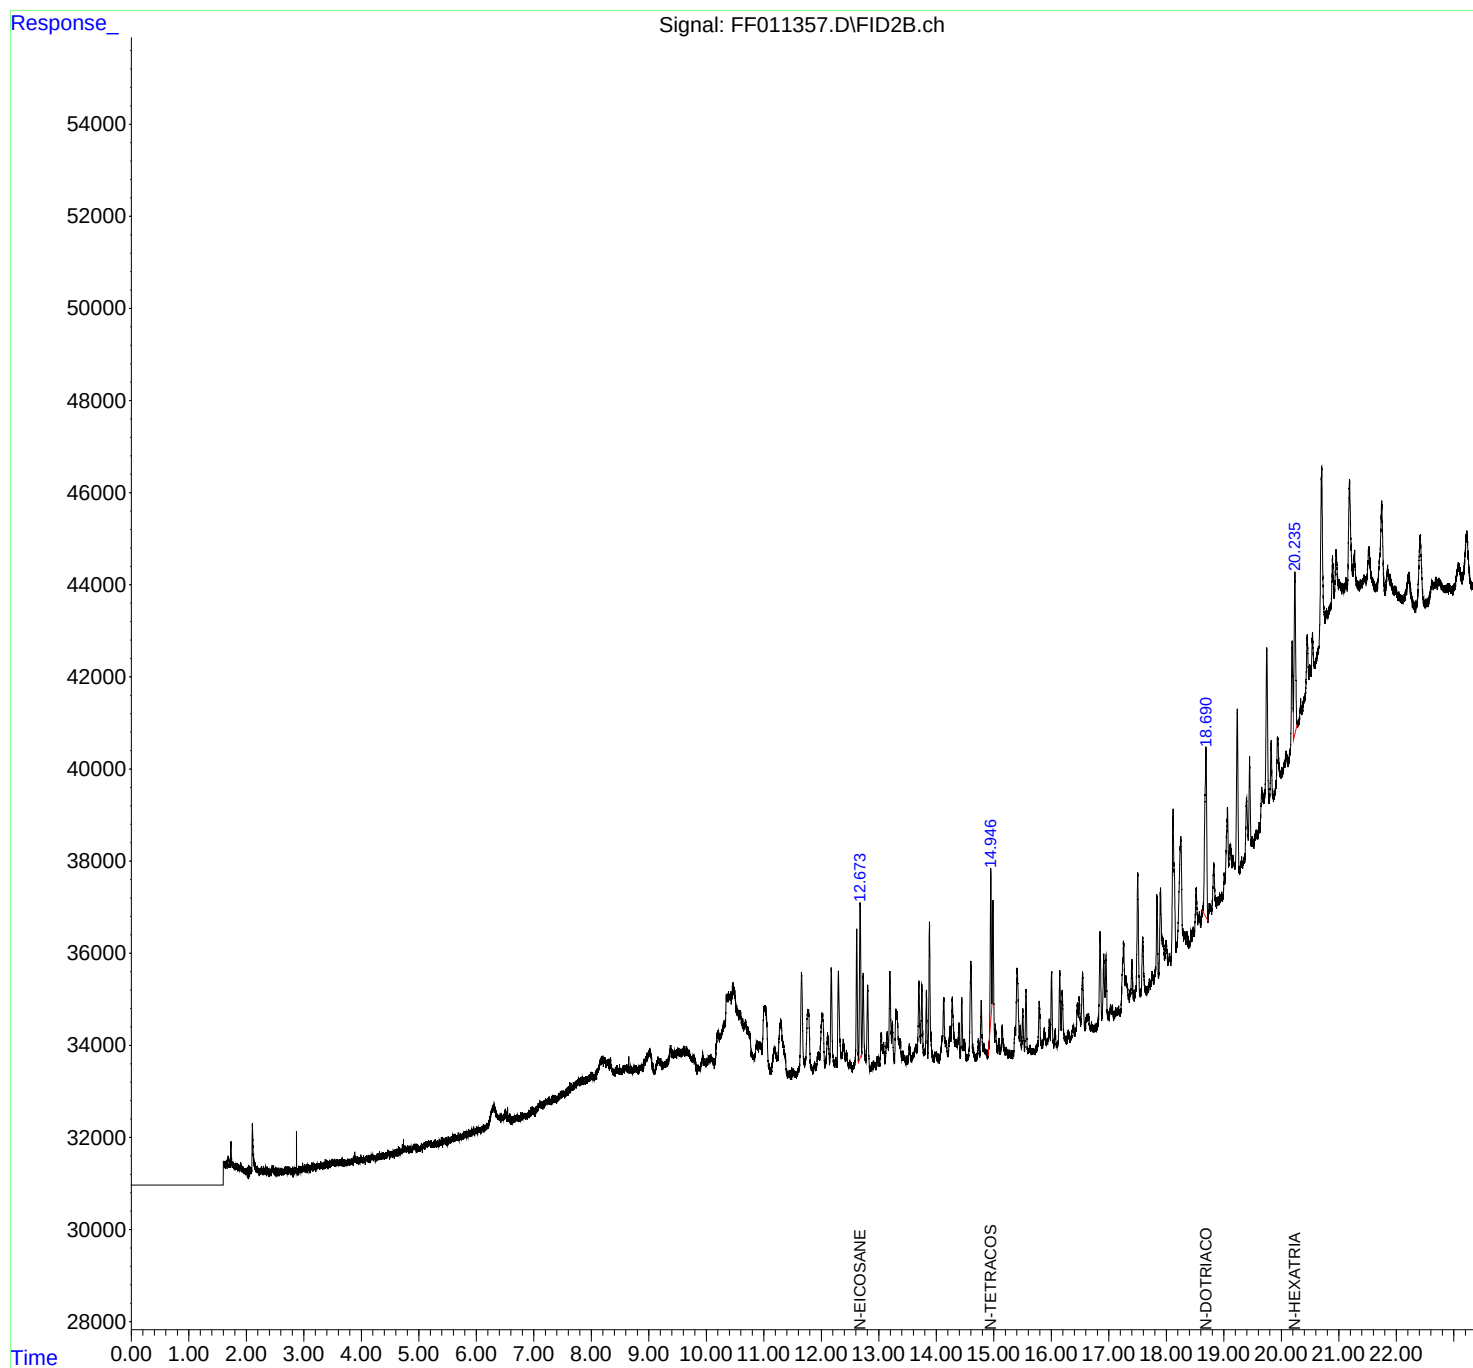


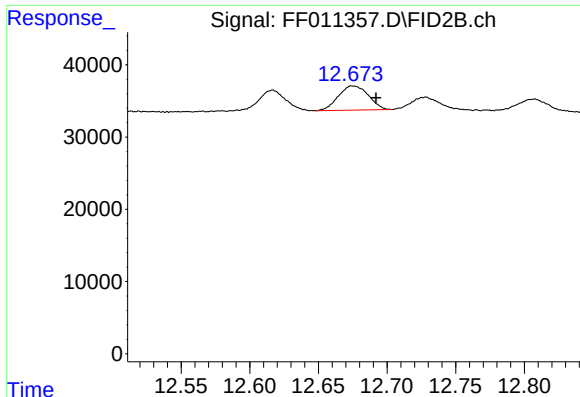

#7 N-EICOSANE


R.T.: 12.675 min
Delta R.T.: -0.017 min
Response: 51067
Conc: 0.39 ug/ml

Instrument :
FID_F
ClientSampleId :

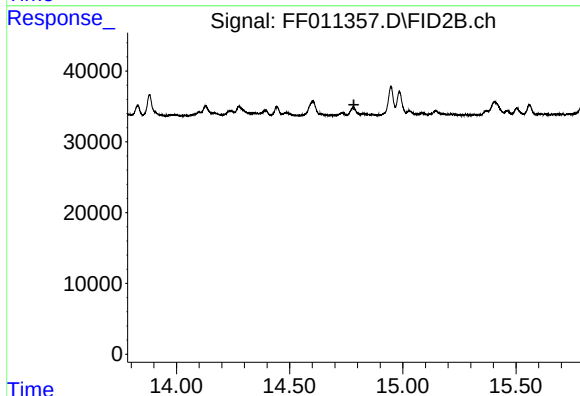


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

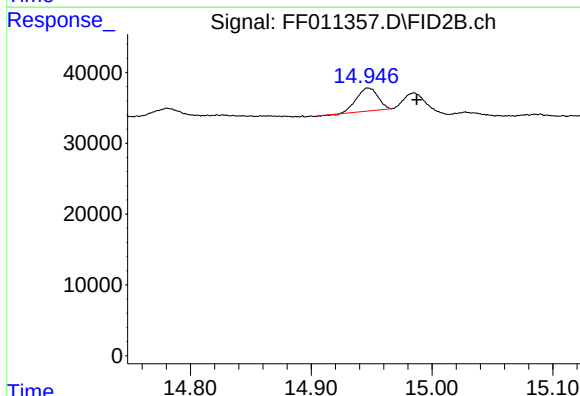


#10 N-TETRACOSANE

R.T.: 14.947 min
Delta R.T.: -0.040 min
Response: 39477
Conc: 0.31 ug/ml

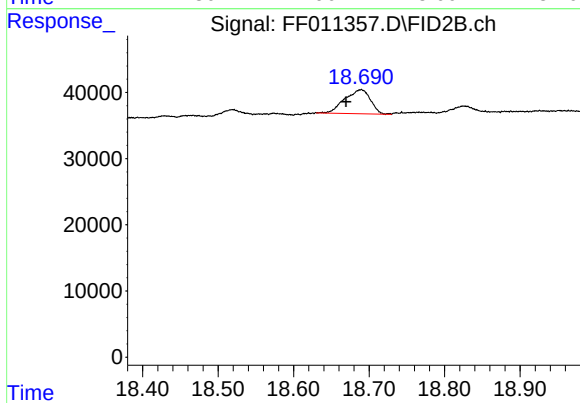

#14 N-DOTRIACONTANE

R.T.: 18.689 min
Delta R.T.: 0.020 min
Response: 85725
Conc: 0.72 ug/ml

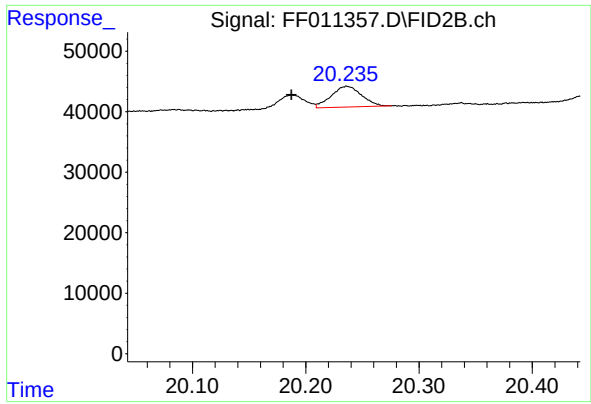

#16 N-HEXATRIACONTANE

R.T.: 20.236 min
Delta R.T.: 0.049 min
Response: 64157
Conc: 0.60 ug/ml

Instrument :

FID_F

ClientSampleId :