

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
 Data File : FF011358.D
 Signal(s) : FID2B.ch
 Acq On : 02 Sep 2022 12:18
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 05 02:06:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.784	2503168	22.332 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.839	110827	0.919 ug/ml
14) N-DOTRIACONTANE	18.669	154749	1.308 ug/ml
15) N-TETRATRIACONTANE	19.450	128049	1.122 ug/ml
16) N-HEXATRIACONTANE	20.187	87312	0.820 ug/ml
17) N-OCTATRIACONTANE	20.891	58182	0.559 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
Data File : FF011358.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2022 12:18
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 02:06:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

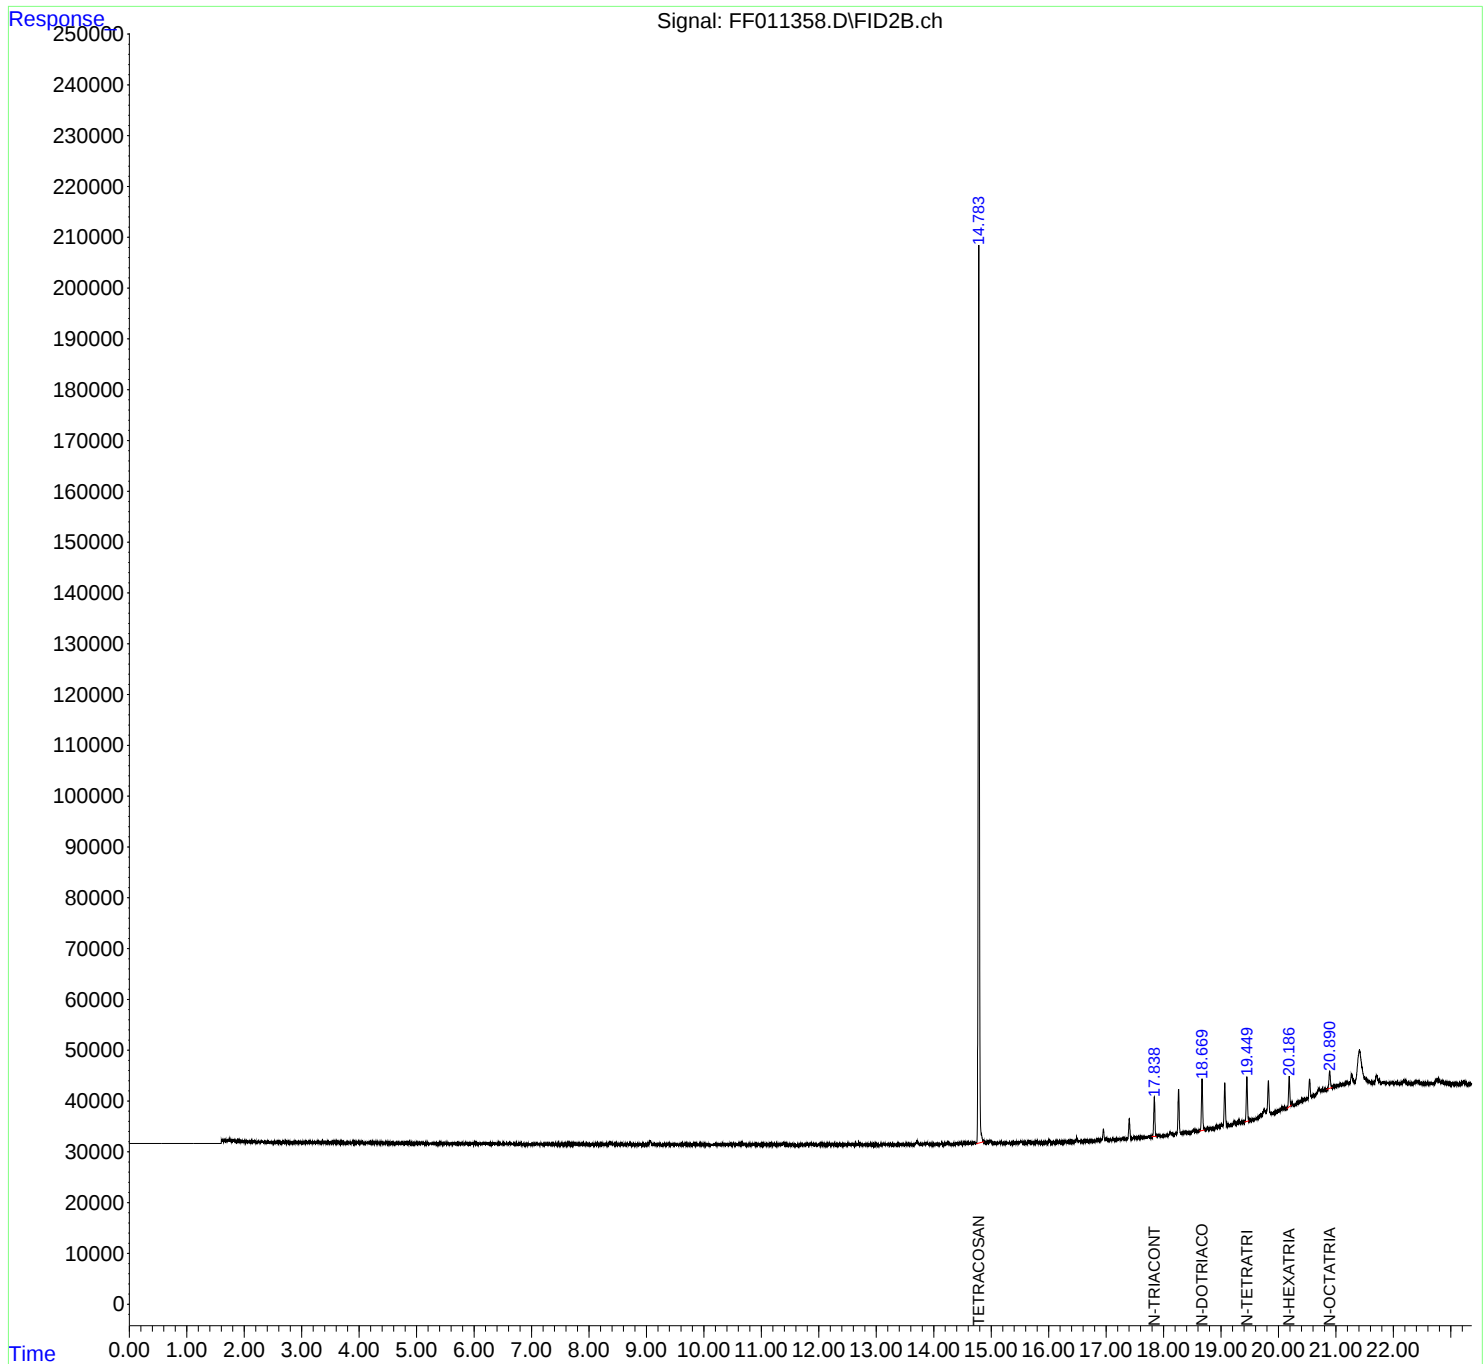


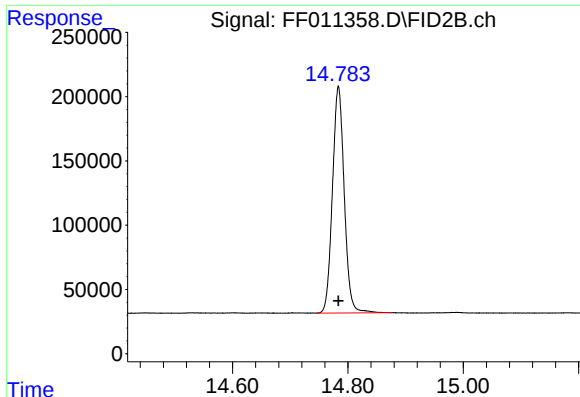

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.784 min
Delta R.T.: 0.000 min
Response: 2503168
Conc: 22.33 ug/ml

Instrument :
FID_F
ClientSampleId :

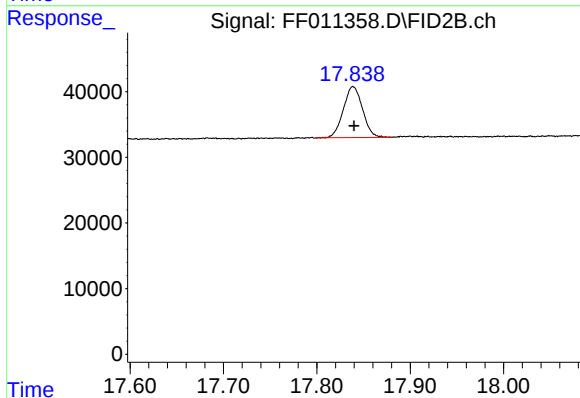


#13 N-TRIACONTANE

R.T.: 17.839 min
Delta R.T.: -0.001 min
Response: 110827
Conc: 0.92 ug/ml

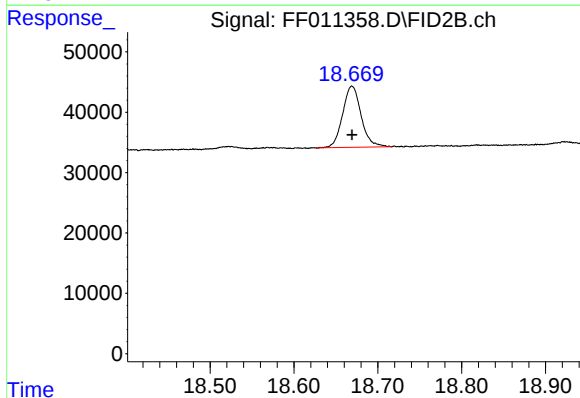


#14 N-DOTRIACONTANE

R.T.: 18.669 min
Delta R.T.: 0.000 min
Response: 154749
Conc: 1.31 ug/ml

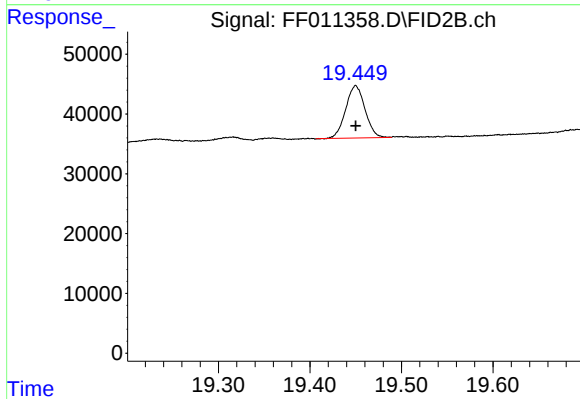

#15 N-TETRATRIACONTANE


R.T.: 19.450 min
Delta R.T.: 0.000 min
Response: 128049
Conc: 1.12 ug/ml

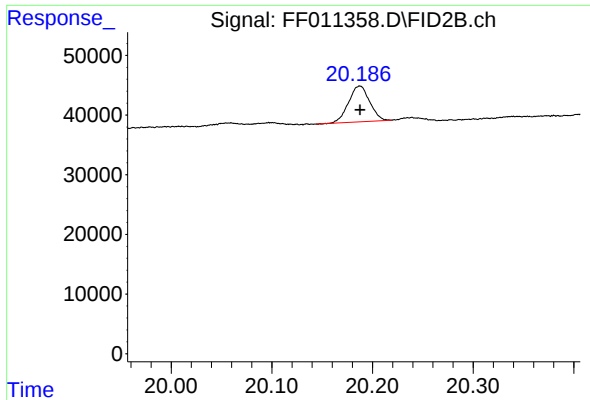

#16 N-HEXATRIACONTANE

R.T.: 20.187 min
Delta R.T.: 0.000 min
Response: 87312
Conc: 0.82 ug/ml

Instrument :
FID_F
ClientSampleId :

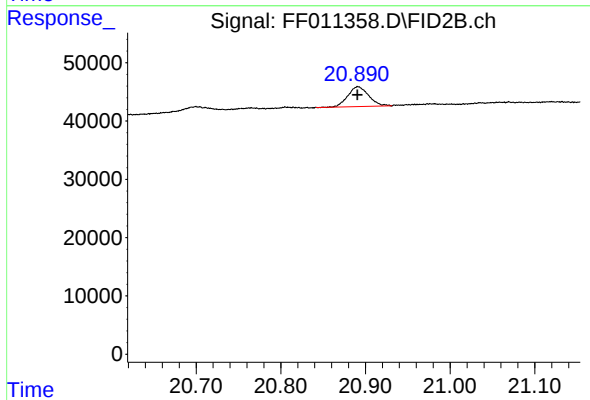

#17 N-OCTATRIACONTANE

R.T.: 20.891 min
Delta R.T.: 0.000 min
Response: 58182
Conc: 0.56 ug/ml