

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
Data File : FF011365.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2022 16:37
Operator : YP\AJ
Sample : N4490-04 250X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 02:07:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10)	N-TETRACOSANE	14.992	50591	0.397 ug/ml
11)	N-HEXACOSANE	16.021	54528	0.437 ug/ml
12)	N-OCTACOSANE	16.963	141316	1.154 ug/ml
13)	N-TRIACONTANE	17.808	117580	0.975 ug/ml
15)	N-TETRATRIACONTANE	19.469	75873	0.665 ug/ml
16)	N-HEXATRIACONTANE	20.168	94218	0.885 ug/ml
17)	N-OCTATRIACONTANE	20.847	285928	2.749 ug/ml
18)	N-TETRACONTANE	21.754	511068	4.844 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
Data File : FF011365.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2022 16:37
Operator : YP\AJ
Sample : N4490-04 250X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 02:07:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

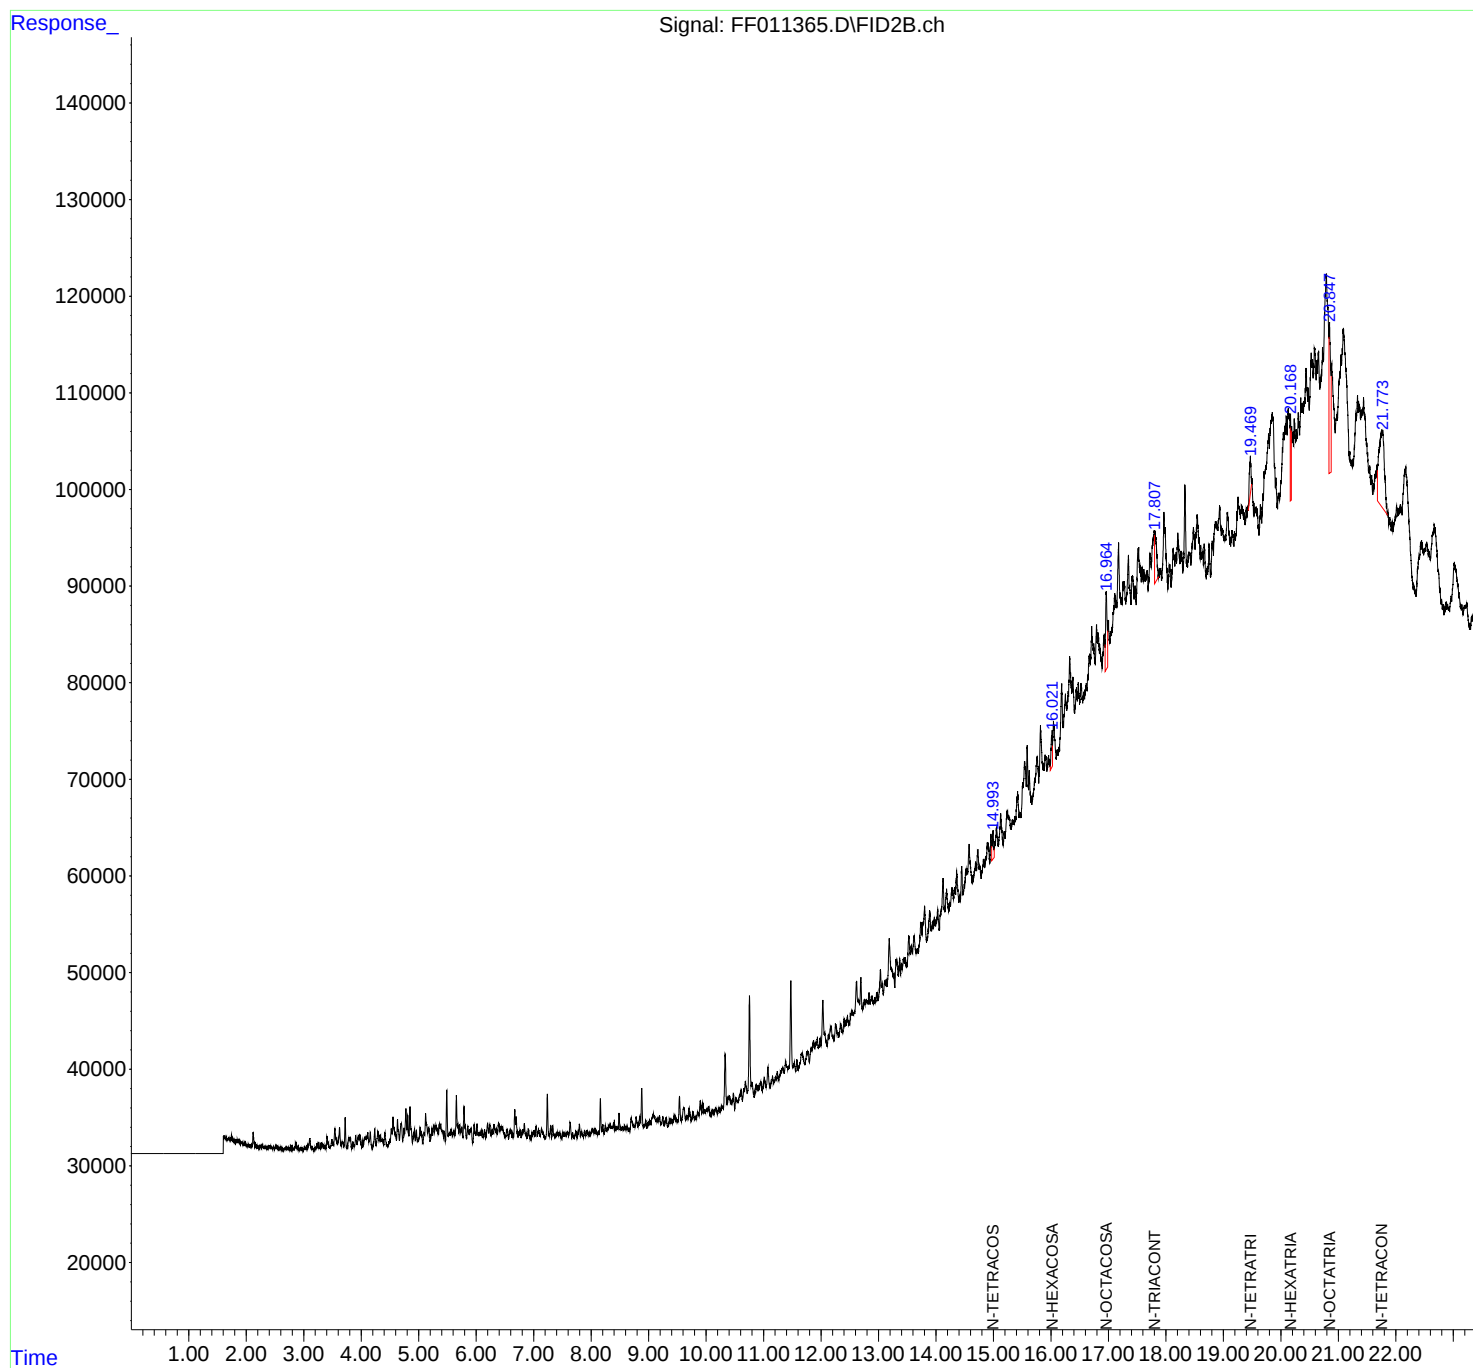


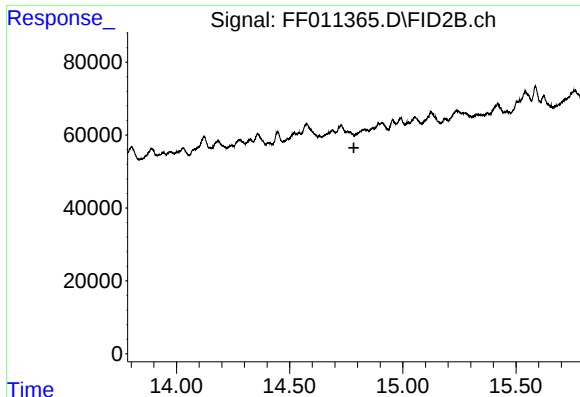

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.784 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

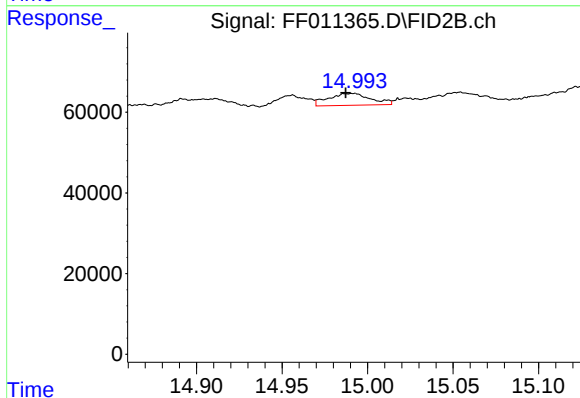


#10 N-TETRACOSANE

R.T.: 14.992 min
Delta R.T.: 0.005 min
Response: 50591
Conc: 0.40 ug/ml

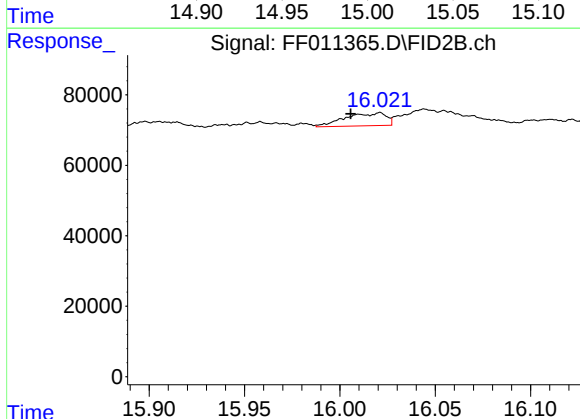


#11 N-HEXACOSANE

R.T.: 16.021 min
Delta R.T.: 0.015 min
Response: 54528
Conc: 0.44 ug/ml

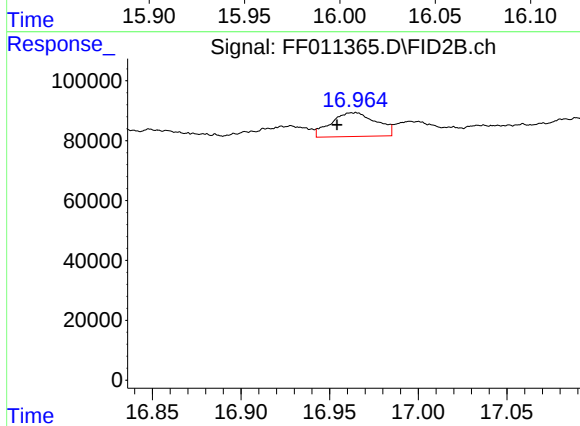

#12 N-OCTACOSANE


R.T.: 16.963 min
Delta R.T.: 0.009 min
Response: 141316
Conc: 1.15 ug/ml

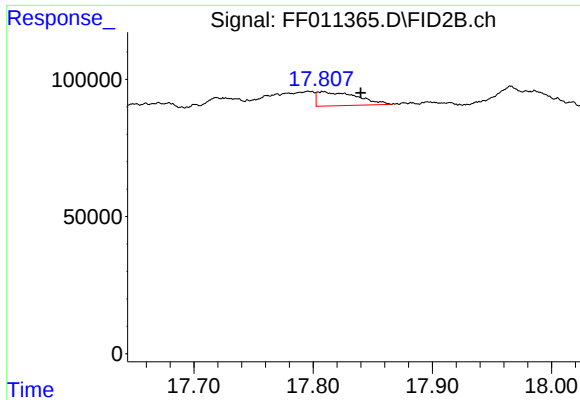

#13 N-TRIACONTANE


R.T.: 17.808 min
Delta R.T.: -0.031 min
Response: 117580
Conc: 0.97 ug/ml

Instrument :
FID_F
ClientSampleId :

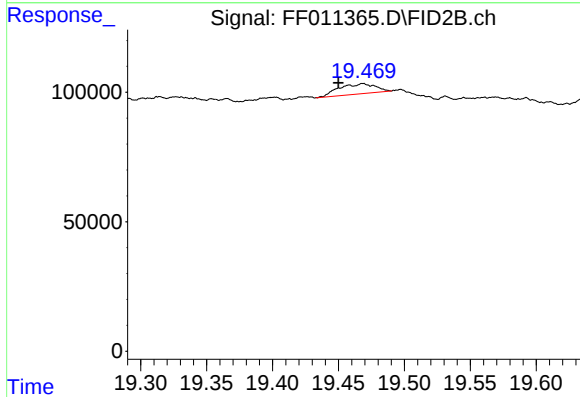


#15 N-TETRATRIACONTANE

R.T.: 19.469 min
Delta R.T.: 0.019 min
Response: 75873
Conc: 0.66 ug/ml

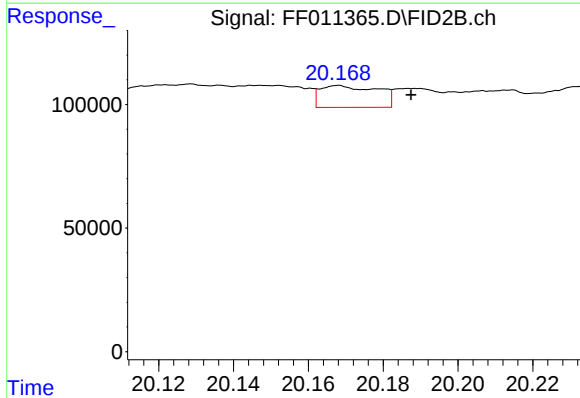


#16 N-HEXATRIACONTANE

R.T.: 20.168 min
Delta R.T.: -0.019 min
Response: 94218
Conc: 0.89 ug/ml

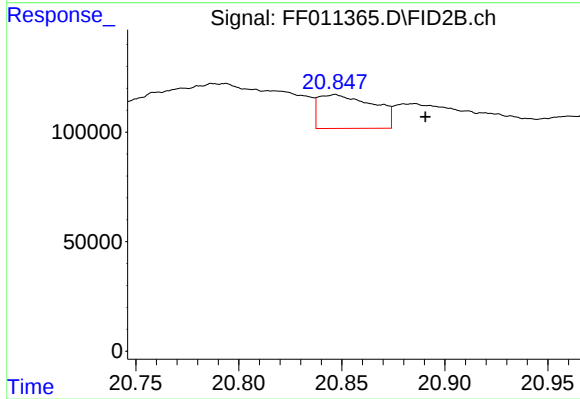

#17 N-OCTATRIACONTANE

R.T.: 20.847 min
Delta R.T.: -0.044 min
Response: 285928
Conc: 2.75 ug/ml

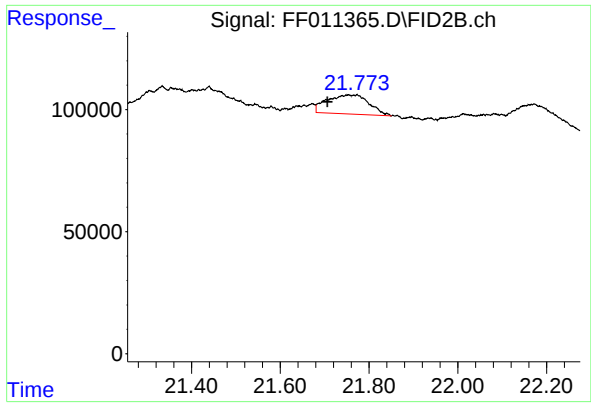

#18 N-TETRACONTANE

R.T.: 21.754 min
Delta R.T.: 0.048 min
Response: 511068
Conc: 4.84 ug/ml

Instrument :
FID_F
ClientSampleId :