

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
Data File : FF011366.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2022 17:07
Operator : YP\AJ
Sample : N4490-09 250X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 02:07:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

5)	N-HEXADECANE	9.898	50934	0.384 ug/ml
10)	N-TETRACOSANE	14.954	29502	0.232 ug/ml
15)	N-TETRATRIACONTANE	19.456	51227	0.449 ug/ml
16)	N-HEXATRIACONTANE	20.197	51353	0.482 ug/ml
17)	N-OCTATRIACONTANE	20.842	53596	0.515 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
Data File : FF011366.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2022 17:07
Operator : YP\AJ
Sample : N4490-09 250X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 02:07:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

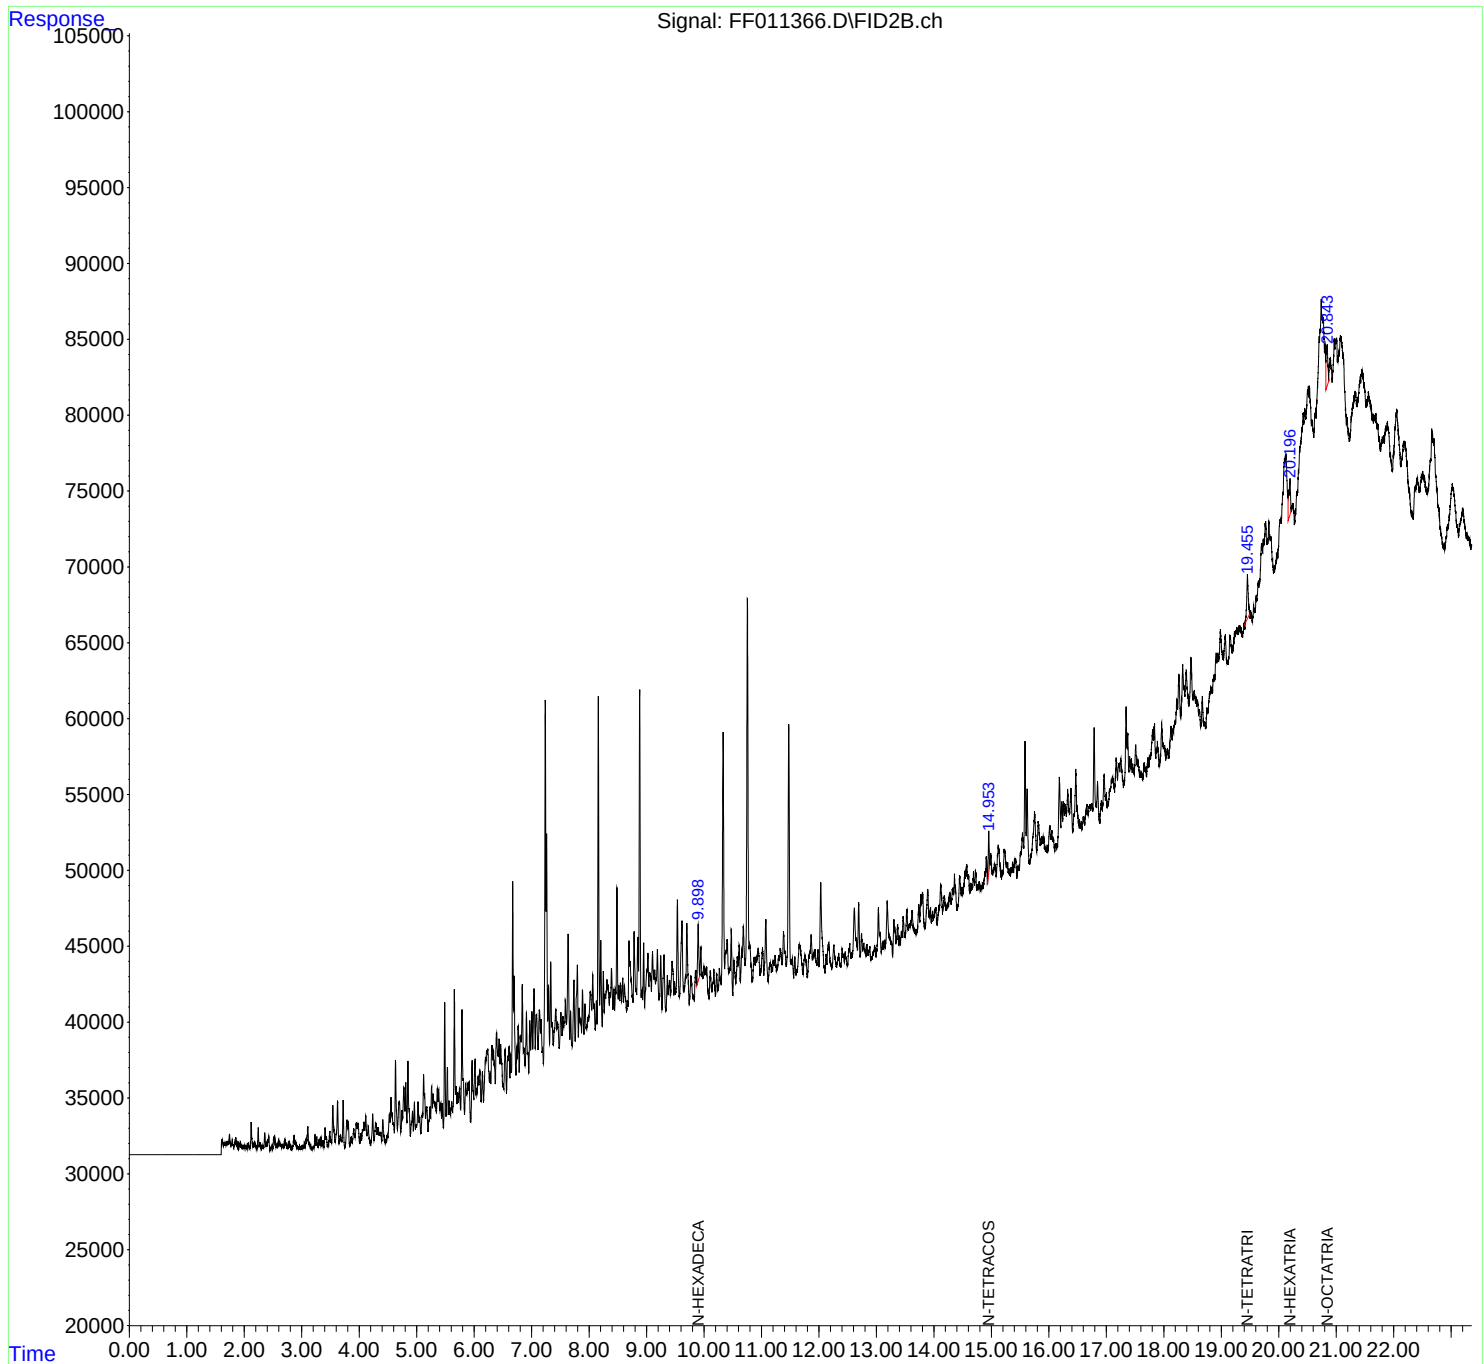


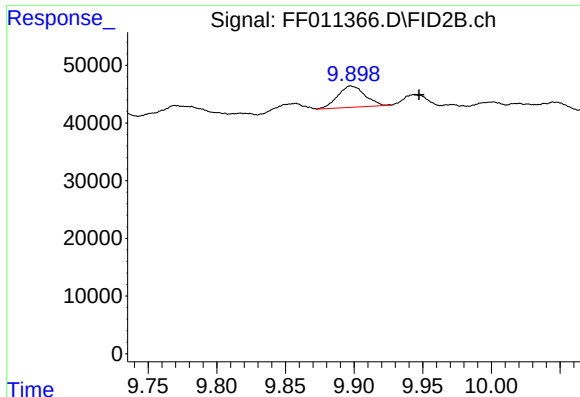

#5 N-HEXADECANE


R.T.: 9.898 min
Delta R.T.: -0.049 min
Response: 50934
Conc: 0.38 ug/ml

Instrument :
FID_F
ClientSampleId :

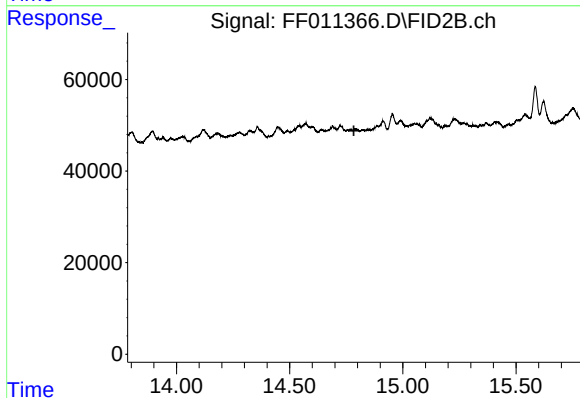


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

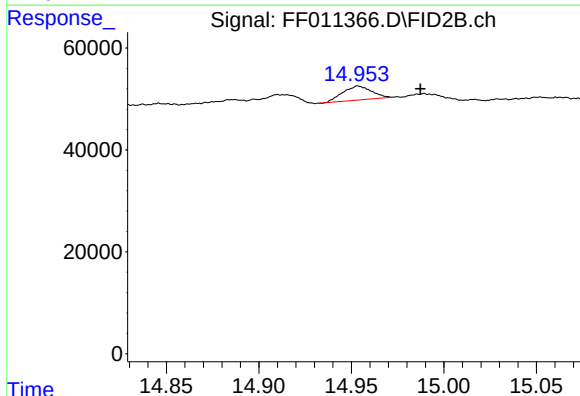


#10 N-TETRACOSANE

R.T.: 14.954 min
Delta R.T.: -0.033 min
Response: 29502
Conc: 0.23 ug/ml

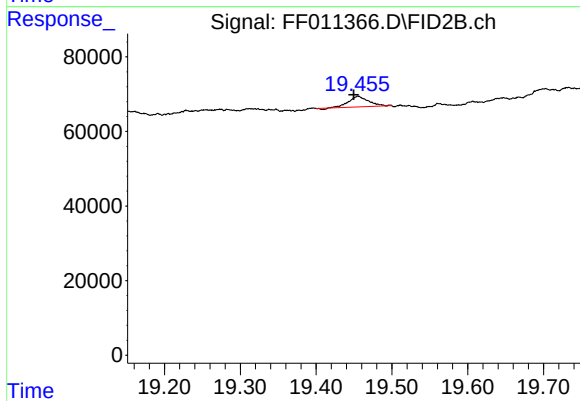

#15 N-TETRATRIACONTANE


R.T.: 19.456 min
Delta R.T.: 0.006 min
Response: 51227
Conc: 0.45 ug/ml

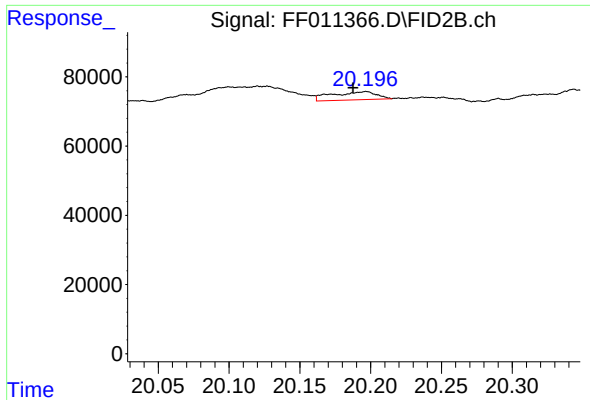

#16 N-HEXATRIACONTANE

R.T.: 20.197 min
Delta R.T.: 0.009 min
Response: 51353
Conc: 0.48 ug/ml

Instrument :
FID_F
ClientSampleId :

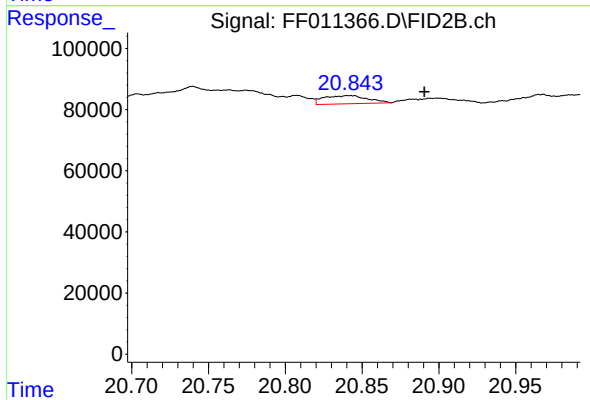

#17 N-OCTATRIACONTANE

R.T.: 20.842 min
Delta R.T.: -0.048 min
Response: 53596
Conc: 0.52 ug/ml