

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
 Data File : FF011362.D
 Signal(s) : FID2B.ch
 Acq On : 02 Sep 2022 15:08
 Operator : YP\AJ
 Sample : PB147448BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB147448BS

Integration File: autoint1.e
 Quant Time: Sep 05 02:07:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.784	2202111	19.646 ug/ml
Target Compounds			
2) N-DECANE	4.347	2397675	18.479 ug/ml
3) N-DODECANE	6.517	2444374	18.666 ug/ml
4) N-TETRADECANE	8.341	2473549	18.832 ug/ml
5) N-HEXADECANE	9.944	2308236	17.402 ug/ml
6) N-OCTADECANE	11.383	2512653	18.902 ug/ml
7) N-EICOSANE	12.690	2494450	18.963 ug/ml
8) N-DOCOSANE	13.886	2448662	19.158 ug/ml
10) N-TETRACOSANE	14.987	2447171	19.219 ug/ml
11) N-HEXACOSANE	16.005	2379099	19.047 ug/ml
12) N-OCTACOSANE	16.953	2330727	19.028 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090222\
Data File : FF011362.D
Signal(s) : FID2B.ch
Acq On : 02 Sep 2022 15:08
Operator : YP\AJ
Sample : PB147448BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB147448BS

Integration File: autoint1.e
Quant Time: Sep 05 02:07:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

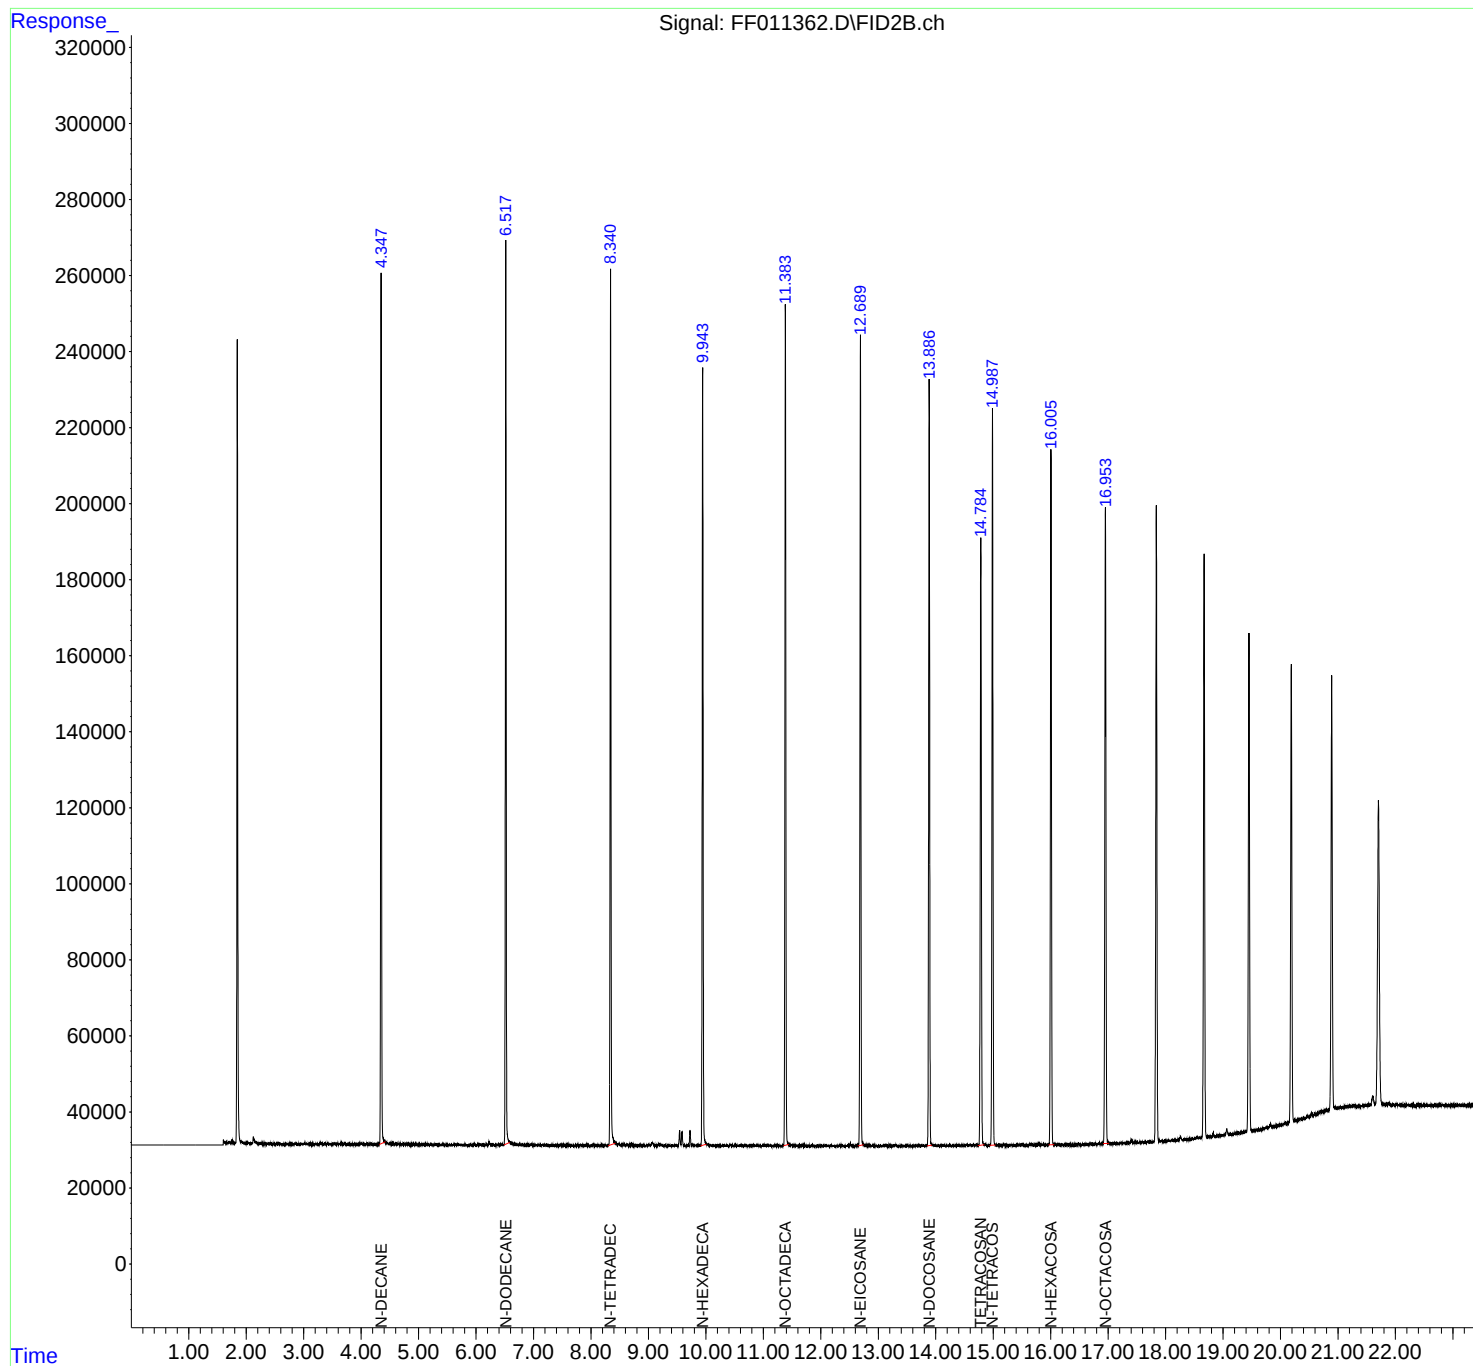


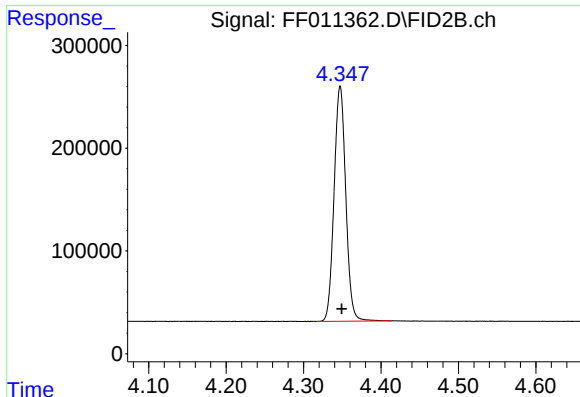

#2 N-DECANE


R.T.: 4.347 min
Delta R.T.: -0.002 min
Response: 2397675
Conc: 18.48 ug/ml

Instrument :
FID_F
ClientSampleId :
PB147448BS

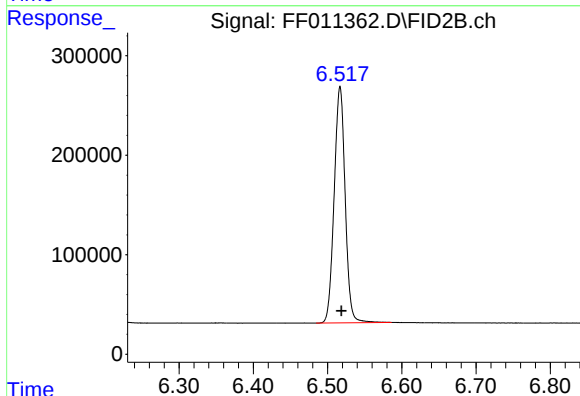


#3 N-DODECANE

R.T.: 6.517 min
Delta R.T.: -0.002 min
Response: 2444374
Conc: 18.67 ug/ml

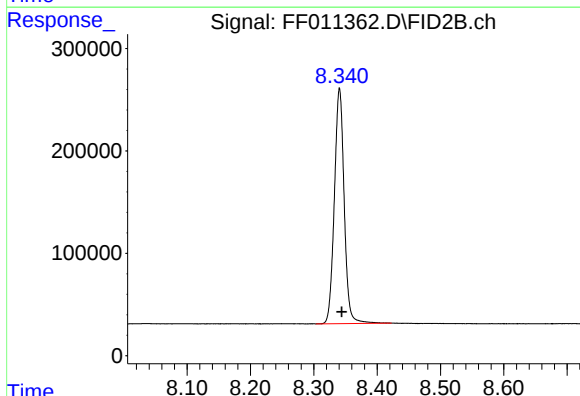


#4 N-TETRADECANE

R.T.: 8.341 min
Delta R.T.: -0.003 min
Response: 2473549
Conc: 18.83 ug/ml

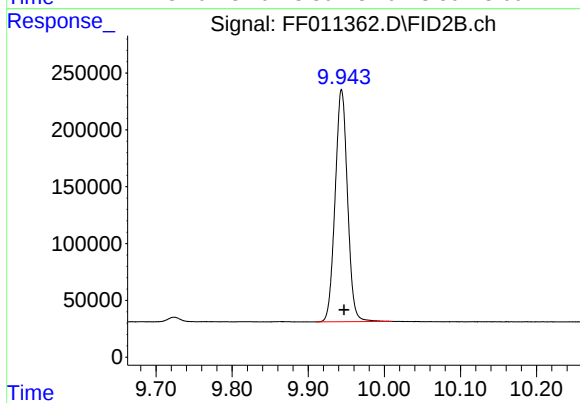

#5 N-HEXADECANE


R.T.: 9.944 min
Delta R.T.: -0.003 min
Response: 2308236
Conc: 17.40 ug/ml

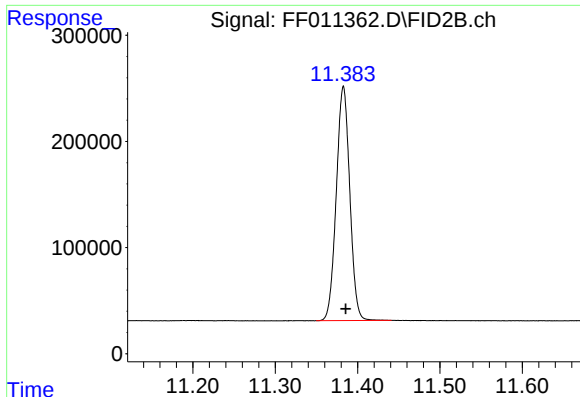

#6 N-OCTADECANE


R.T.: 11.383 min
Delta R.T.: -0.003 min
Response: 2512653
Conc: 18.90 ug/ml

Instrument :
FID_F
ClientSampleId :
PB147448BS

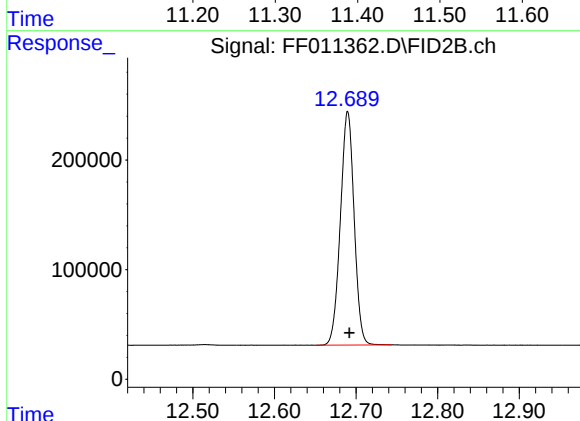


#7 N-EICOSANE

R.T.: 12.690 min
Delta R.T.: -0.002 min
Response: 2494450
Conc: 18.96 ug/ml

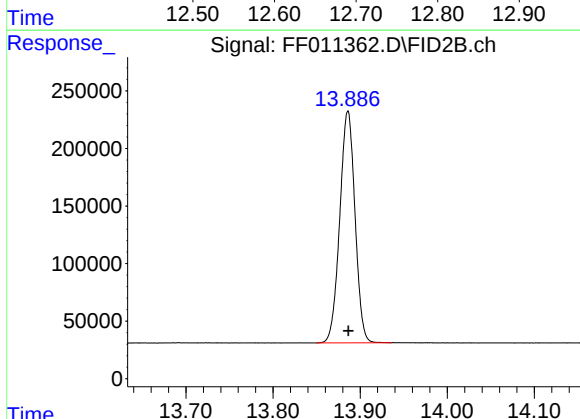


#8 N-DOCOSANE

R.T.: 13.886 min
Delta R.T.: 0.000 min
Response: 2448662
Conc: 19.16 ug/ml

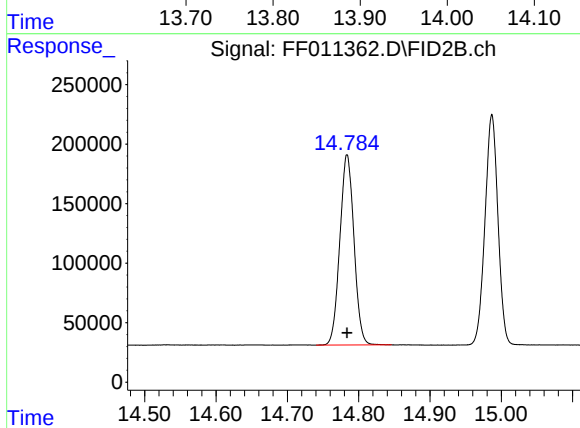

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.784 min
Delta R.T.: 0.000 min
Response: 2202111
Conc: 19.65 ug/ml

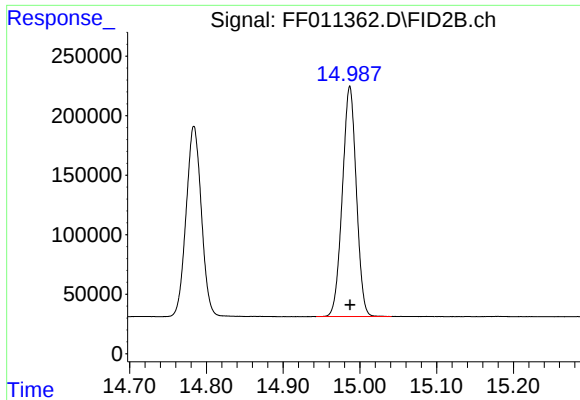

#10 N-TETRACOSANE


R.T.: 14.987 min
Delta R.T.: 0.000 min
Response: 2447171
Conc: 19.22 ug/ml

Instrument :
FID_F
ClientSampleId :
PB147448BS

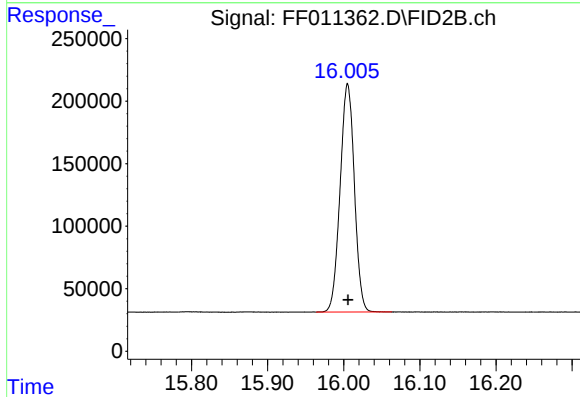

#11 N-HEXACOSANE

R.T.: 16.005 min
Delta R.T.: 0.000 min
Response: 2379099
Conc: 19.05 ug/ml

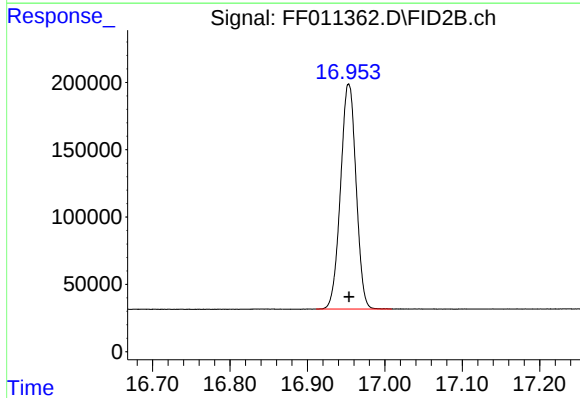

#12 N-OCTACOSANE

R.T.: 16.953 min
Delta R.T.: 0.000 min
Response: 2330727
Conc: 19.03 ug/ml