

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090419\
 Data File : FF005414.D
 Signal(s) : FID2B.ch
 Acq On : 04 Sep 2019 11:58
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 04 15:38:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.672	319401	2.985 ug/ml
Target Compounds			
3) N-DODECANE	6.380	11566102	80.685 ug/ml
8) N-DOCOSANE	13.680f	199476	1.584 ug/ml
10) N-TETRACOSANE	14.834	112871	0.923 ug/ml
11) N-HEXACOSANE	15.859	290994	2.431 ug/ml
12) N-OCTACOSANE	16.820	10622390	89.021 ug/ml
13) N-TRIACONTANE	17.706	1189788	9.836 ug/ml
14) N-DOTRIACONTANE	18.546	1439543	11.613 ug/ml
15) N-TETRATRIACONTANE	19.337	991161	8.225 ug/ml
16) N-HEXATRIACONTANE	20.085	639513	5.328 ug/ml
17) N-OCTATRIACONTANE	20.829	402106	3.686 ug/ml
18) N-TETRACONTANE	21.761	821527	6.462 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090419\
Data File : FF005414.D
Signal(s) : FID2B.ch
Acq On : 04 Sep 2019 11:58
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 04 15:38:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

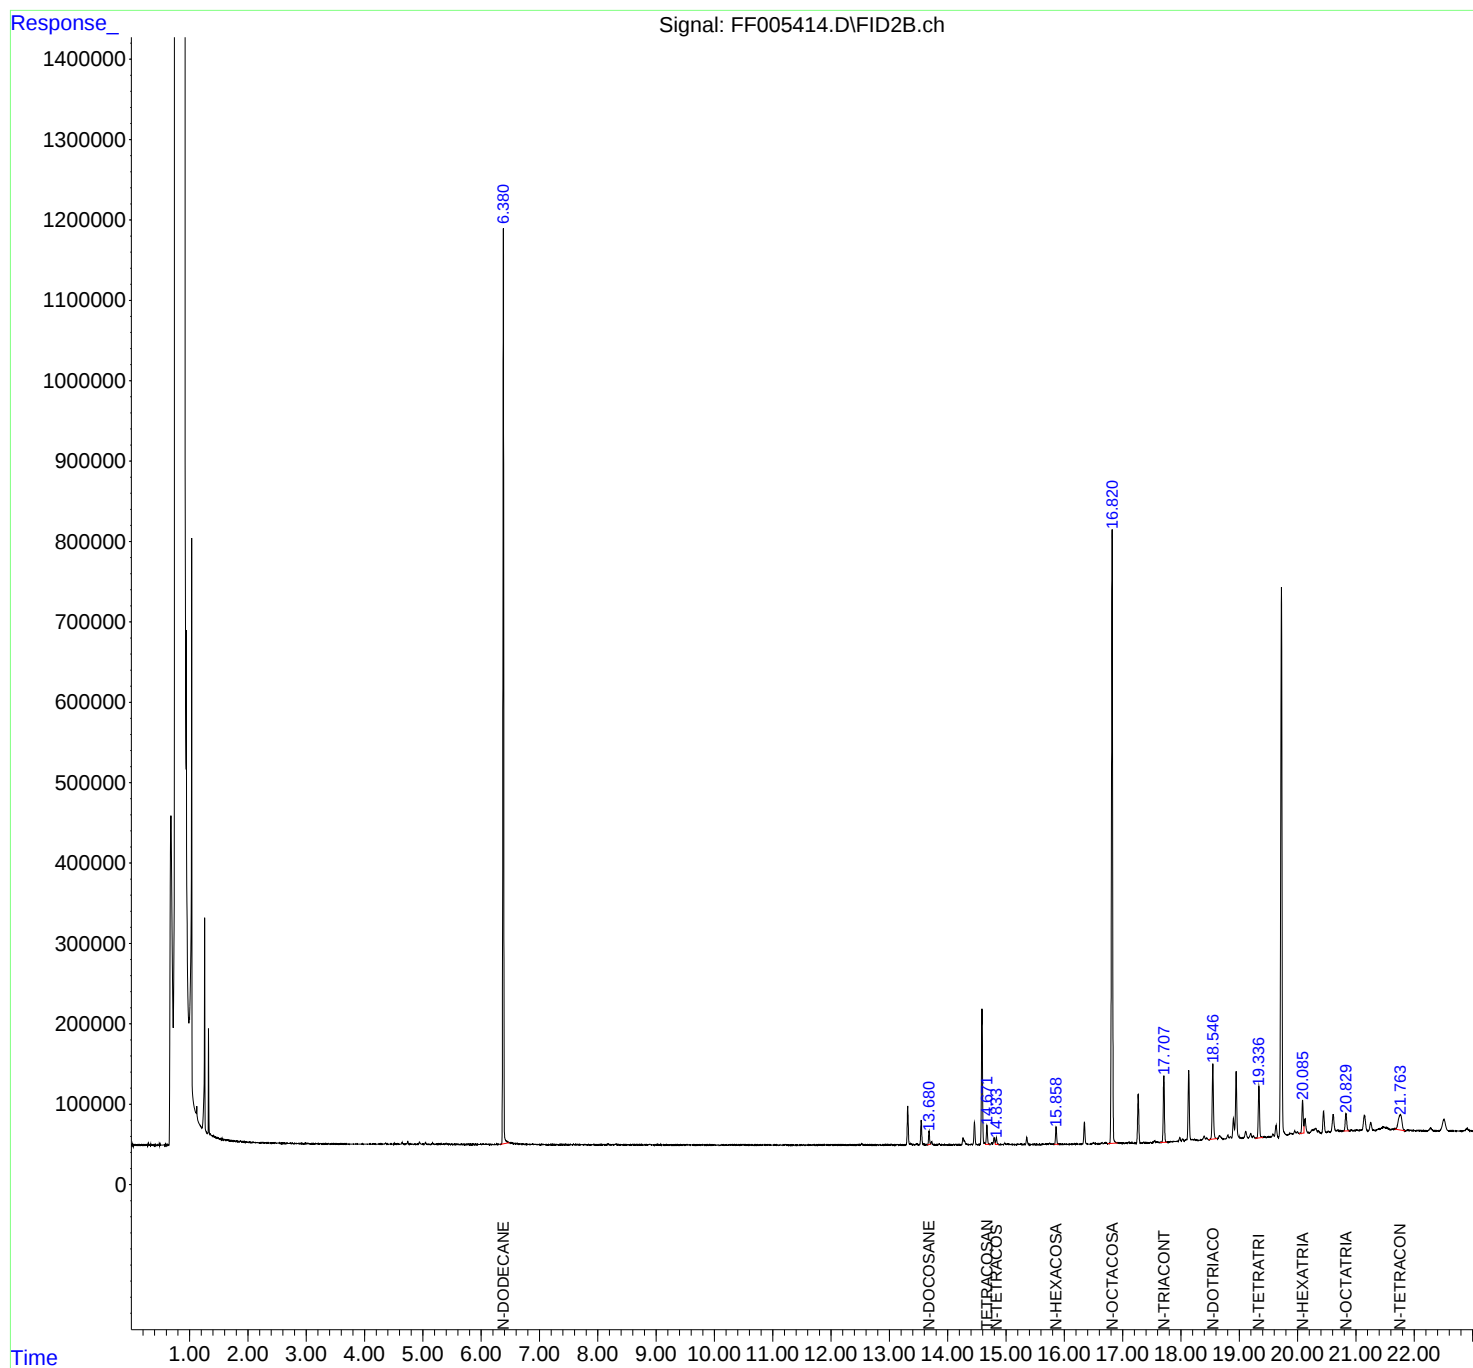

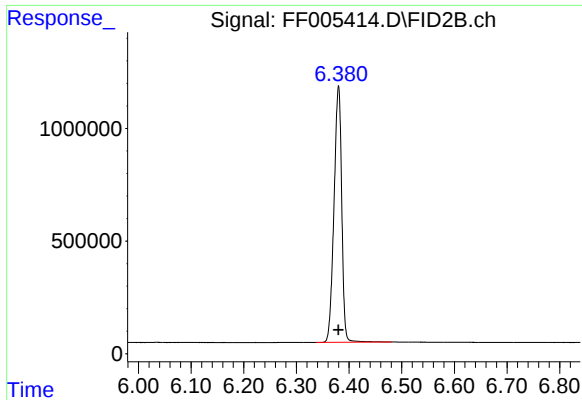


#3 N-DODECANE

R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 11566102
Conc: 80.69 ug/ml

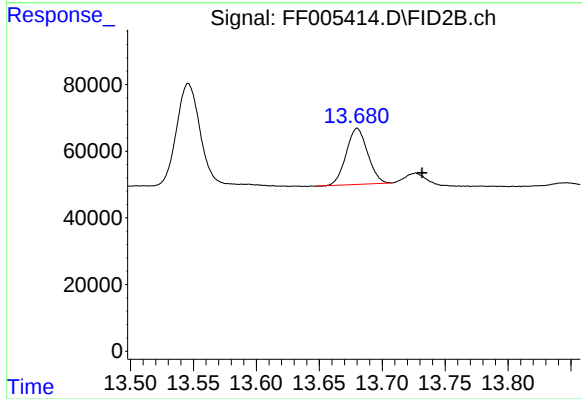


#8 N-DOCOSANE

R.T.: 13.680 min
Delta R.T.: -0.052 min
Response: 199476
Conc: 1.58 ug/ml

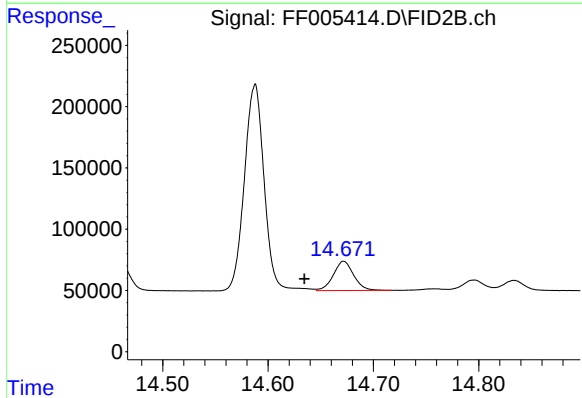


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.672 min
Delta R.T.: 0.037 min
Response: 319401
Conc: 2.98 ug/ml

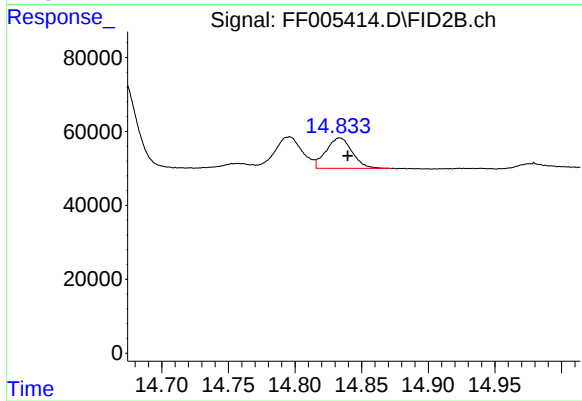


#10 N-TETRACOSANE

R.T.: 14.834 min
Delta R.T.: -0.006 min
Response: 112871
Conc: 0.92 ug/ml

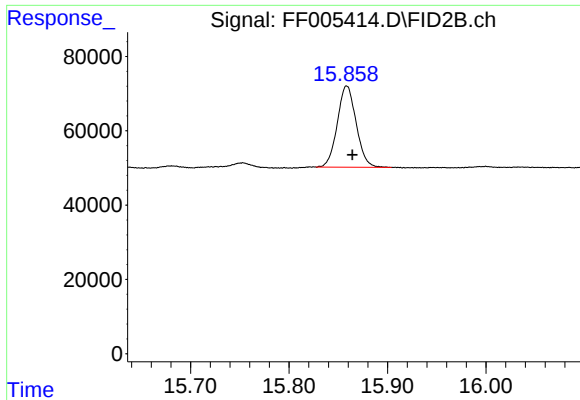


#11 N-HEXACOSANE

R.T.: 15.859 min
Delta R.T.: -0.006 min
Response: 290994
Conc: 2.43 ug/ml

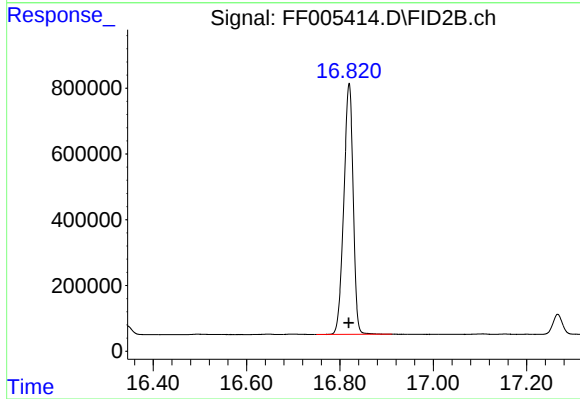


#12 N-OCTACOSANE

R.T.: 16.820 min
Delta R.T.: 0.000 min
Response: 10622390
Conc: 89.02 ug/ml

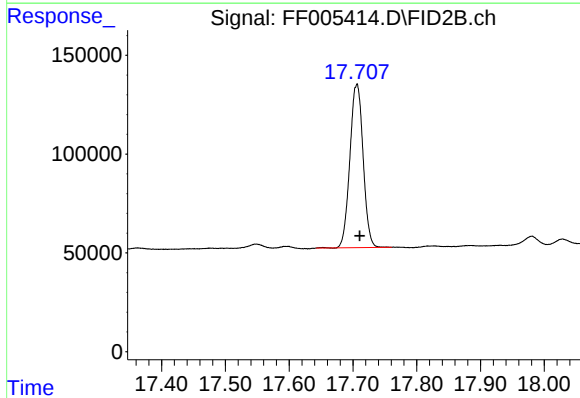


#13 N-TRIACONTANE

R.T.: 17.706 min
Delta R.T.: -0.004 min
Response: 1189788
Conc: 9.84 ug/ml

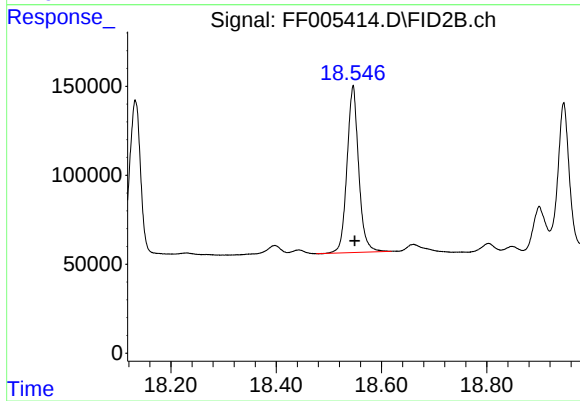


#14 N-DOTRIACONTANE

R.T.: 18.546 min
Delta R.T.: -0.003 min
Response: 1439543
Conc: 11.61 ug/ml

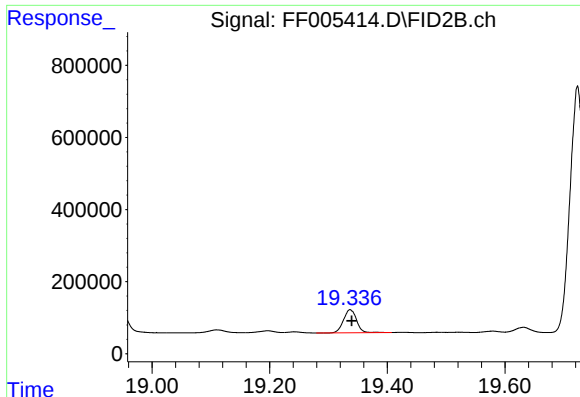


#15 N-TETRATRIACONTANE

R.T.: 19.337 min
Delta R.T.: -0.003 min
Response: 991161
Conc: 8.22 ug/ml

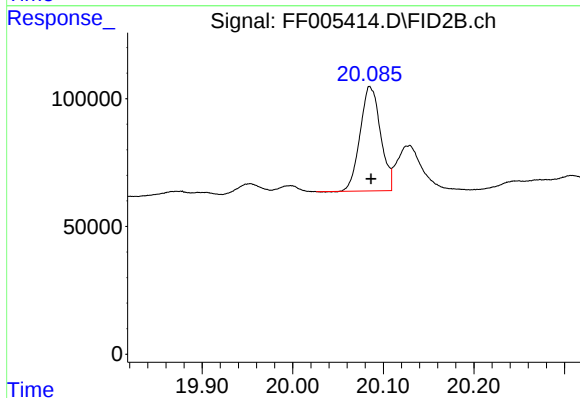


#16 N-HEXATRIACONTANE

R.T.: 20.085 min
Delta R.T.: -0.002 min
Response: 639513
Conc: 5.33 ug/ml

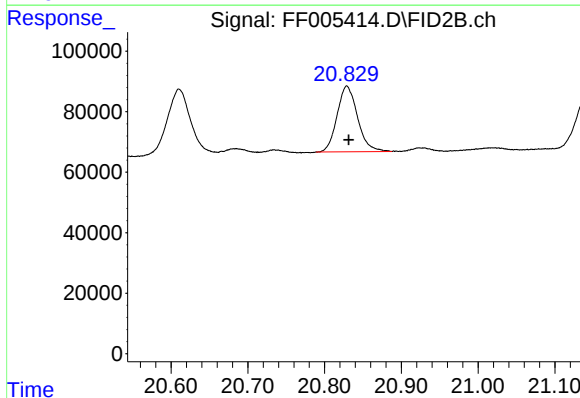

#17 N-OCTATRIACONTANE

R.T.: 20.829 min
Delta R.T.: -0.003 min
Response: 402106
Conc: 3.69 ug/ml

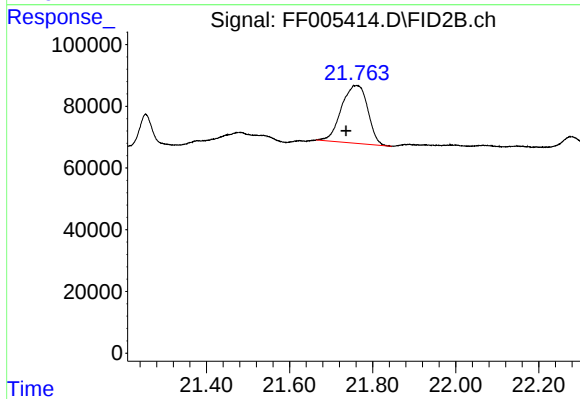

#18 N-TETRACONTANE

R.T.: 21.761 min
Delta R.T.: 0.025 min
Response: 821527
Conc: 6.46 ug/ml