

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090420\
 Data File : FF007464.D
 Signal(s) : FID2B.ch
 Acq On : 04 Sep 2020 12:17
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 05 01:31:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
3) N-DODECANE	6.479	4115589	25.298	ug/ml
12) N-OCTACOSANE	16.918	3685955	24.018	ug/ml
13) N-TRIACONTANE	17.805	130634	0.884	ug/ml
14) N-DOTRIACONTANE	18.641	167353	1.206	ug/ml
15) N-TETRATRIACONTANE	19.429	114122	0.904	ug/ml
16) N-HEXATRIACONTANE	20.215	150515	1.259	ug/ml
18) N-TETRACONTANE	21.920	301763	2.720	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090420\
Data File : FF007464.D
Signal(s) : FID2B.ch
Acq On : 04 Sep 2020 12:17
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 01:31:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

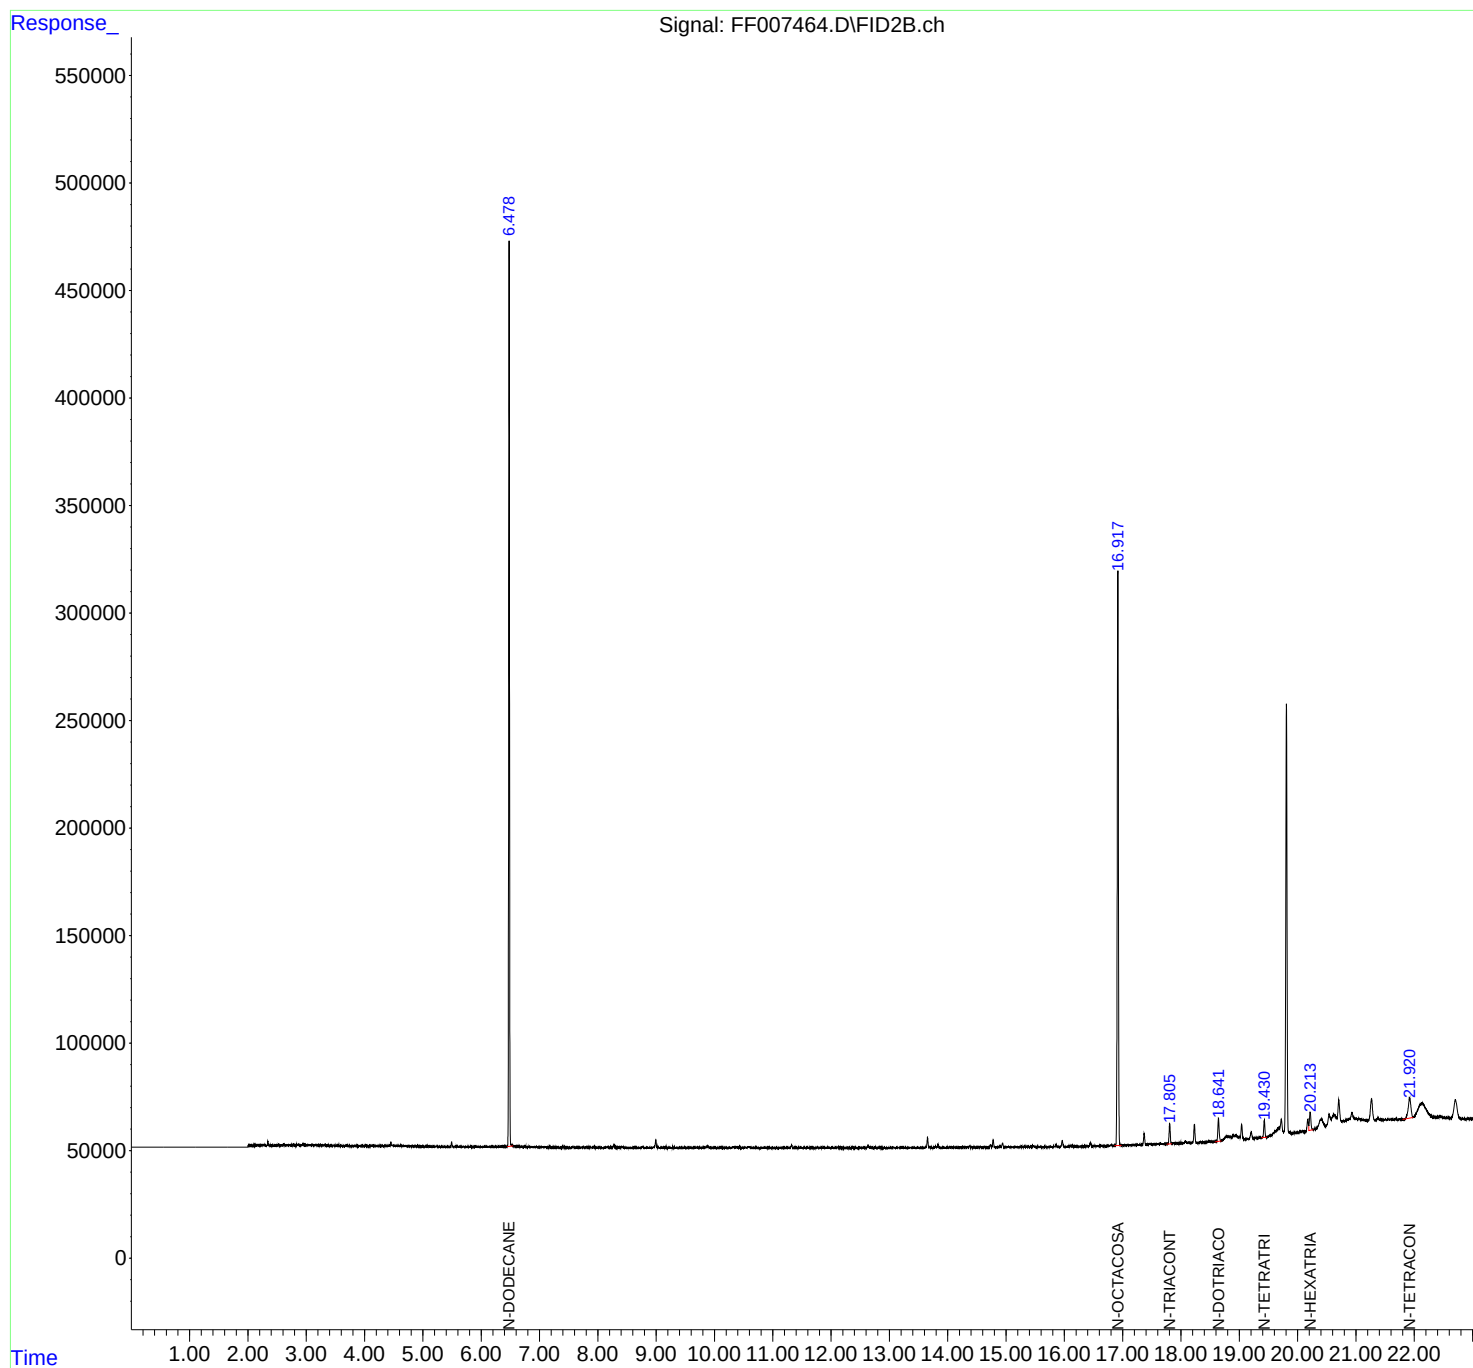


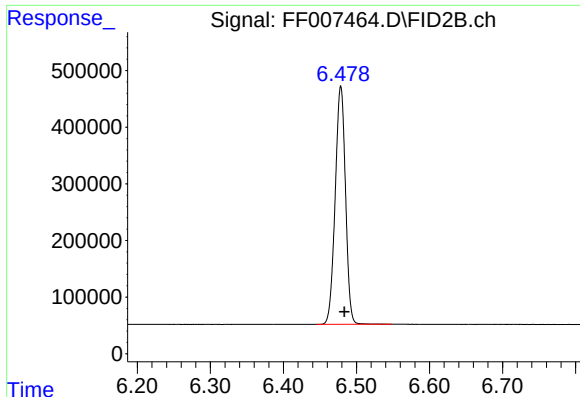

#3 N-DODECANE


R.T.: 6.479 min
Delta R.T.: -0.005 min
Response: 4115589
Conc: 25.30 ug/ml

Instrument :
FID_F
ClientSampleId :

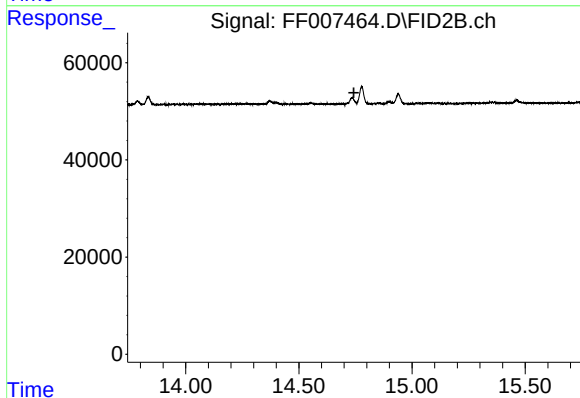


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.743 min
Response: 0
Conc: N.D.

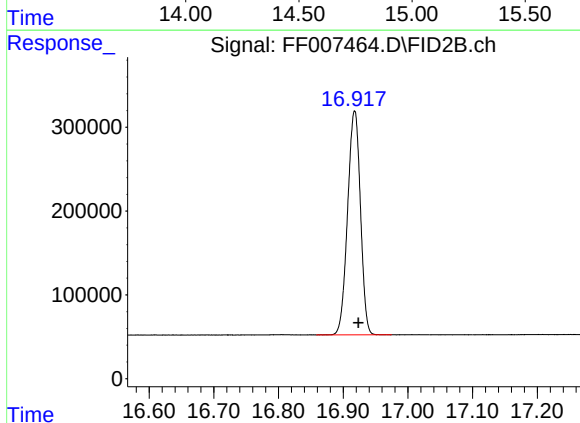


#12 N-OCTACOSANE

R.T.: 16.918 min
Delta R.T.: -0.006 min
Response: 3685955
Conc: 24.02 ug/ml

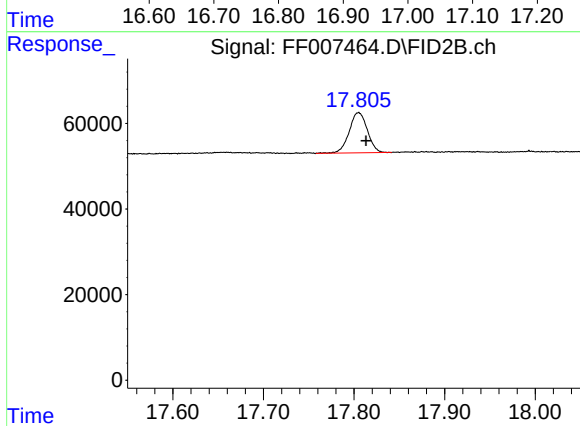

#13 N-TRIACONTANE


R.T.: 17.805 min
Delta R.T.: -0.008 min
Response: 130634
Conc: 0.88 ug/ml

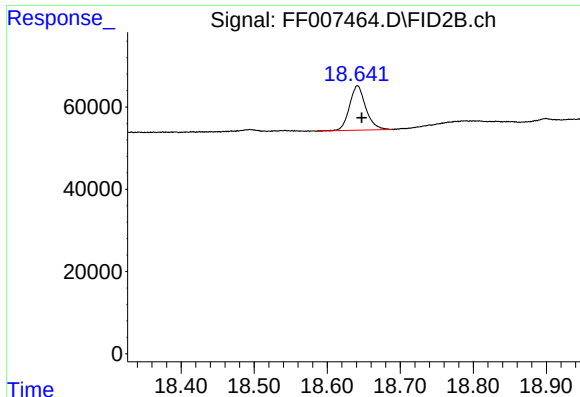

#14 N-DOTRIACONTANE


R.T.: 18.641 min
Delta R.T.: -0.006 min
Response: 167353
Conc: 1.21 ug/ml

Instrument :
FID_F
ClientSampleId :

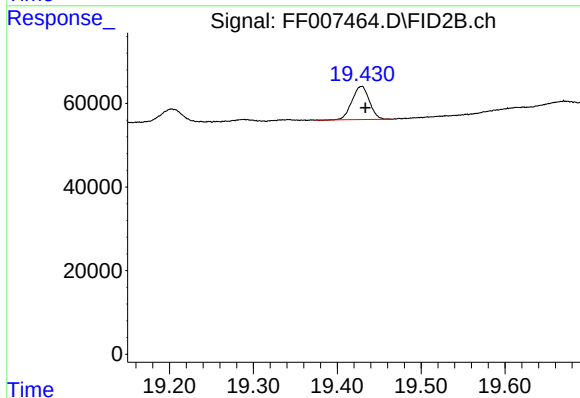


#15 N-TETRATRIACONTANE

R.T.: 19.429 min
Delta R.T.: -0.005 min
Response: 114122
Conc: 0.90 ug/ml

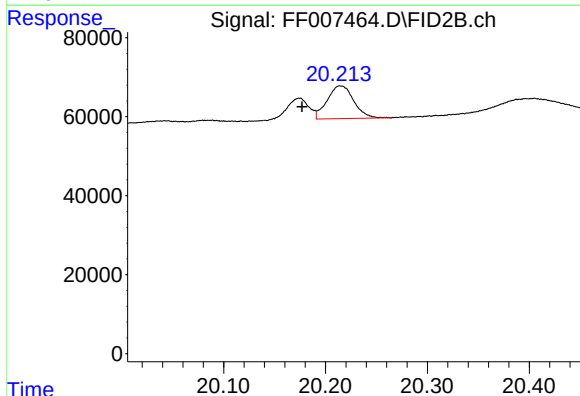

#16 N-HEXATRIACONTANE

R.T.: 20.215 min
Delta R.T.: 0.038 min
Response: 150515
Conc: 1.26 ug/ml

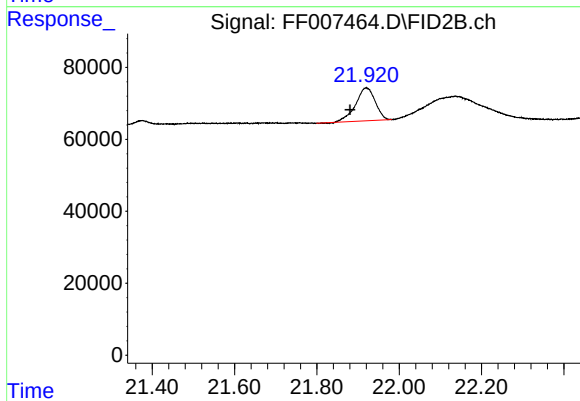

#18 N-TETRACONTANE

R.T.: 21.920 min
Delta R.T.: 0.039 min
Response: 301763
Conc: 2.72 ug/ml