

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090420\
 Data File : FF007467.D
 Signal(s) : FID2B.ch
 Acq On : 04 Sep 2020 13:50
 Operator : DD\AJ
 Sample : L3912-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 05 01:31:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.743	47408512	322.343 ug/ml
Target Compounds			
5) N-HEXADECANE	9.877	380003	2.252 ug/ml
6) N-OCTADECANE	11.323	1771640	10.397 ug/ml
7) N-EICOSANE	12.642	9455460	56.240 ug/ml
8) N-DOCOSANE	13.890	72492700	439.992 ug/ml
10) N-TETRACOSANE	14.931	121877143	747.265 ug/ml
11) N-HEXACOSANE	15.985	89666932	567.229 ug/ml
12) N-OCTACOSANE	16.877	189194232	1232.805 ug/ml
13) N-TRIACONTANE	17.821	157976927	1068.846 ug/ml
14) N-DOTRIACONTANE	18.609	201700833	1453.628 ug/ml
15) N-TETRATRIACONTANE	19.426	49677313	393.642 ug/ml
16) N-HEXATRIACONTANE	20.171	40250304	336.811 ug/ml
17) N-OCTATRIACONTANE	20.937	26599104	249.095 ug/ml
18) N-TETRACONTANE	21.860	1375737	12.400 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090420\
Data File : FF007467.D
Signal(s) : FID2B.ch
Acq On : 04 Sep 2020 13:50
Operator : DD\AJ
Sample : L3912-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 01:31:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

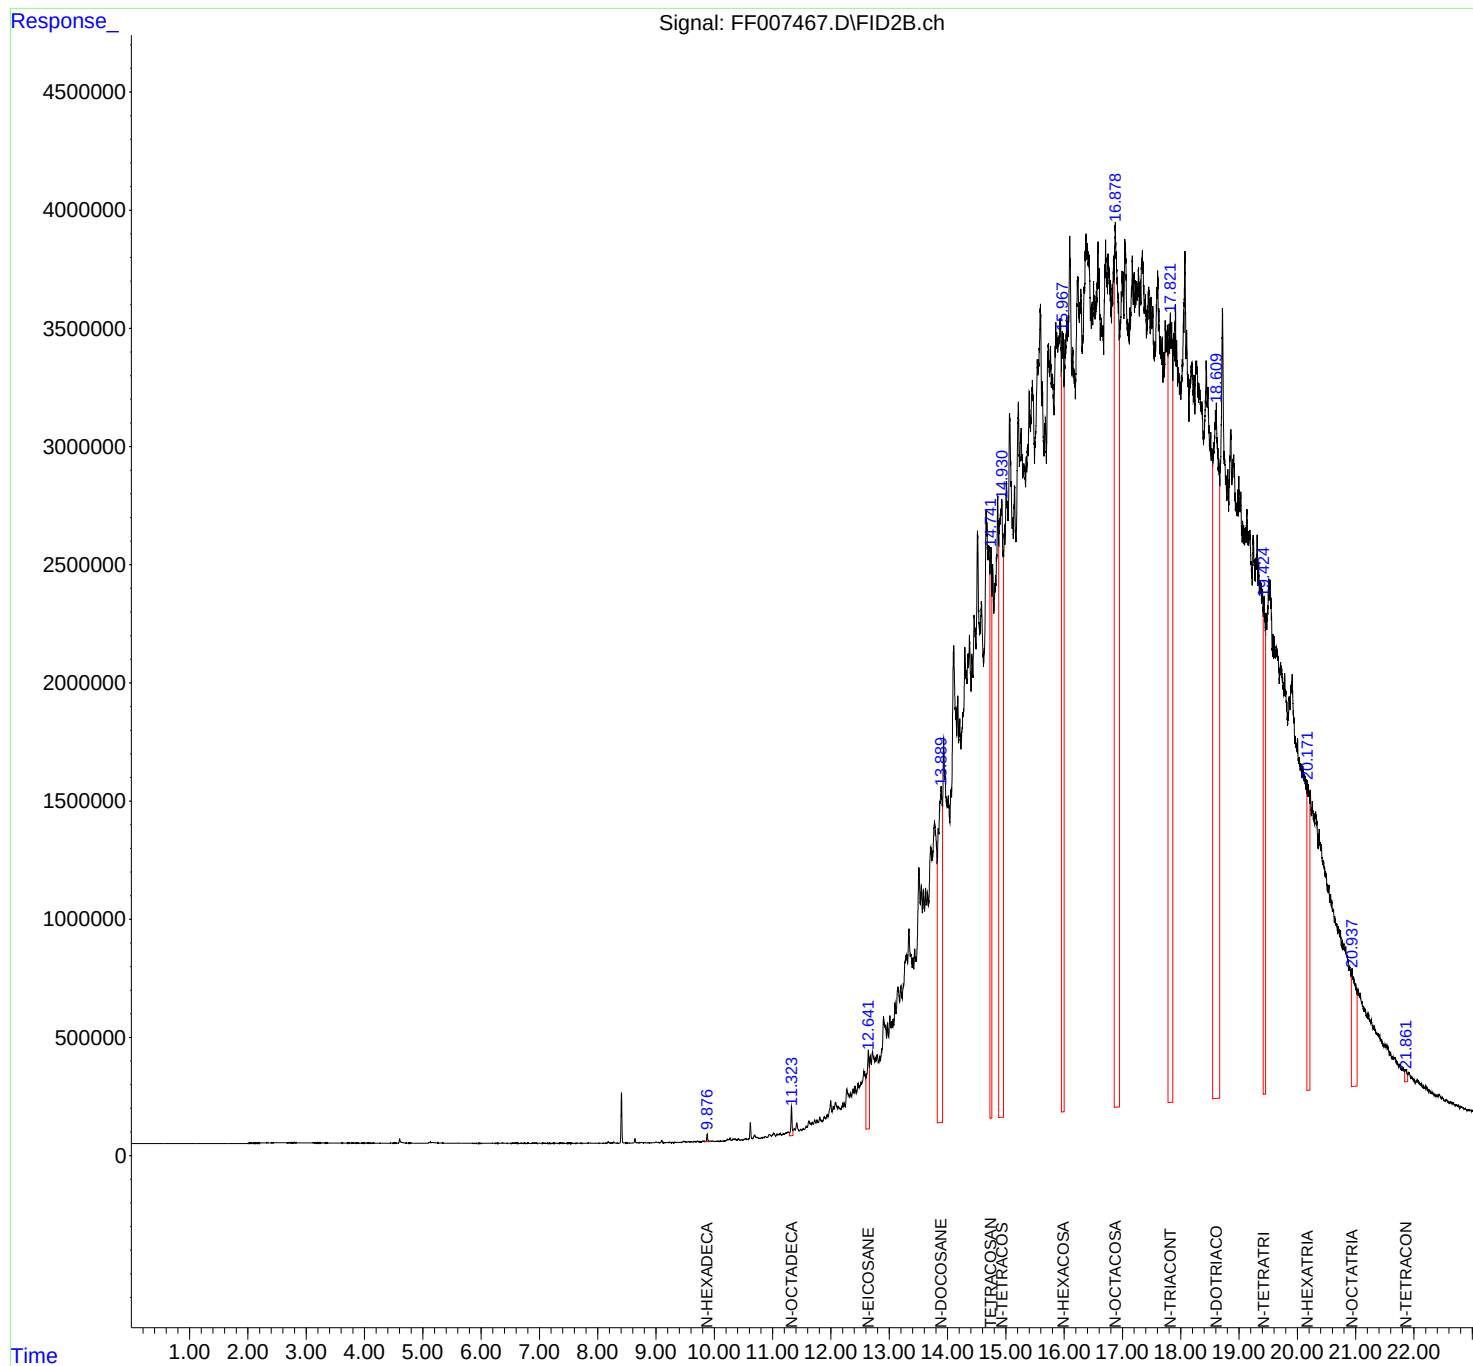


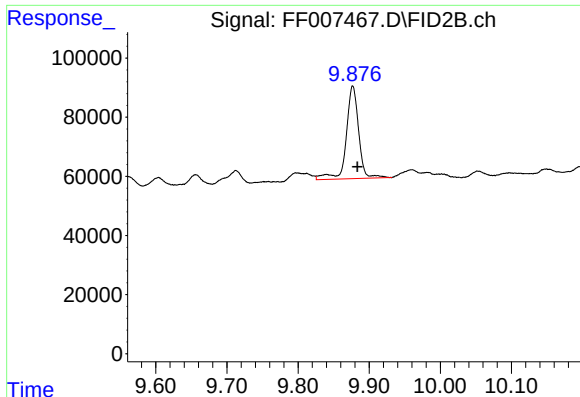

#5 N-HEXADECANE


R.T.: 9.877 min
Delta R.T.: -0.006 min
Response: 380003
Conc: 2.25 ug/ml

Instrument :
FID_F
ClientSampleId :

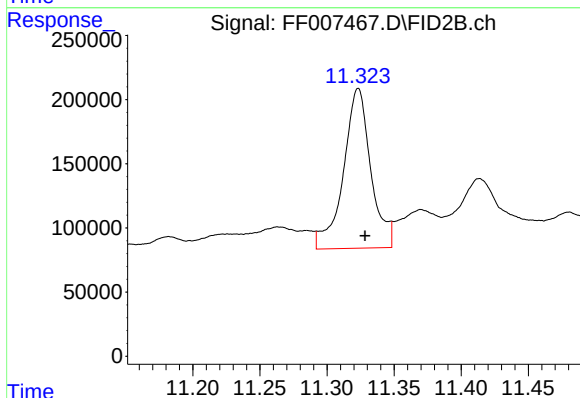


#6 N-OCTADECANE

R.T.: 11.323 min
Delta R.T.: -0.005 min
Response: 1771640
Conc: 10.40 ug/ml

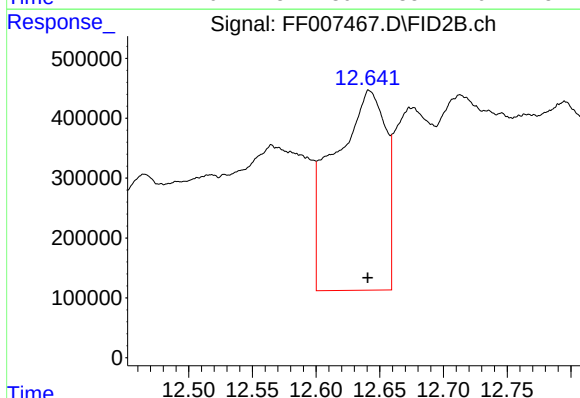


#7 N-EICOSANE

R.T.: 12.642 min
Delta R.T.: 0.002 min
Response: 9455460
Conc: 56.24 ug/ml

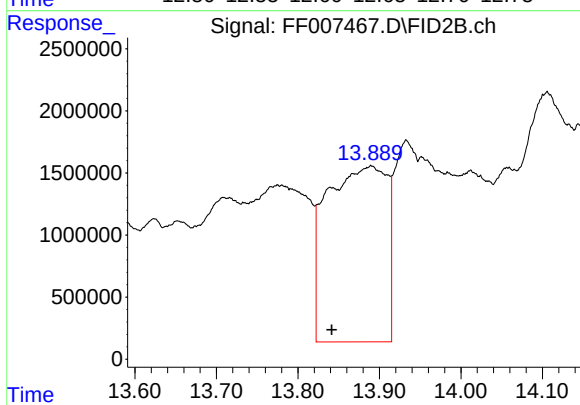

#8 N-DOCOSANE


R.T.: 13.890 min
Delta R.T.: 0.048 min
Response: 72492700
Conc: 439.99 ug/ml

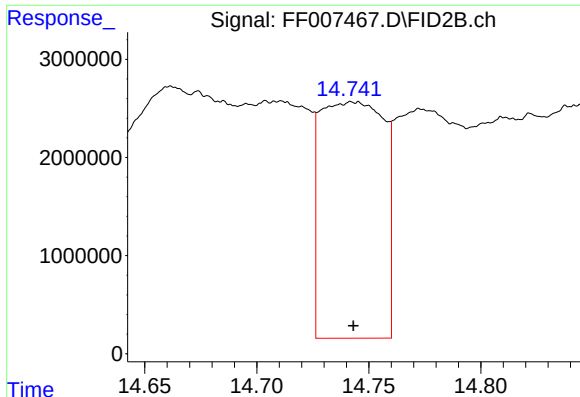

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.743 min
Delta R.T.: 0.000 min
Response: 47408512
Conc: 322.34 ug/ml

Instrument :
FID_F
ClientSampleId :

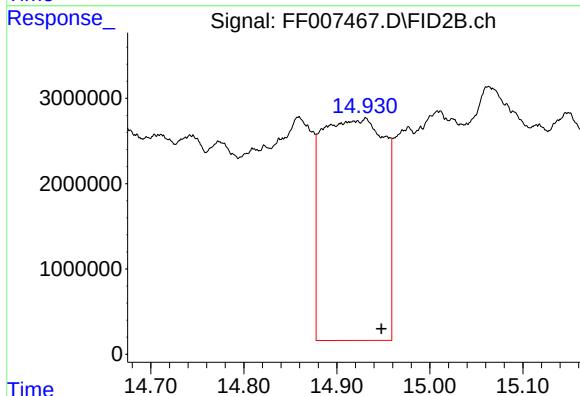


#10 N-TETRACOSANE

R.T.: 14.931 min
Delta R.T.: -0.017 min
Response: 121877143
Conc: 747.27 ug/ml

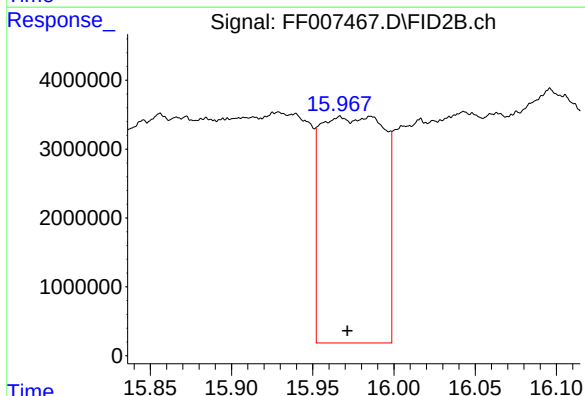


#11 N-HEXACOSANE

R.T.: 15.985 min
Delta R.T.: 0.013 min
Response: 89666932
Conc: 567.23 ug/ml

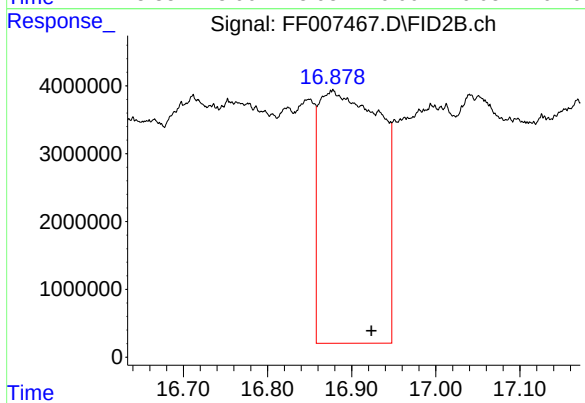

#12 N-OCTACOSANE


R.T.: 16.877 min
Delta R.T.: -0.046 min
Response: 189194232
Conc: 1232.81 ug/ml

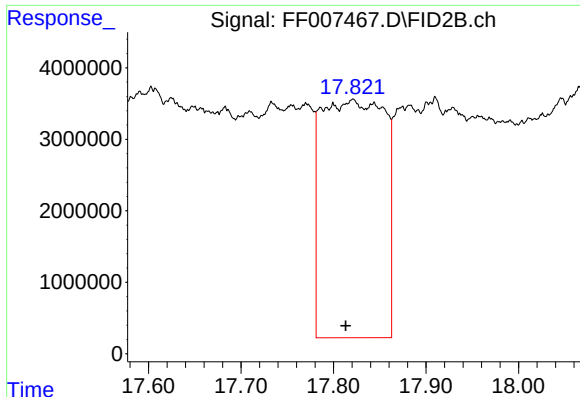

#13 N-TRIACONTANE


R.T.: 17.821 min
Delta R.T.: 0.007 min
Response: 157976927
Conc: 1068.85 ug/ml

Instrument :
FID_F
ClientSampleId :

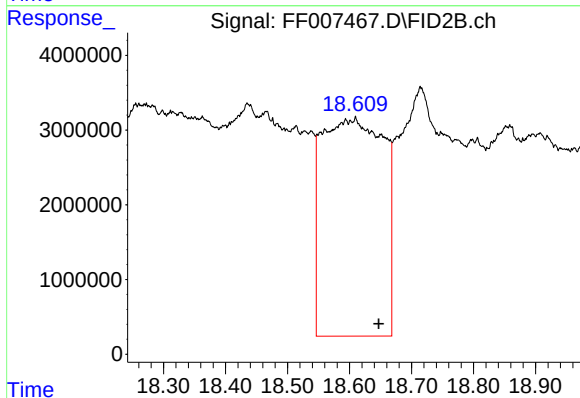


#14 N-DOTRIACONTANE

R.T.: 18.609 min
Delta R.T.: -0.038 min
Response: 201700833
Conc: 1453.63 ug/ml

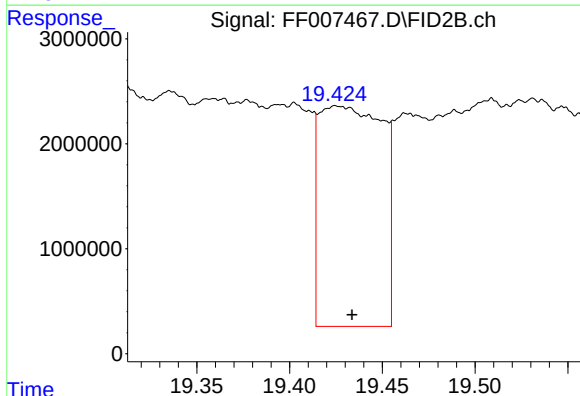


#15 N-TETRATRIACONTANE

R.T.: 19.426 min
Delta R.T.: -0.007 min
Response: 49677313
Conc: 393.64 ug/ml

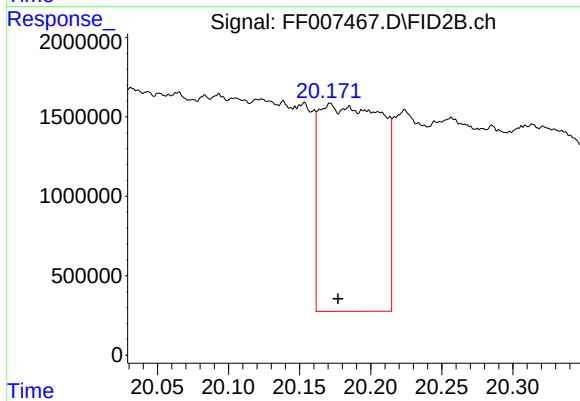

#16 N-HEXATRIACONTANE


R.T.: 20.171 min
Delta R.T.: -0.006 min
Response: 40250304
Conc: 336.81 ug/ml

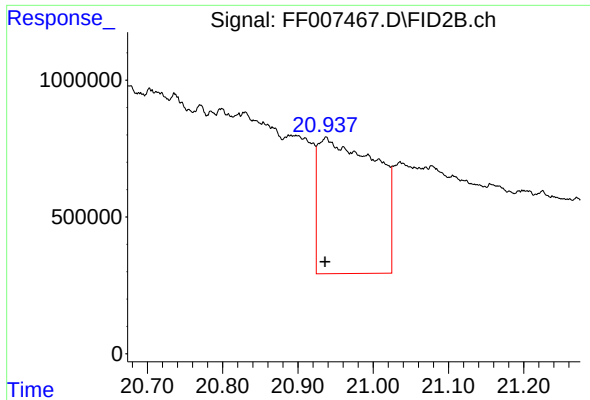

#17 N-OCTATRIACONTANE

R.T.: 20.937 min
Delta R.T.: 0.001 min
Response: 26599104
Conc: 249.10 ug/ml

Instrument :
FID_F
ClientSampleId :

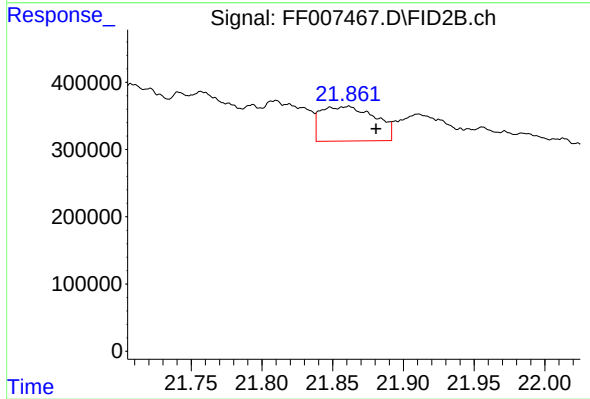

#18 N-TETRACONTANE

R.T.: 21.860 min
Delta R.T.: -0.020 min
Response: 1375737
Conc: 12.40 ug/ml