

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090420\
Data File : FF007468.D
Signal(s) : FID2B.ch
Acq On : 04 Sep 2020 14:29
Operator : DD\AJ
Sample : L3912-02 200X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 01:32:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.813	607716	4.112 ug/ml
14) N-DOTRIACONTANE	18.643	144821	1.044 ug/ml
16) N-HEXATRIACONTANE	20.150	616173	5.156 ug/ml
17) N-OCTATRIACONTANE	20.874f	2119883	19.852 ug/ml
18) N-TETRACONTANE	21.910	351797	3.171 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090420\
Data File : FF007468.D
Signal(s) : FID2B.ch
Acq On : 04 Sep 2020 14:29
Operator : DD\AJ
Sample : L3912-02 200X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 05 01:32:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

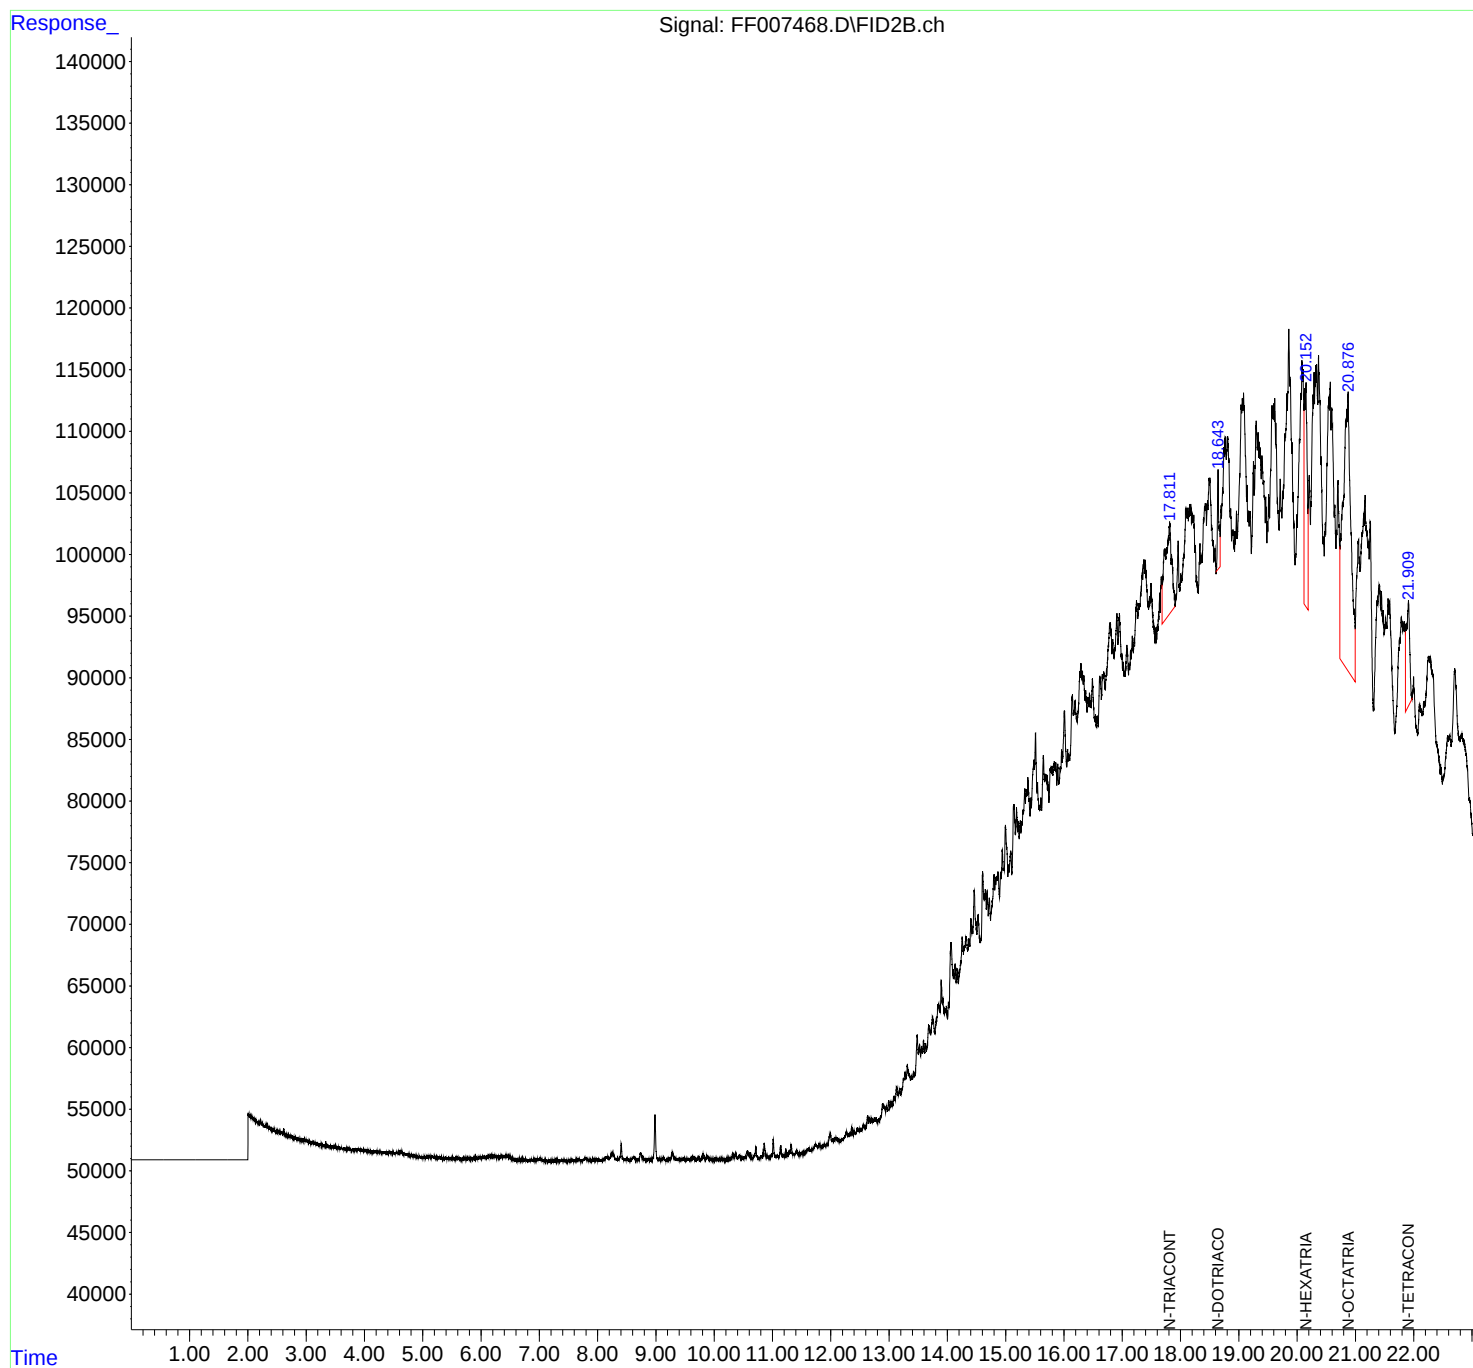


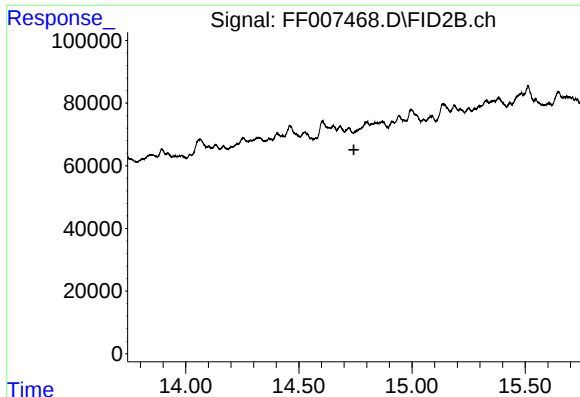

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.743 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

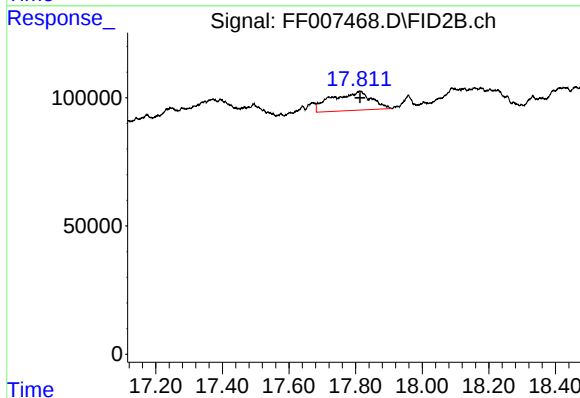


#13 N-TRIACONTANE

R.T.: 17.813 min
Delta R.T.: 0.000 min
Response: 607716
Conc: 4.11 ug/ml

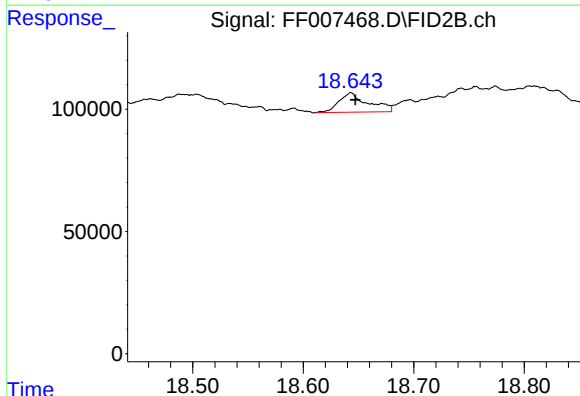


#14 N-DOTRIACONTANE

R.T.: 18.643 min
Delta R.T.: -0.004 min
Response: 144821
Conc: 1.04 ug/ml

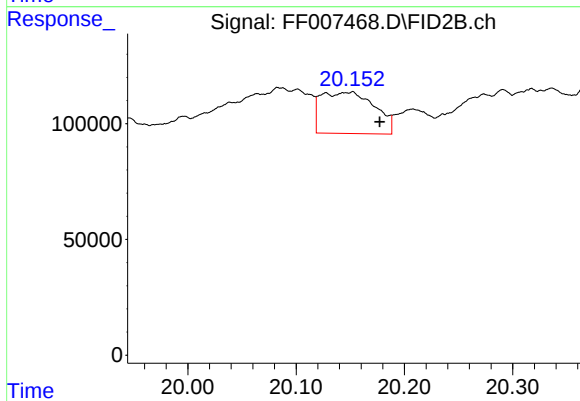

#16 N-HEXATRIACONTANE


R.T.: 20.150 min
Delta R.T.: -0.027 min
Response: 616173
Conc: 5.16 ug/ml

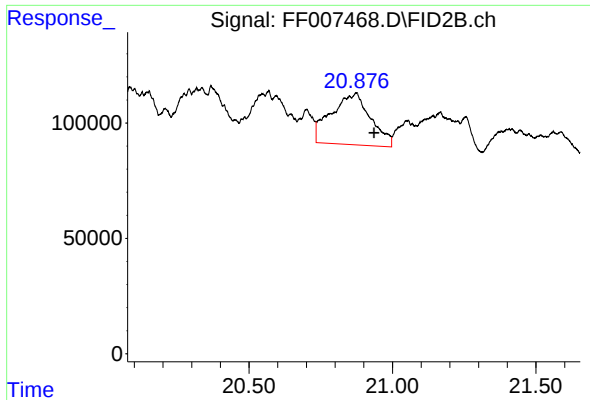

#17 N-OCTATRIACONTANE

R.T.: 20.874 min
Delta R.T.: -0.062 min
Response: 2119883
Conc: 19.85 ug/ml

Instrument :
FID_F
ClientSampleId :

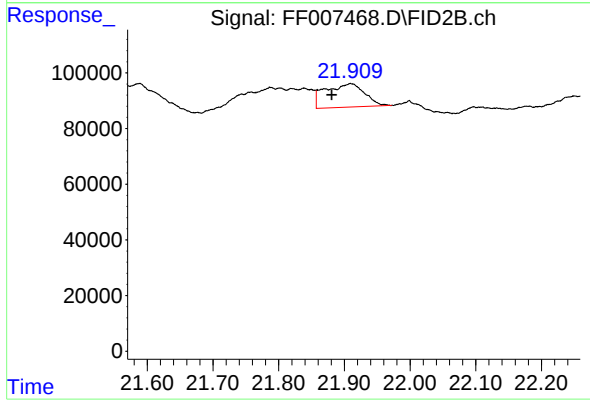

#18 N-TETRACONTANE

R.T.: 21.910 min
Delta R.T.: 0.029 min
Response: 351797
Conc: 3.17 ug/ml