

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090420\
Data File : FF007469.D
Signal(s) : FID2B.ch
Acq On : 04 Sep 2020 15:34
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 01:32:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	2323461	15.798 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.804	104485	0.707 ug/ml
14) N-DOTRIACONTANE	18.641	138037	0.995 ug/ml
16) N-HEXATRIACONTANE	20.209	179420	1.501 ug/ml
18) N-TETRACONTANE	21.914	305962	2.758 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090420\
Data File : FF007469.D
Signal(s) : FID2B.ch
Acq On : 04 Sep 2020 15:34
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 01:32:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

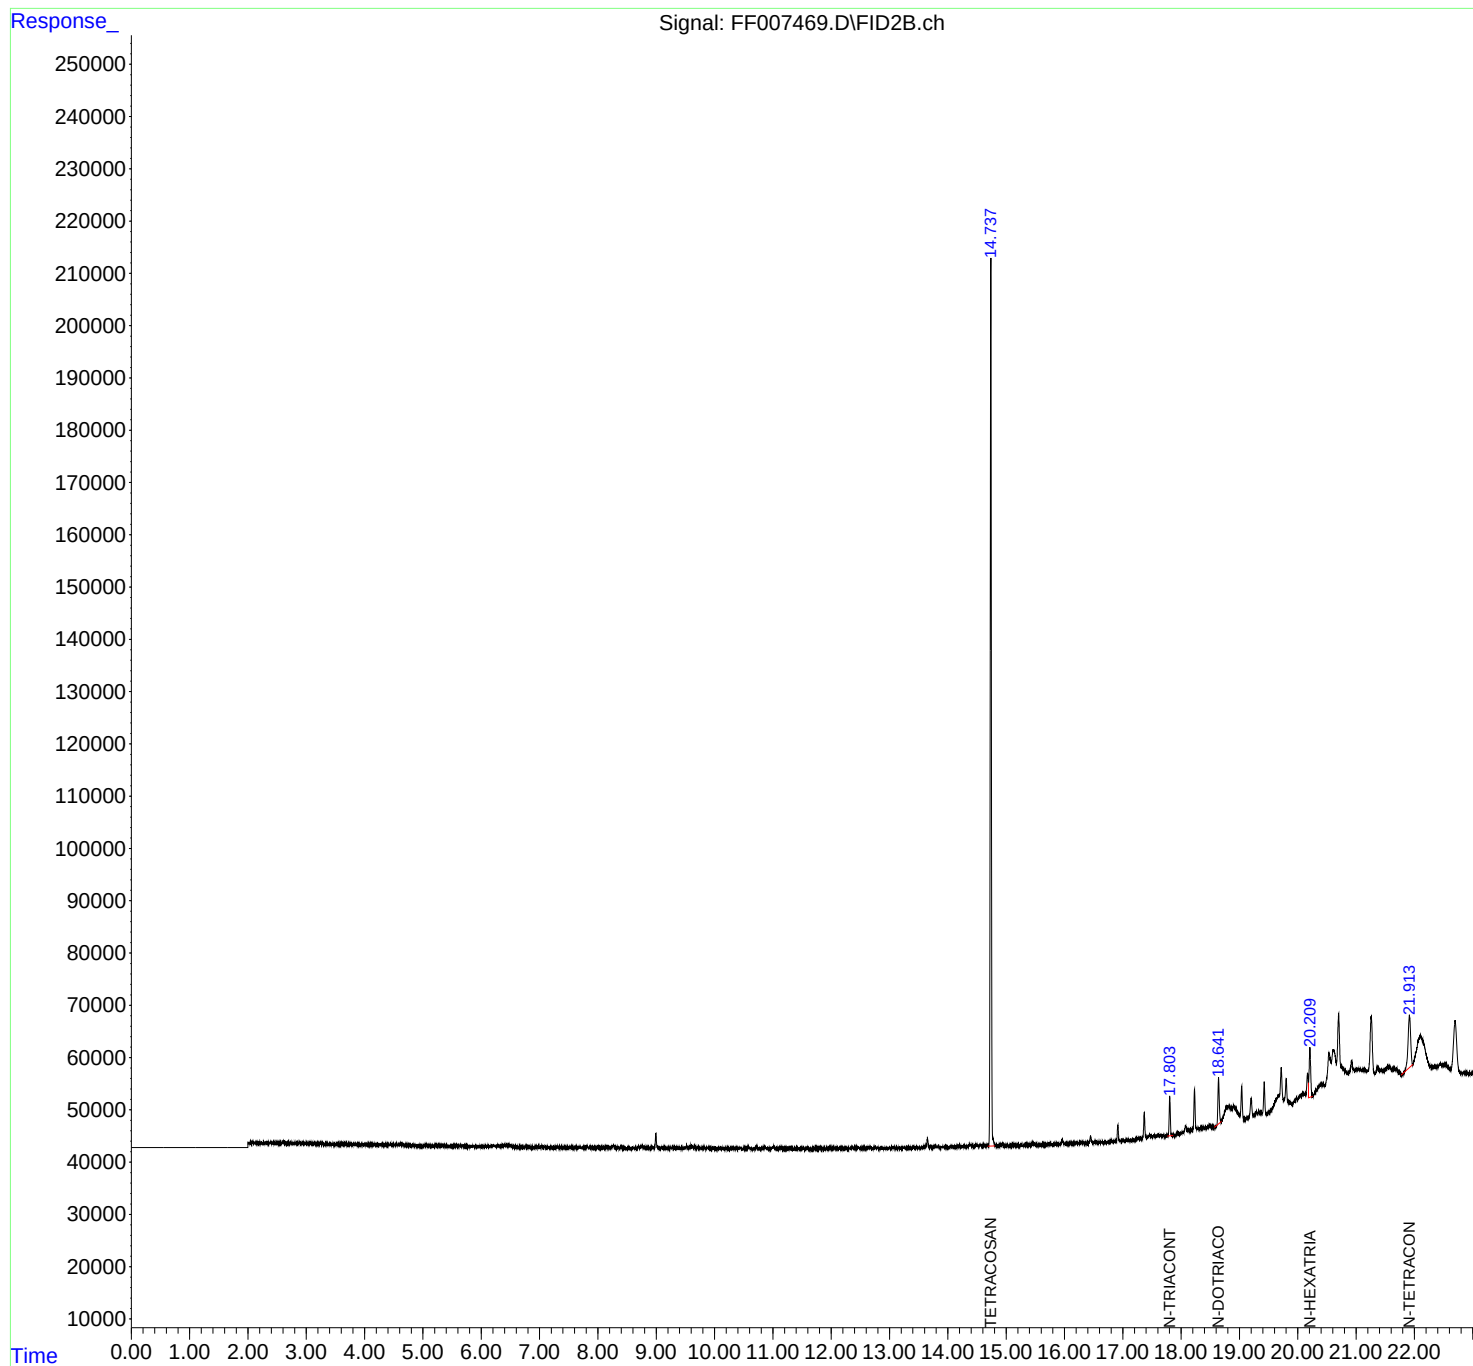


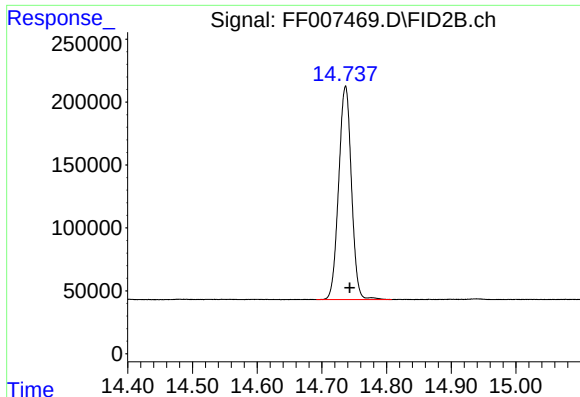

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.736 min
Delta R.T.: -0.007 min
Response: 2323461
Conc: 15.80 ug/ml

Instrument :
FID_F
ClientSampleId :

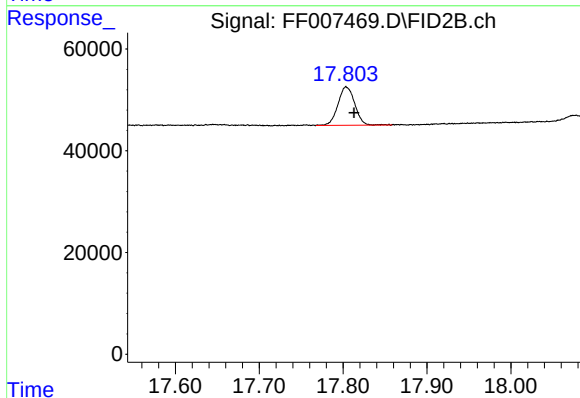


#13 N-TRIACONTANE

R.T.: 17.804 min
Delta R.T.: -0.009 min
Response: 104485
Conc: 0.71 ug/ml

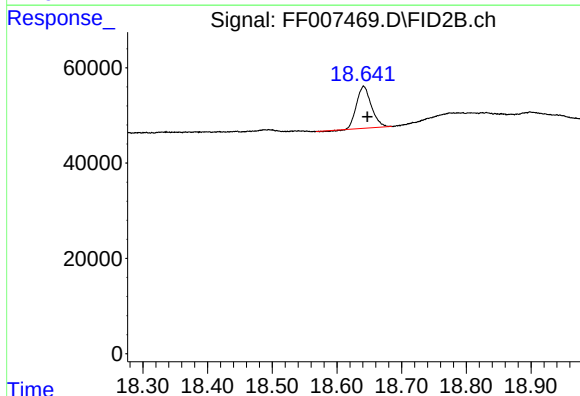


#14 N-DOTRIACONTANE

R.T.: 18.641 min
Delta R.T.: -0.006 min
Response: 138037
Conc: 0.99 ug/ml

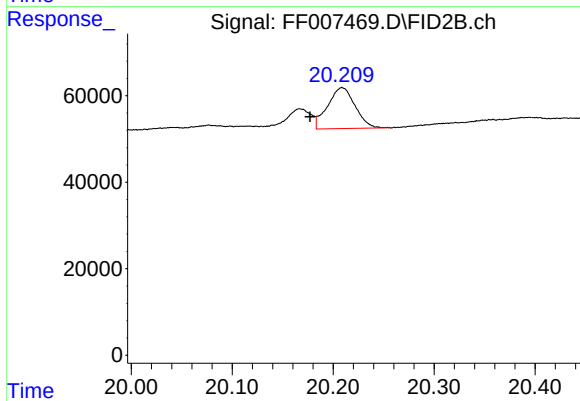

#16 N-HEXATRIACONTANE

R.T.: 20.209 min
Delta R.T.: 0.032 min
Response: 179420
Conc: 1.50 ug/ml

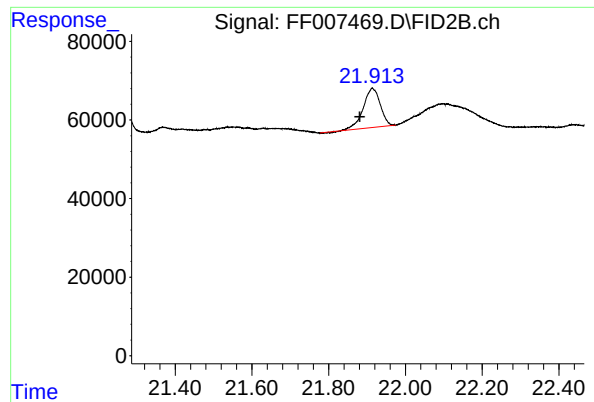

#18 N-TETRACONTANE

R.T.: 21.914 min
Delta R.T.: 0.033 min
Response: 305962
Conc: 2.76 ug/ml

Instrument :
FID_F
ClientSampleId :