

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
 Data File : FF005420.D
 Signal(s) : FID2B.ch
 Acq On : 05 Sep 2019 10:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 06 01:12:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	2360379	22.058 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.708	95195	0.787 ug/ml
14) N-DOTRIACONTANE	18.553	283024	2.283 ug/ml
16) N-HEXATRIACONTANE	20.125	715030	5.957 ug/ml
18) N-TETRACONTANE	21.764	2030075	15.968 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
Data File : FF005420.D
Signal(s) : FID2B.ch
Acq On : 05 Sep 2019 10:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 06 01:12:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

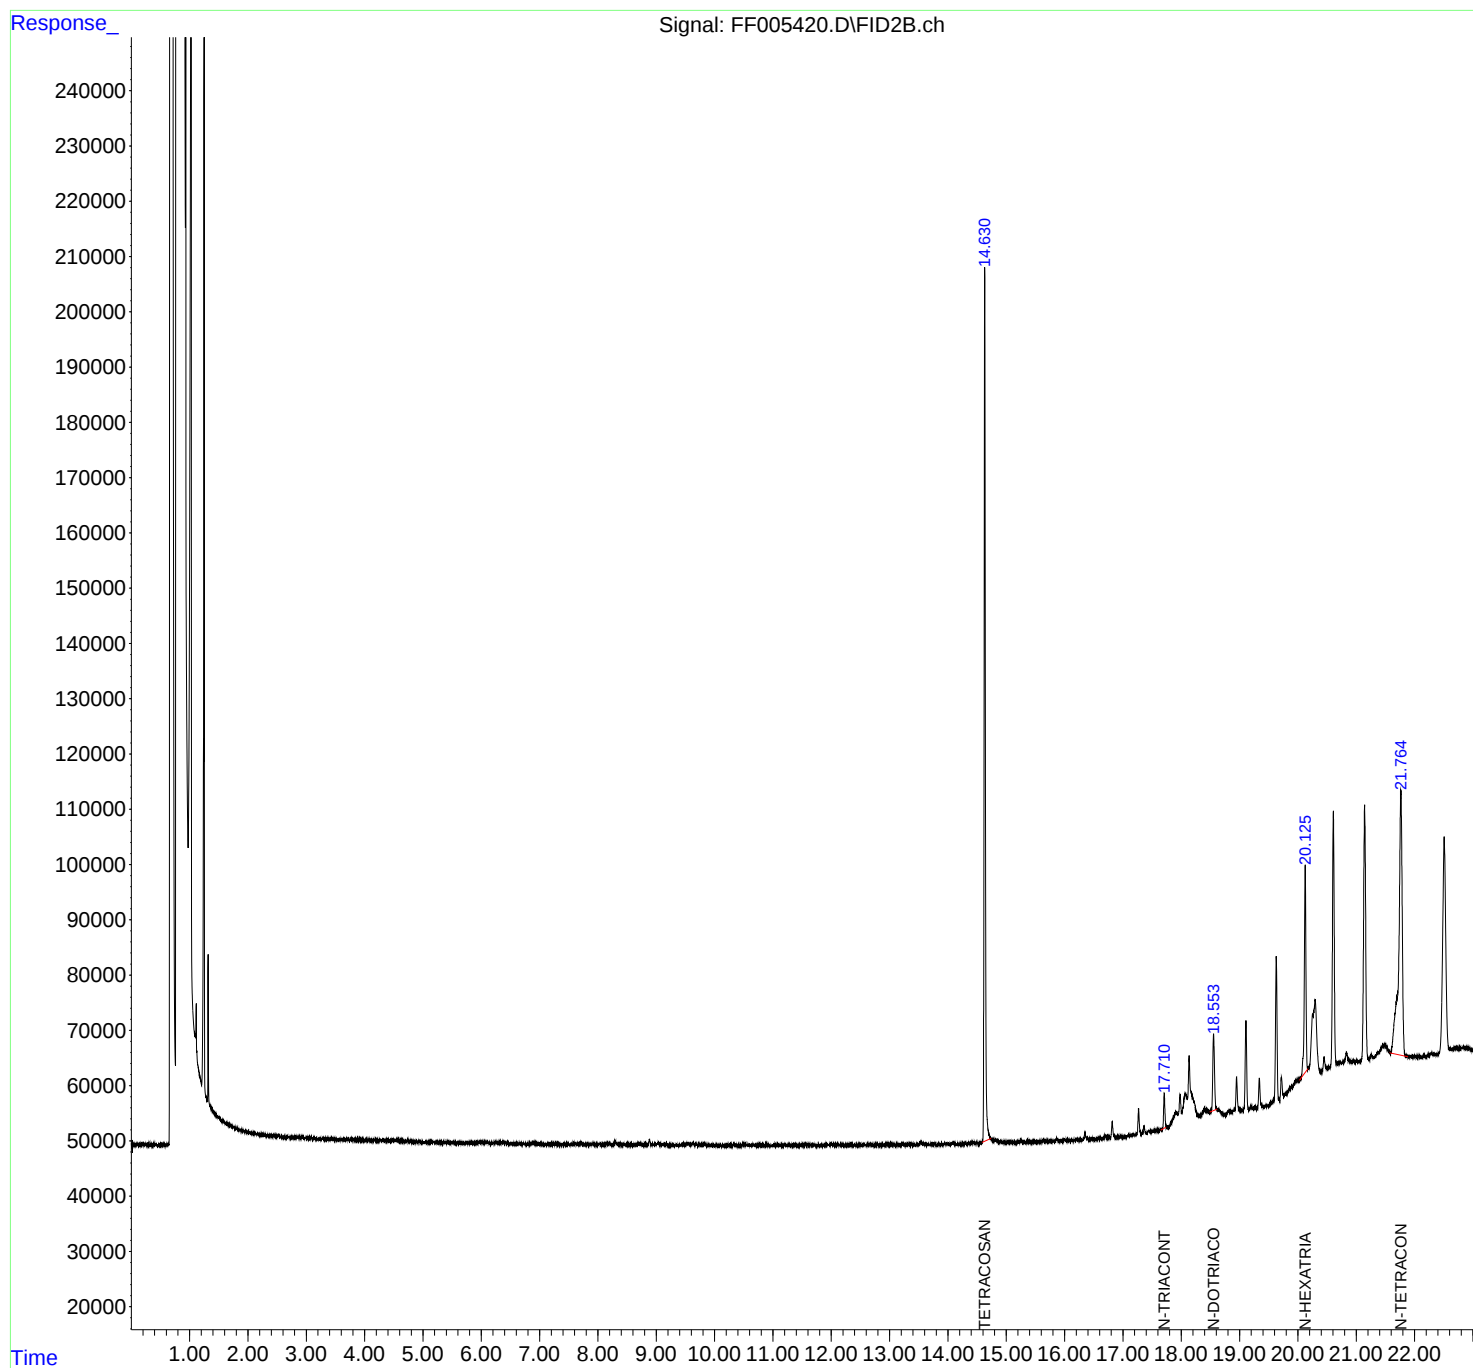


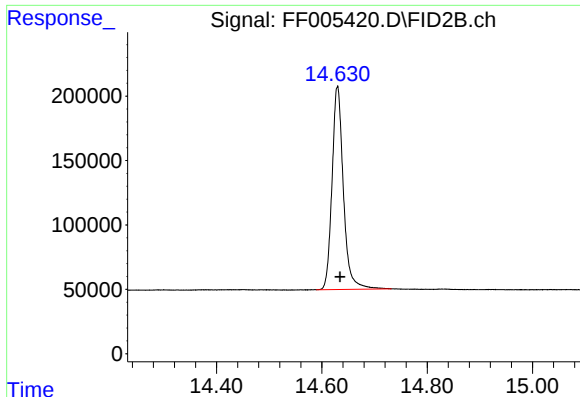

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.630 min
Delta R.T.: -0.005 min
Response: 2360379
Conc: 22.06 ug/ml

Instrument :
FID_F
ClientSampleId :

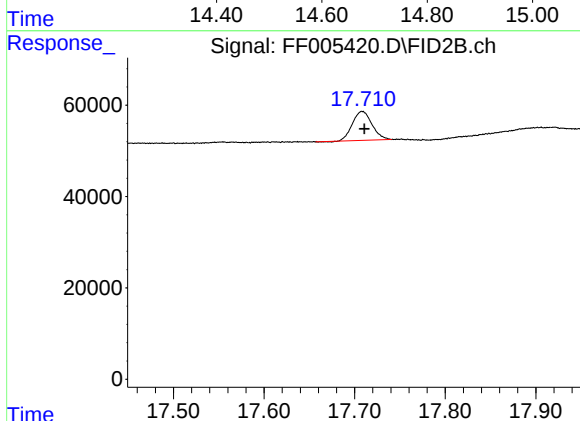


#13 N-TRIACONTANE

R.T.: 17.708 min
Delta R.T.: -0.002 min
Response: 95195
Conc: 0.79 ug/ml

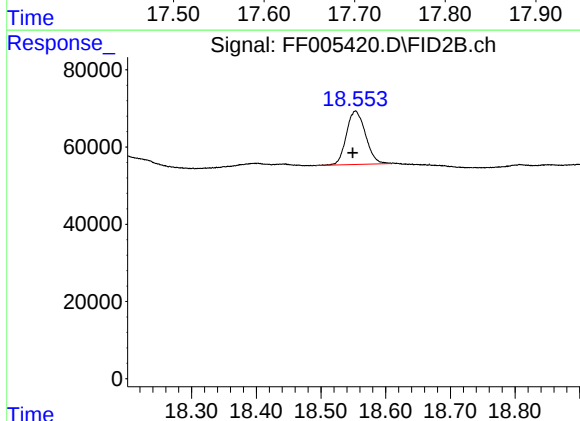


#14 N-DOTRIACONTANE

R.T.: 18.553 min
Delta R.T.: 0.004 min
Response: 283024
Conc: 2.28 ug/ml

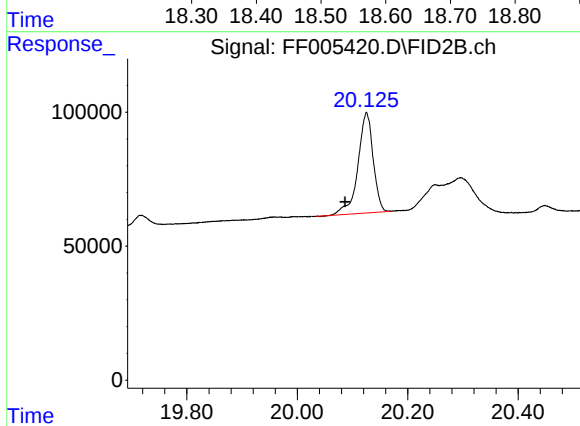

#16 N-HEXATRIACONTANE

R.T.: 20.125 min
Delta R.T.: 0.039 min
Response: 715030
Conc: 5.96 ug/ml

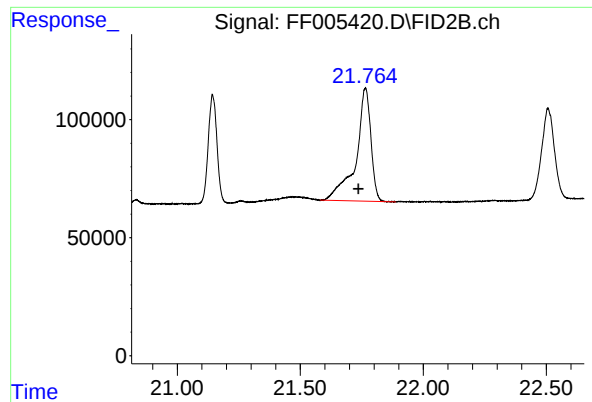

#18 N-TETRACONTANE

R.T.: 21.764 min
Delta R.T.: 0.028 min
Response: 2030075
Conc: 15.97 ug/ml

Instrument :
FID_F
ClientSampleId :