

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
Data File : FF005422.D
Signal(s) : FID2B.ch
Acq On : 05 Sep 2019 12:46
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 06 01:12:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.367	5263920	36.721 ug/ml
12) N-OCTACOSANE	16.816	4432239	37.144 ug/ml
14) N-DOTRIACONTANE	18.554	407684	3.289 ug/ml
18) N-TETRACONTANE	21.771	804651	6.329 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
Data File : FF005422.D
Signal(s) : FID2B.ch
Acq On : 05 Sep 2019 12:46
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 06 01:12:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

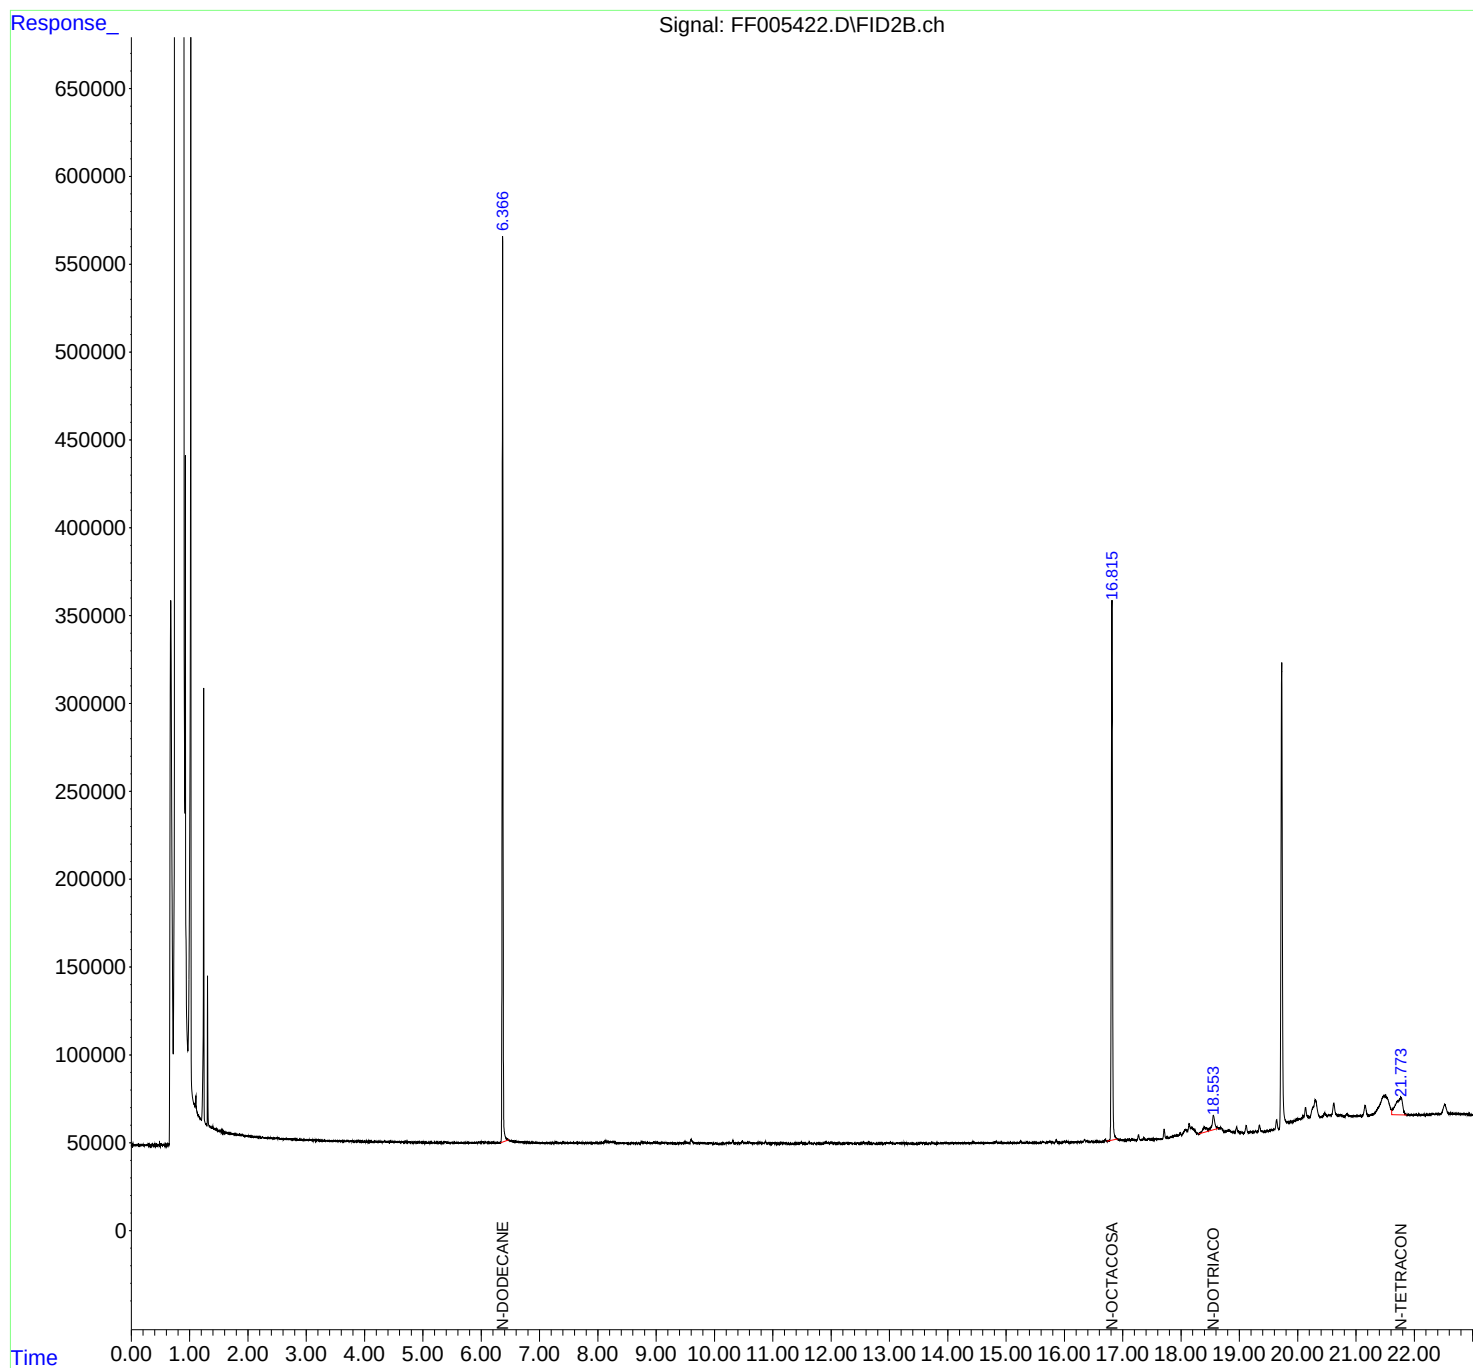


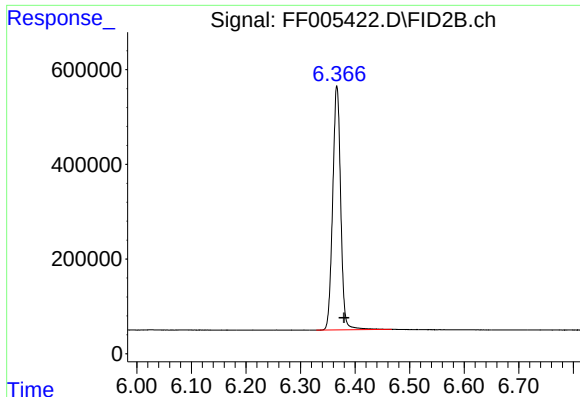

#3 N-DODECANE


R.T.: 6.367 min
Delta R.T.: -0.013 min
Response: 5263920
Conc: 36.72 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

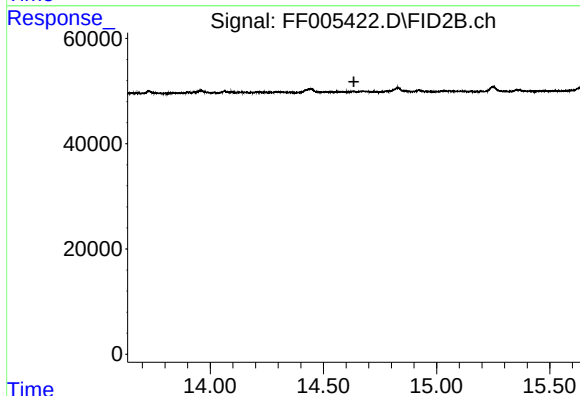


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.635 min
Response: 0
Conc: N.D.

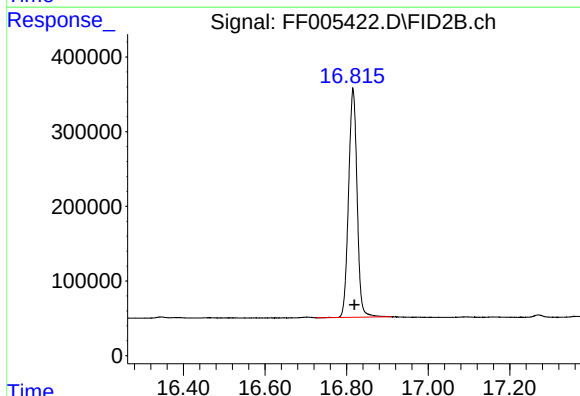


#12 N-OCTACOSANE

R.T.: 16.816 min
Delta R.T.: -0.003 min
Response: 4432239
Conc: 37.14 ug/ml

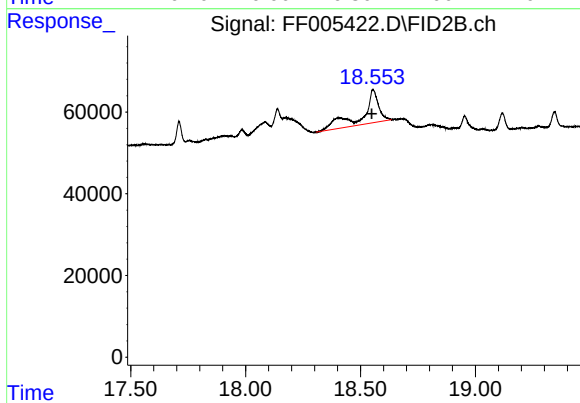

#14 N-DOTRIACONTANE

R.T.: 18.554 min
Delta R.T.: 0.005 min
Response: 407684
Conc: 3.29 ug/ml

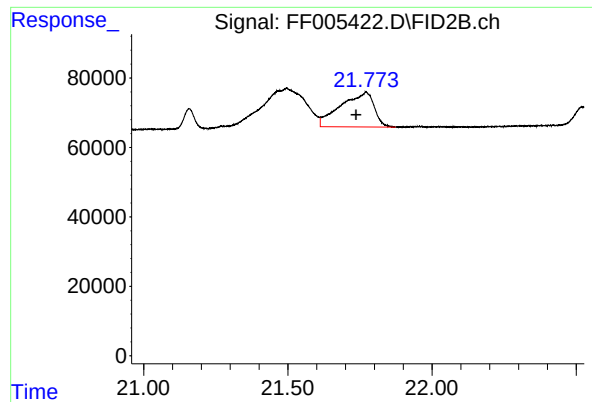

#18 N-TETRACONTANE

R.T.: 21.771 min
Delta R.T.: 0.035 min
Response: 804651
Conc: 6.33 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER