

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
 Data File : FF005427.D
 Signal(s) : FID2B.ch
 Acq On : 05 Sep 2019 17:26
 Operator : DD\AJ
 Sample : K4696-02
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WS-SB04-COMP

Integration File: autoint1.e
 Quant Time: Sep 06 01:14:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	2193564	20.499 ug/ml
Target Compounds			
4) N-TETRADECANE	8.230f	326763	2.318 ug/ml
7) N-EICOSANE	12.584f	1765667	13.463 ug/ml
10) N-TETRACOSANE	14.814	859536	7.028 ug/ml
12) N-OCTACOSANE	16.830	250420	2.099 ug/ml
13) N-TRIACONTANE	17.704	83120	0.687 ug/ml
14) N-DOTRIACONTANE	18.549	298679	2.409 ug/ml
16) N-HEXATRIACONTANE	20.126	476047	3.966 ug/ml
18) N-TETRACONTANE	21.766	1525557	11.999 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
Data File : FF005427.D
Signal(s) : FID2B.ch
Acq On : 05 Sep 2019 17:26
Operator : DD\AJ
Sample : K4696-02
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WS-SB04-COMP

Integration File: autoint1.e
Quant Time: Sep 06 01:14:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

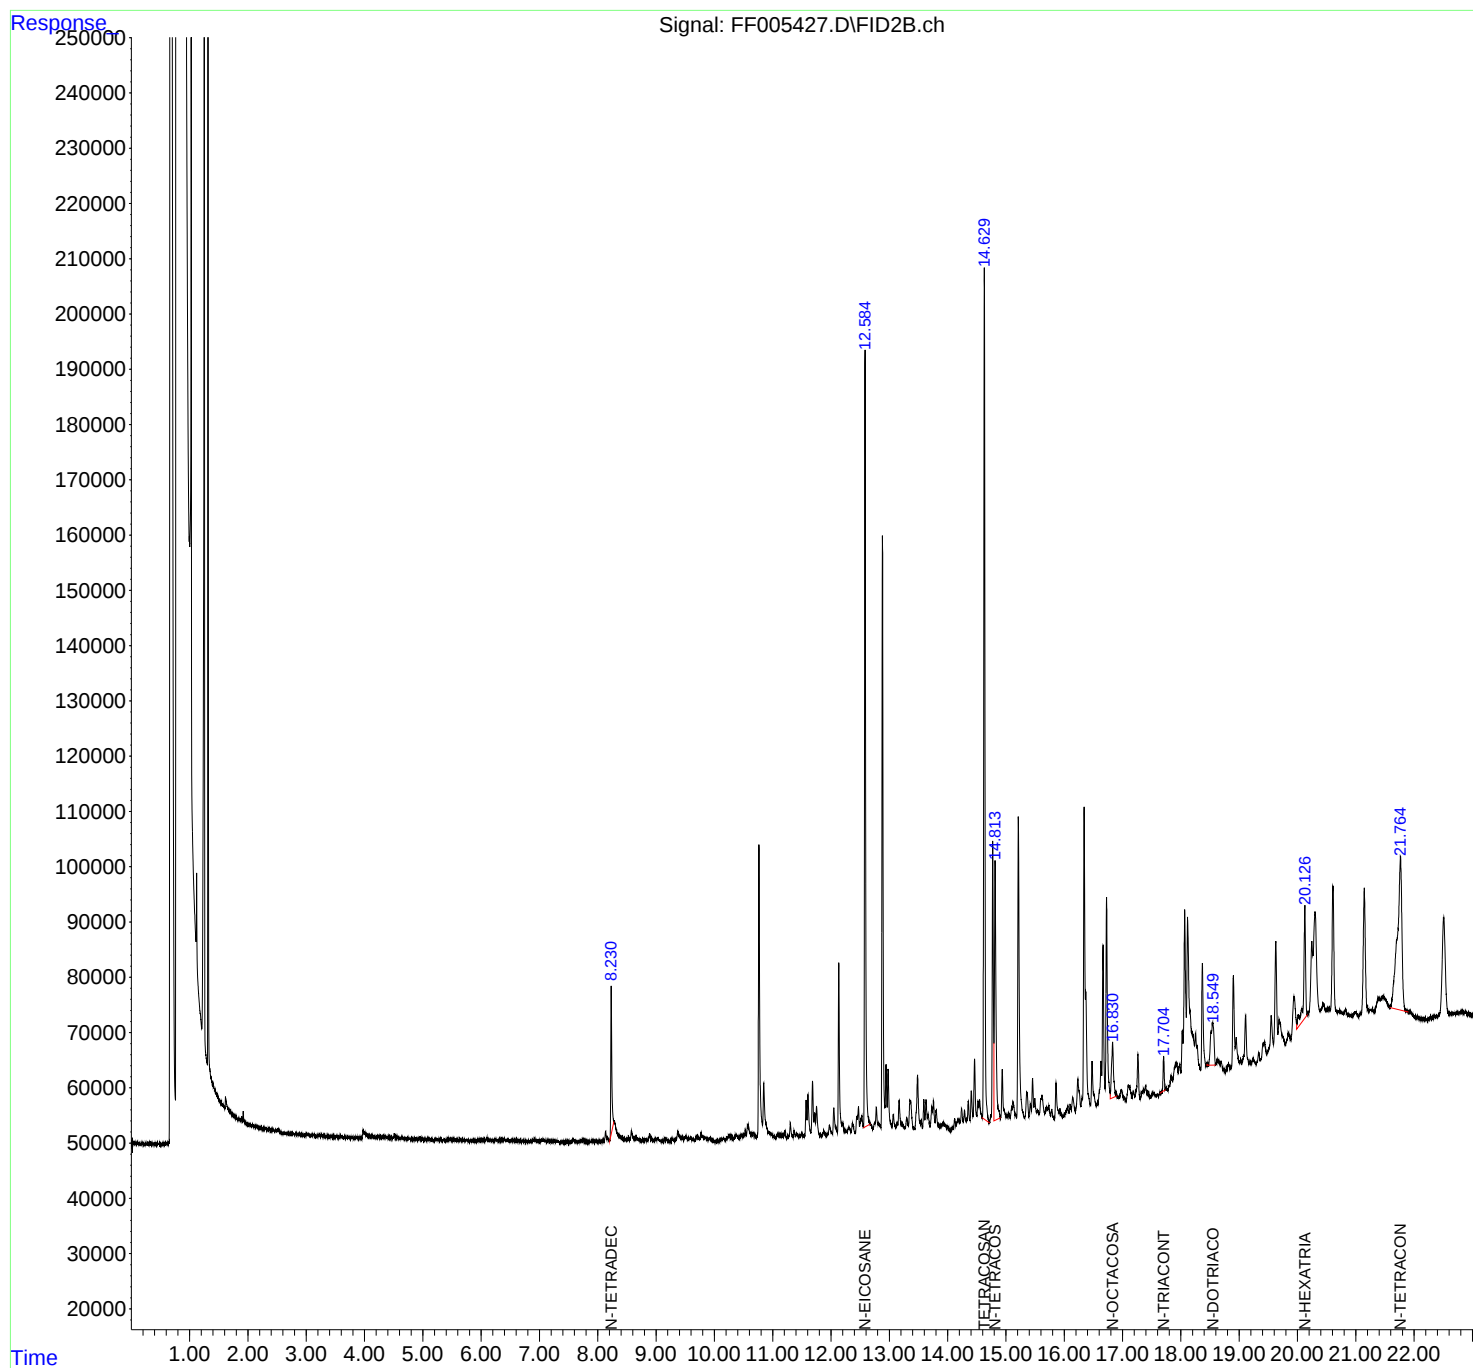


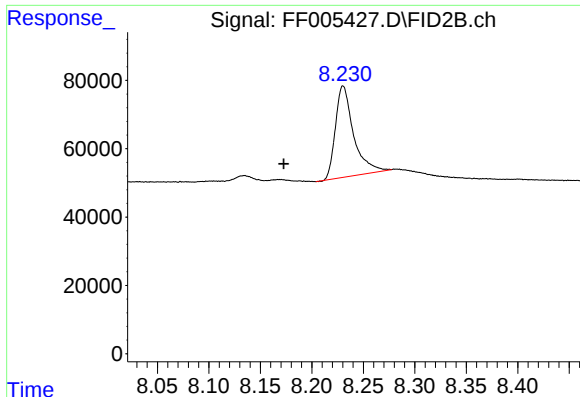

#4 N-TETRADECANE


R.T.: 8.230 min
Delta R.T.: 0.058 min
Response: 326763
Conc: 2.32 ug/ml

Instrument :
FID_F
ClientSampleId :
WS-SB04-COMP

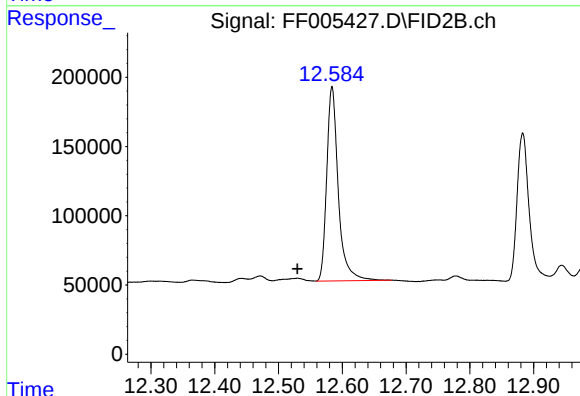


#7 N-EICOSANE

R.T.: 12.584 min
Delta R.T.: 0.054 min
Response: 1765667
Conc: 13.46 ug/ml

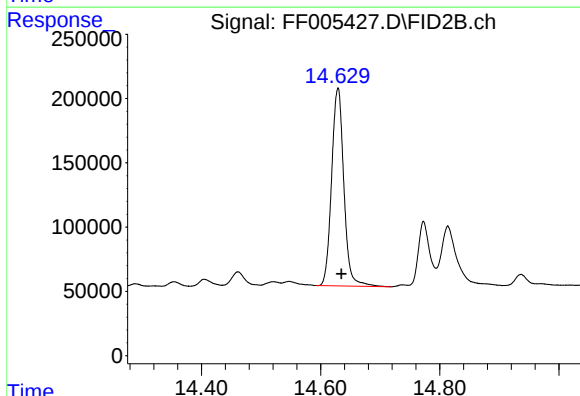


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.629 min
Delta R.T.: -0.005 min
Response: 2193564
Conc: 20.50 ug/ml

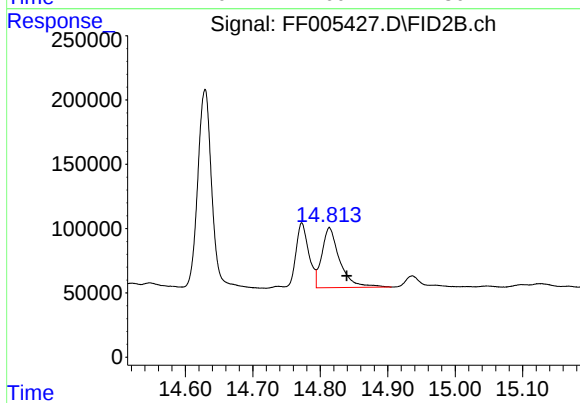

#10 N-TETRACOSANE


R.T.: 14.814 min
Delta R.T.: -0.026 min
Response: 859536
Conc: 7.03 ug/ml

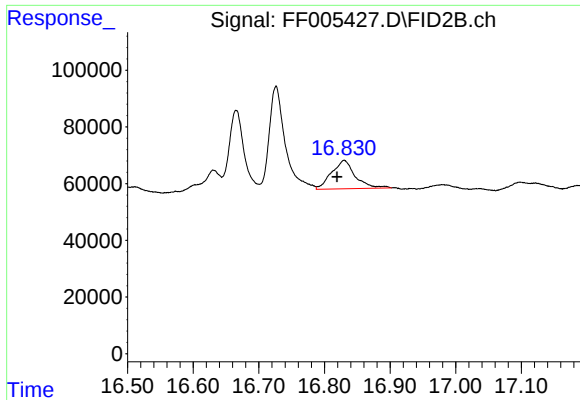

#12 N-OCTACOSANE


R.T.: 16.830 min
Delta R.T.: 0.011 min
Response: 250420
Conc: 2.10 ug/ml

Instrument :
FID_F
ClientSampleId :
WS-SB04-COMP

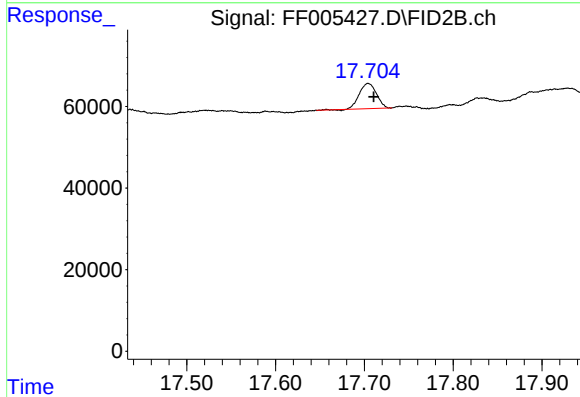


#13 N-TRIACONTANE

R.T.: 17.704 min
Delta R.T.: -0.006 min
Response: 83120
Conc: 0.69 ug/ml

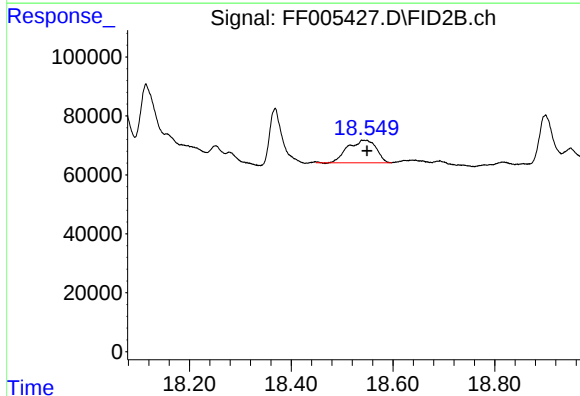


#14 N-DOTRIACONTANE

R.T.: 18.549 min
Delta R.T.: 0.000 min
Response: 298679
Conc: 2.41 ug/ml

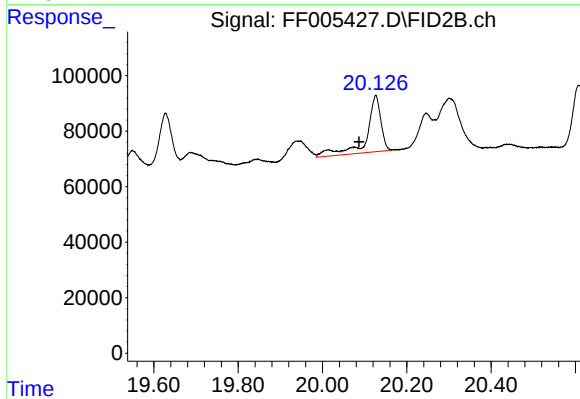

#16 N-HEXATRIACONTANE

R.T.: 20.126 min
Delta R.T.: 0.040 min
Response: 476047
Conc: 3.97 ug/ml

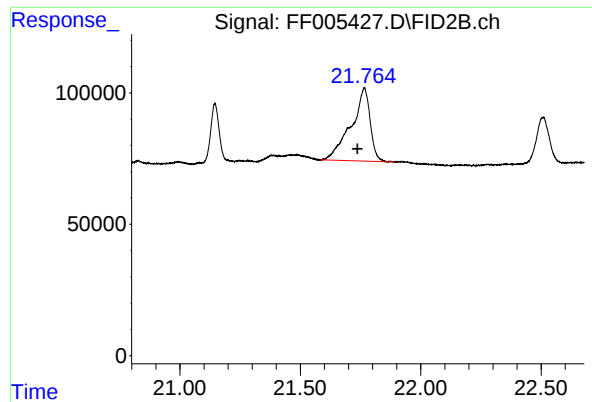

#18 N-TETRACONTANE

R.T.: 21.766 min
Delta R.T.: 0.029 min
Response: 1525557
Conc: 12.00 ug/ml

Instrument :
FID_F
ClientSampleId :
WS-SB04-COMP