

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF090519\  
 Data File : FF005429.D  
 Signal(s) : FID2B.ch  
 Acq On : 05 Sep 2019 18:26  
 Operator : DD\AJ  
 Sample : K4692-02  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Sep 06 01:15:06 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090319.M  
 Quant Title :  
 QLast Update : Wed Sep 04 03:16:00 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	2522727	23.575 ug/ml
Target Compounds			
4) N-TETRADECANE	8.227f	680601	4.827 ug/ml
7) N-EICOSANE	12.527	254757	1.943 ug/ml
8) N-DOCOSANE	13.727	124474	0.989 ug/ml
10) N-TETRACOSANE	14.817	575256	4.704 ug/ml
11) N-HEXACOSANE	15.858	289928	2.422 ug/ml
12) N-OCTACOSANE	16.813	619427	5.191 ug/ml
13) N-TRIACONTANE	17.706	547653	4.527 ug/ml
14) N-DOTRIACONTANE	18.559	1776238	14.329 ug/ml
15) N-TETRATRIACONTANE	19.337	256941	2.132 ug/ml
16) N-HEXATRIACONTANE	20.126	3559692	29.658 ug/ml
18) N-TETRACONTANE	21.770	2603119	20.475 ug/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF090519\  
 Data File : FF005429.D  
 Signal(s) : FID2B.ch  
 Acq On : 05 Sep 2019 18:26  
 Operator : DD\AJ  
 Sample : K4692-02  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampled :

Integration File: autoint1.e  
 Quant Time: Sep 06 01:15:06 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090319.M  
 Quant Title :  
 QLast Update : Wed Sep 04 03:16:00 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

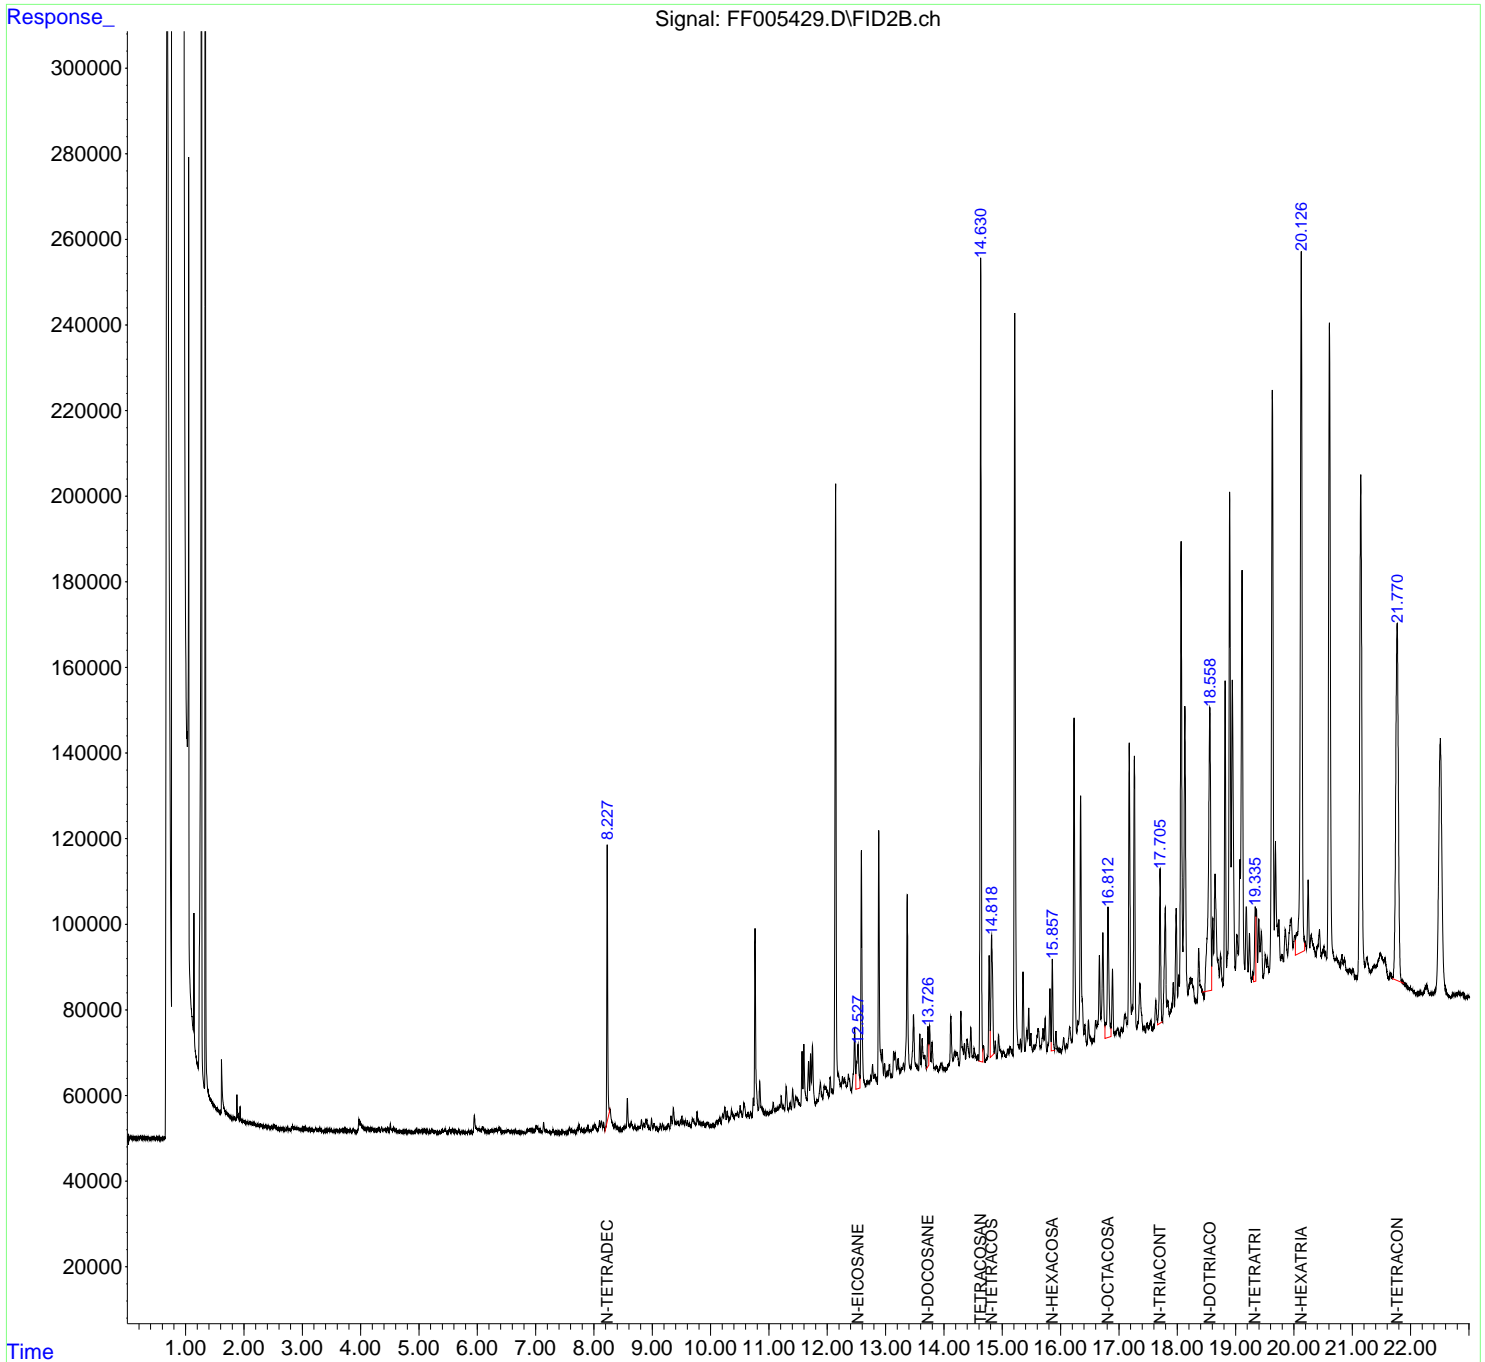

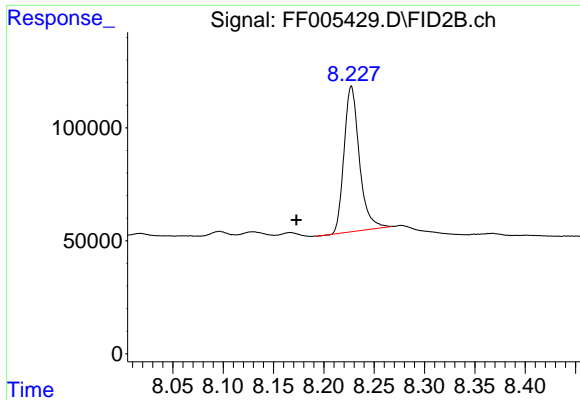


#4 N-TETRADECANE  
R.T.: 8.227 min  
Delta R.T.: 0.055 min  
Response: 680601  
Conc: 4.83 ug/ml


Instrument :  
FID\_F  
ClientSampleId :

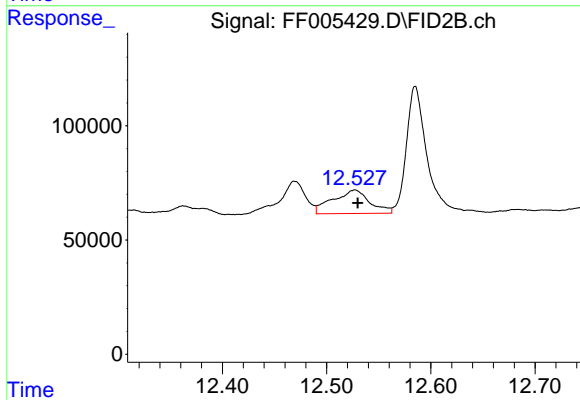


#7 N-EICOSANE  
R.T.: 12.527 min  
Delta R.T.: -0.003 min  
Response: 254757  
Conc: 1.94 ug/ml

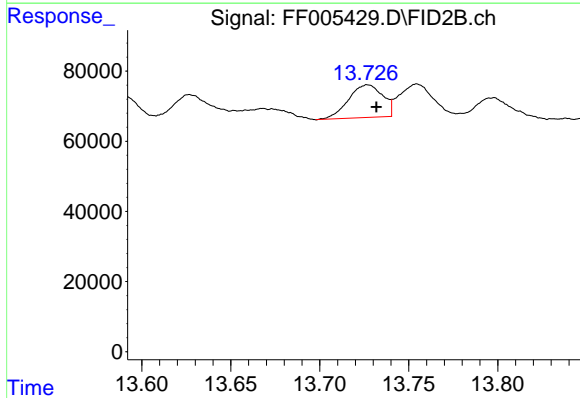

#8 N-DOCOSANE  
R.T.: 13.727 min  
Delta R.T.: -0.005 min  
Response: 124474  
Conc: 0.99 ug/ml

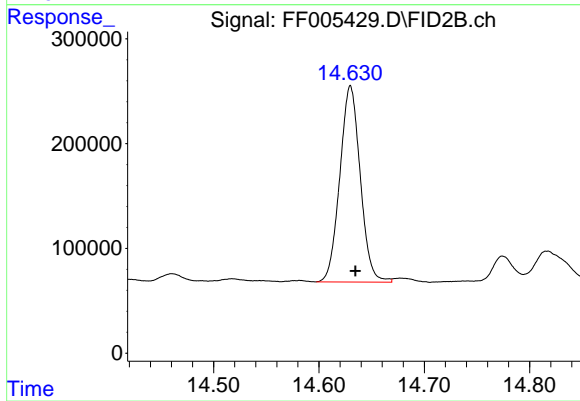


#9 TETRACOSANE-d50 (SURROGATE)  
R.T.: 14.630 min  
Delta R.T.: -0.005 min  
Response: 2522727  
Conc: 23.57 ug/ml

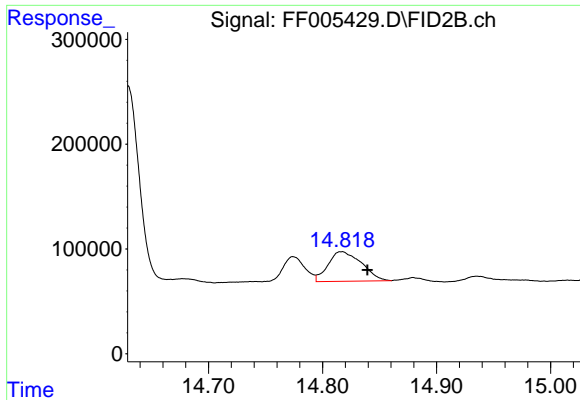


#10 N-TETRACOSANE  
 R.T.: 14.817 min  
 Delta R.T.: -0.023 min  
 Response: 575256  
 Conc: 4.70 ug/ml


Instrument :  
 FID\_F  
 ClientSampled :

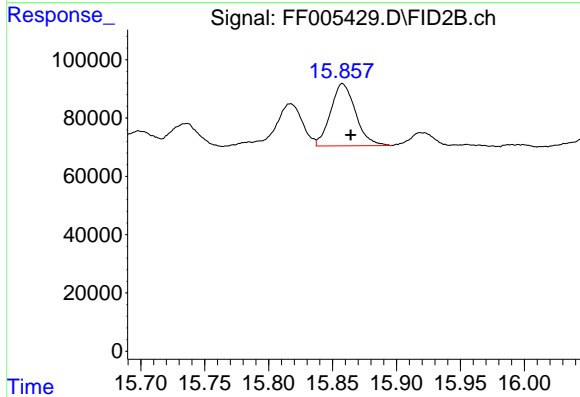


#11 N-HEXACOSANE  
 R.T.: 15.858 min  
 Delta R.T.: -0.006 min  
 Response: 289928  
 Conc: 2.42 ug/ml

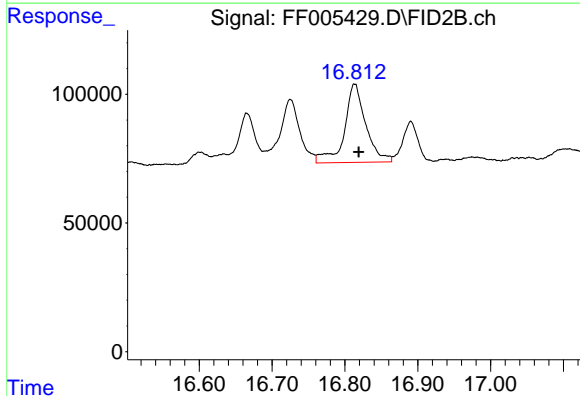

#12 N-OCTACOSANE  
 R.T.: 16.813 min  
 Delta R.T.: -0.006 min  
 Response: 619427  
 Conc: 5.19 ug/ml

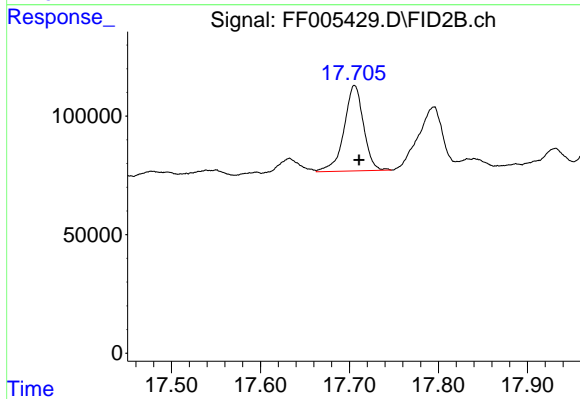


#13 N-TRIACONTANE  
 R.T.: 17.706 min  
 Delta R.T.: -0.005 min  
 Response: 547653  
 Conc: 4.53 ug/ml

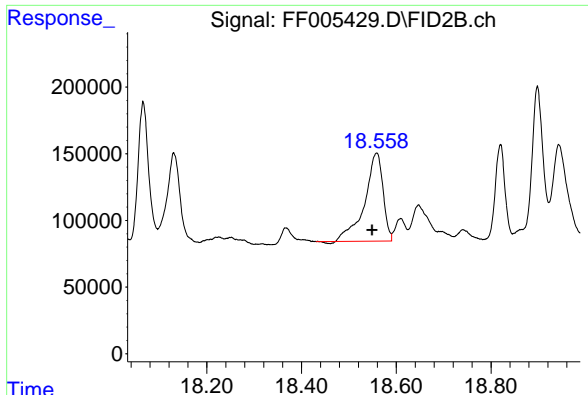

#14 N-DOTRIACONTANE


R.T.: 18.559 min  
Delta R.T.: 0.010 min  
Response: 1776238  
Conc: 14.33 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

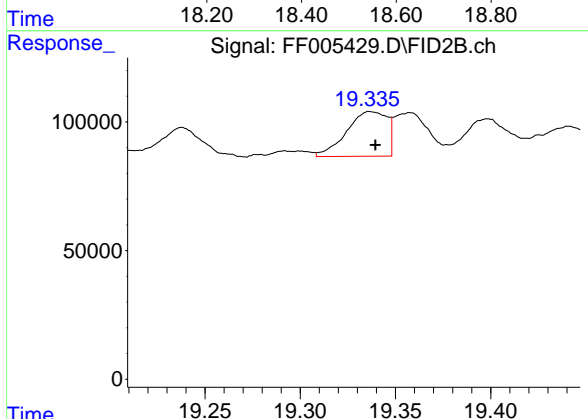


#15 N-TETRATRIACONTANE

R.T.: 19.337 min  
Delta R.T.: -0.003 min  
Response: 256941  
Conc: 2.13 ug/ml

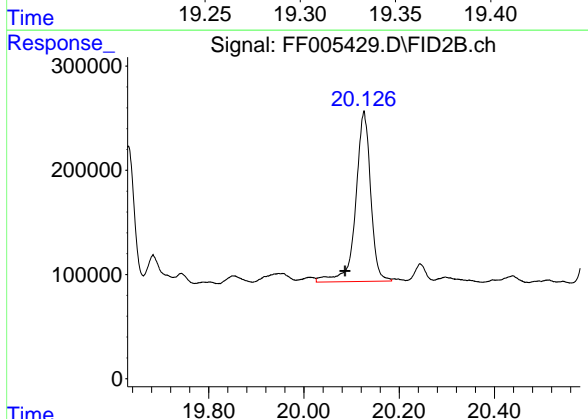

#16 N-HEXATRIACONTANE

R.T.: 20.126 min  
Delta R.T.: 0.039 min  
Response: 3559692  
Conc: 29.66 ug/ml

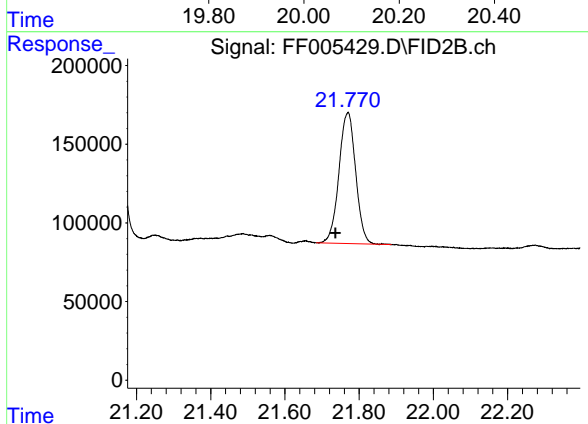

#18 N-TETRACONTANE

R.T.: 21.770 min  
Delta R.T.: 0.033 min  
Response: 2603119  
Conc: 20.47 ug/ml