

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
 Data File : FF005431.D
 Signal(s) : FID2B.ch
 Acq On : 05 Sep 2019 19:25
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Sep 06 01:15:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.631	1986972	18.568 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.555	7106	0.057 ug/ml
16) N-HEXATRIACONTANE	20.130	574233	4.784 ug/ml
18) N-TETRACONTANE	21.768	1170186	9.204 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
Data File : FF005431.D
Signal(s) : FID2B.ch
Acq On : 05 Sep 2019 19:25
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 06 01:15:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

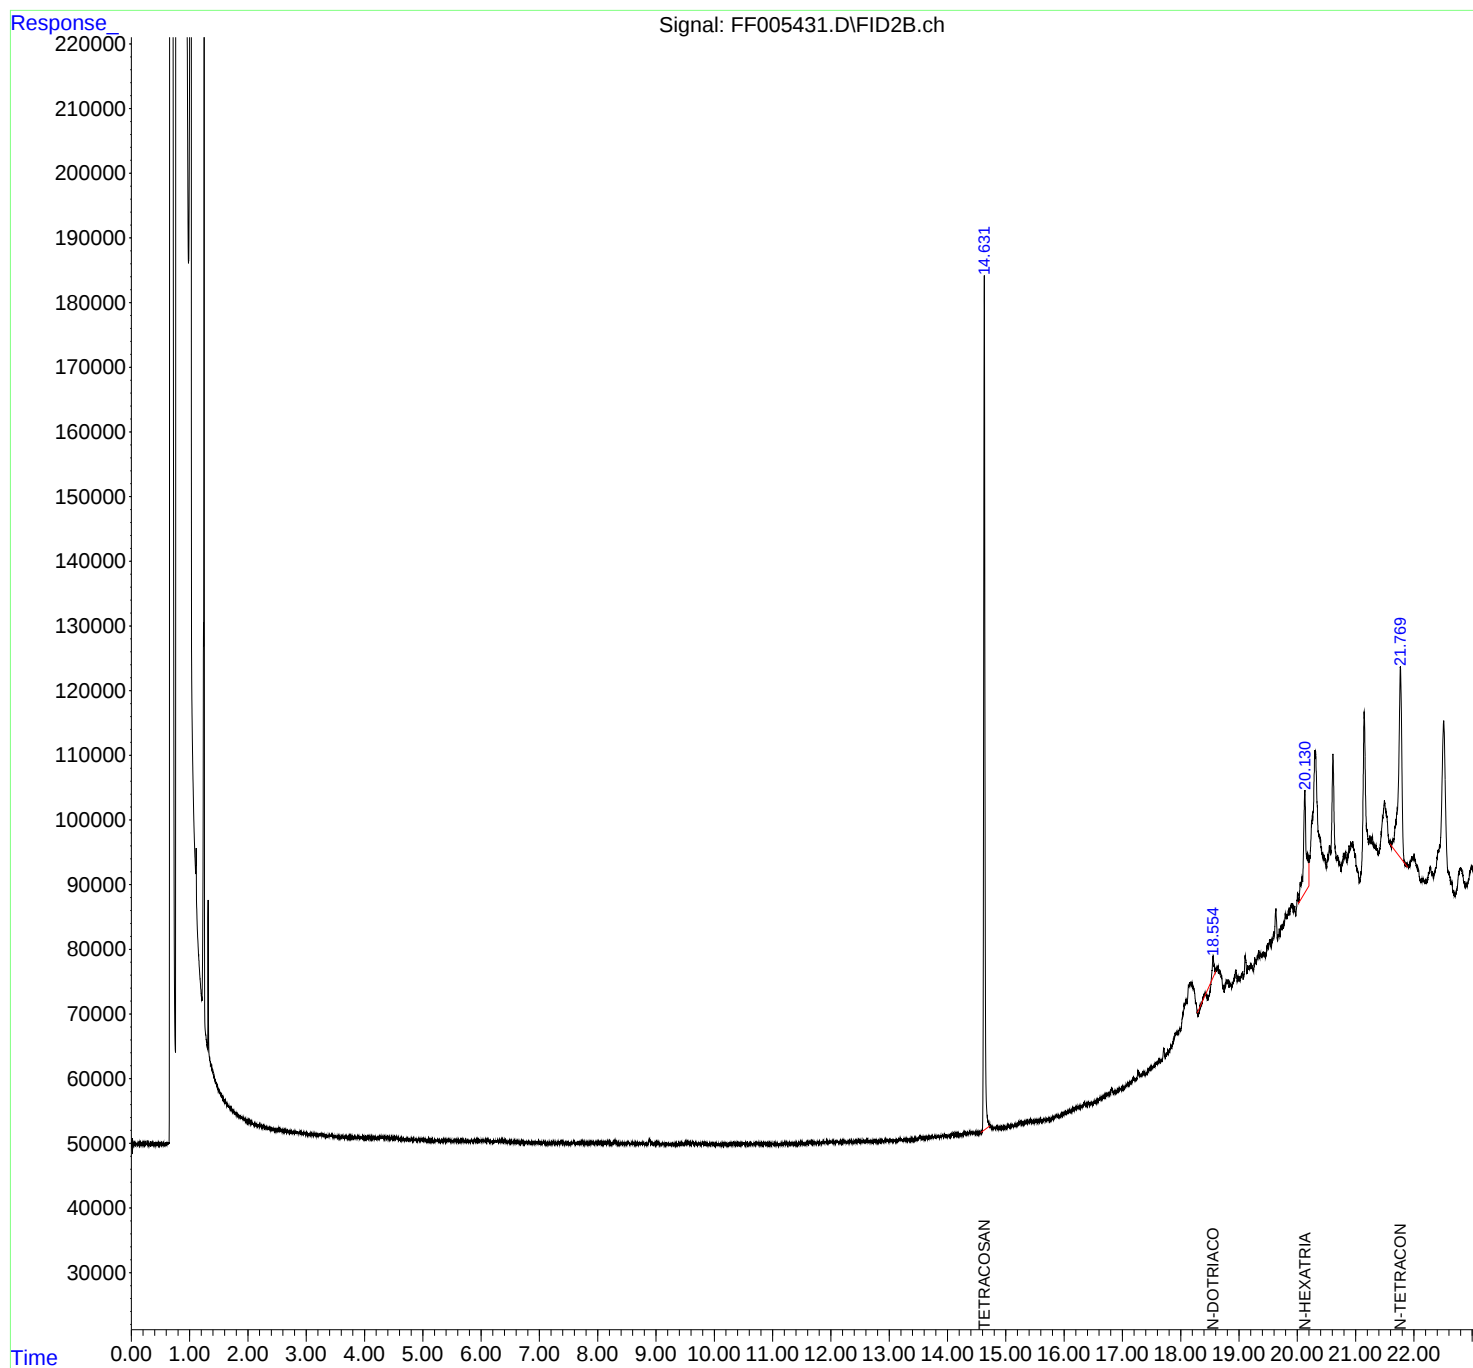


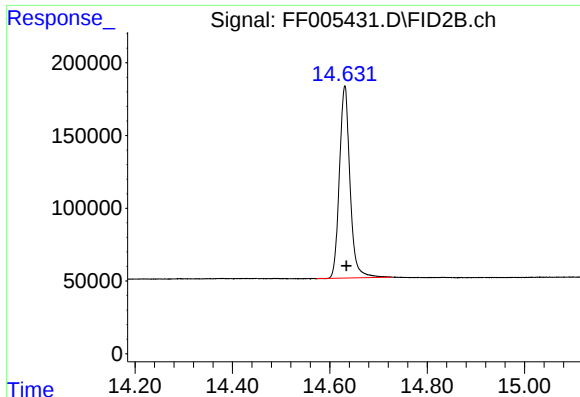

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.631 min
Delta R.T.: -0.003 min
Response: 1986972
Conc: 18.57 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

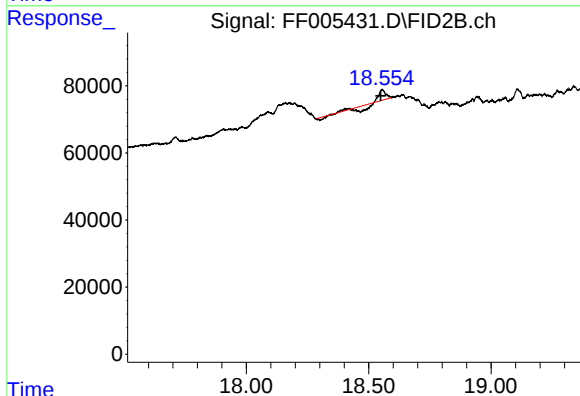


#14 N-DOTRIACONTANE

R.T.: 18.555 min
Delta R.T.: 0.006 min
Response: 7106
Conc: 0.06 ug/ml

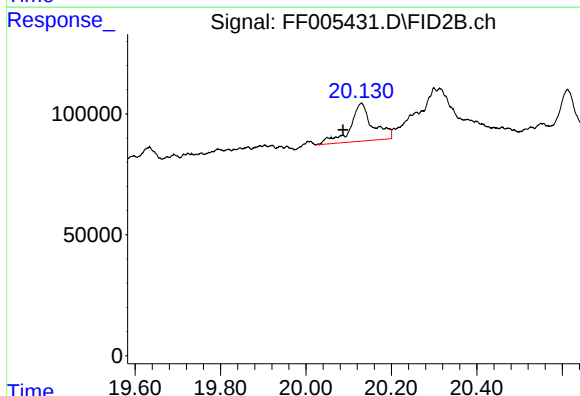

#16 N-HEXATRIACONTANE

R.T.: 20.130 min
Delta R.T.: 0.043 min
Response: 574233
Conc: 4.78 ug/ml

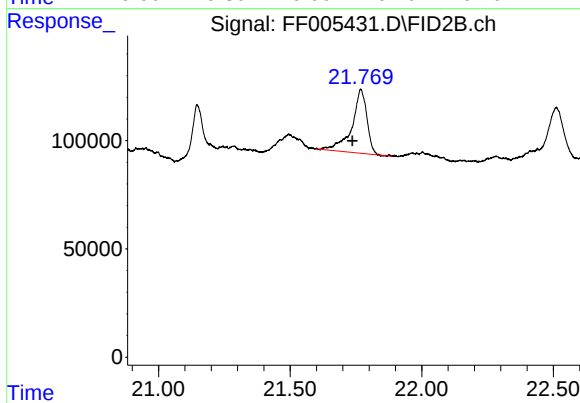

#18 N-TETRACONTANE

R.T.: 21.768 min
Delta R.T.: 0.032 min
Response: 1170186
Conc: 9.20 ug/ml