

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
 Data File : FF005436.D
 Signal(s) : FID2B.ch
 Acq On : 05 Sep 2019 21:54
 Operator : DD\AJ
 Sample : K4692-04 2X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-31-COMP

Integration File: autoint1.e
 Quant Time: Sep 06 01:17:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.635	1243716	11.623 ug/ml
Target Compounds			
4) N-TETRADECANE	8.230f	315438	2.237 ug/ml
7) N-EICOSANE	12.531	520446	3.968 ug/ml
8) N-DOCOSANE	13.731	411461	3.268 ug/ml
10) N-TETRACOSANE	14.820	2816350	23.029 ug/ml
11) N-HEXACOSANE	15.865	686616	5.736 ug/ml
12) N-OCTACOSANE	16.833	1716455	14.385 ug/ml
13) N-TRIACONTANE	17.711	1315817	10.877 ug/ml
14) N-DOTRIACONTANE	18.546	950190	7.665 ug/ml
15) N-TETRATRIACONTANE	19.345	222561	1.847 ug/ml
16) N-HEXATRIACONTANE	20.072	431545	3.595 ug/ml
17) N-OCTATRIACONTANE	20.825	12429	0.114 ug/ml
18) N-TETRACONTANE	21.741	832001	6.544 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
Data File : FF005436.D
Signal(s) : FID2B.ch
Acq On : 05 Sep 2019 21:54
Operator : DD\AJ
Sample : K4692-04 2X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-31-COMP

Integration File: autoint1.e
Quant Time: Sep 06 01:17:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

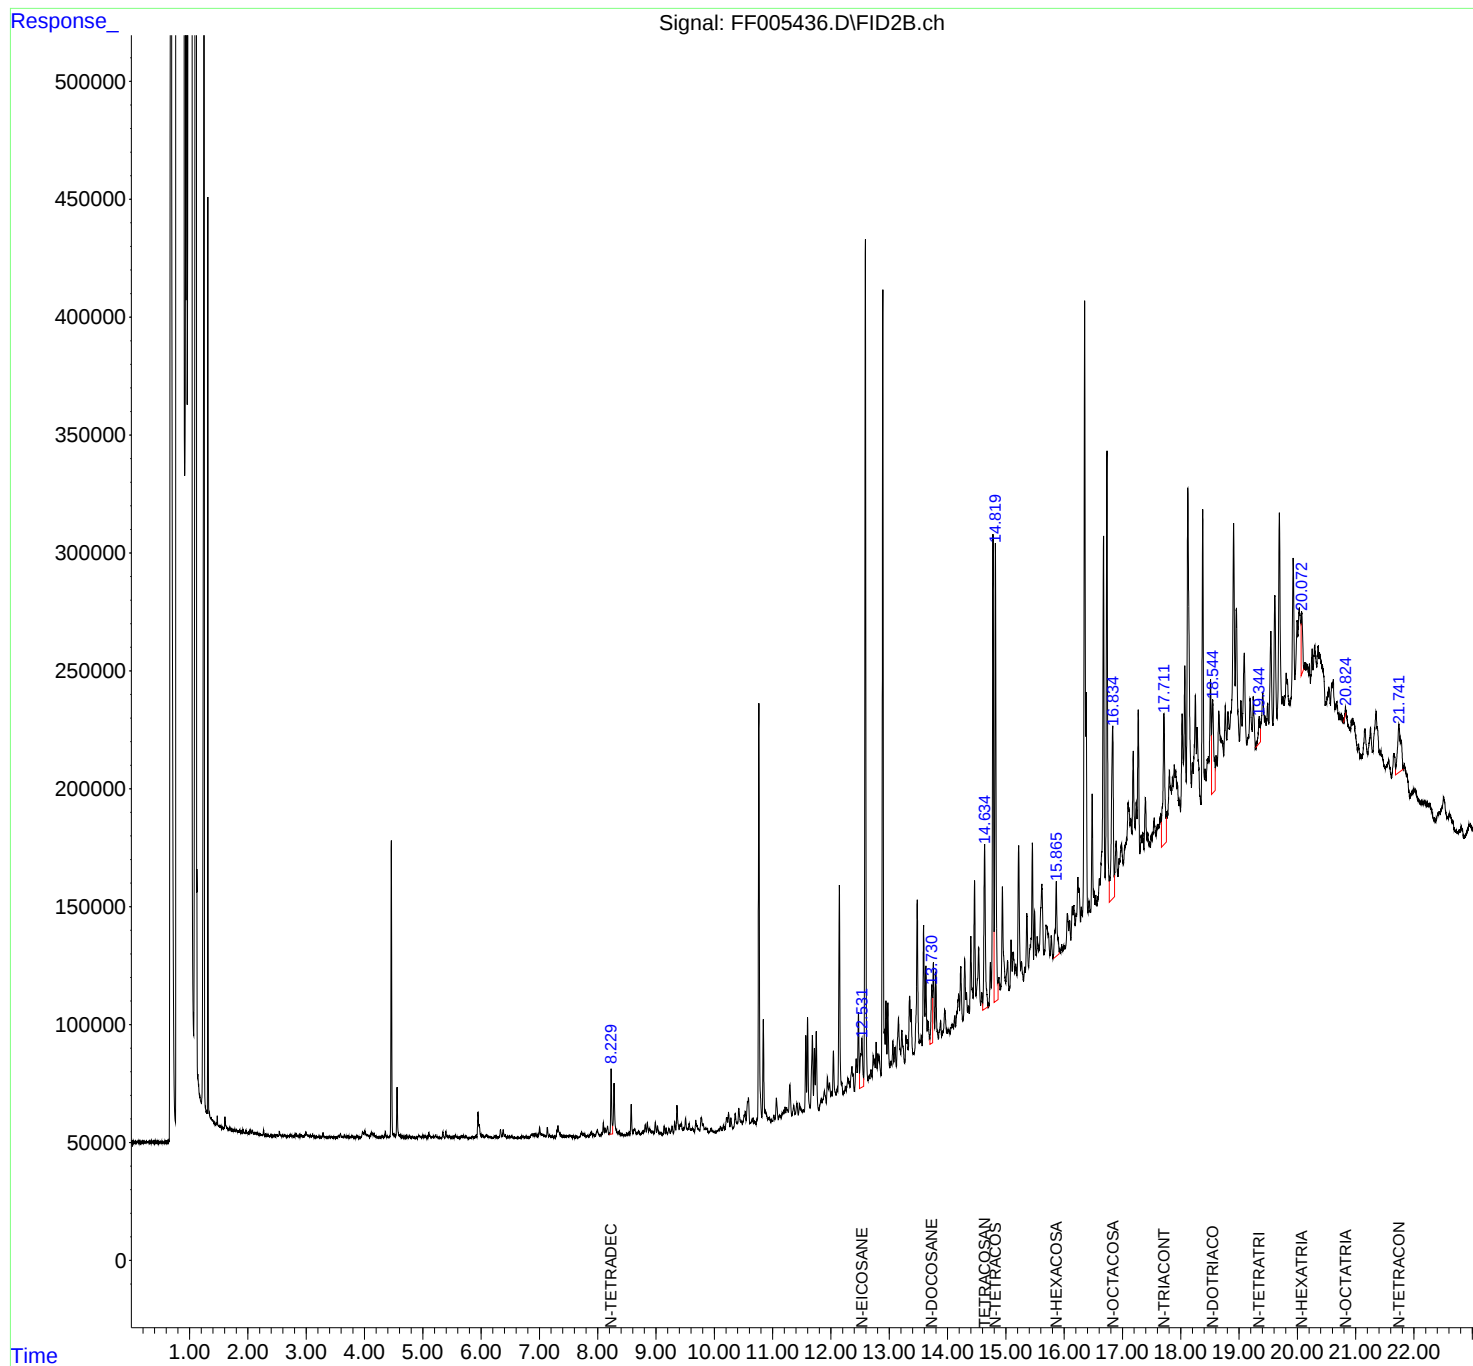


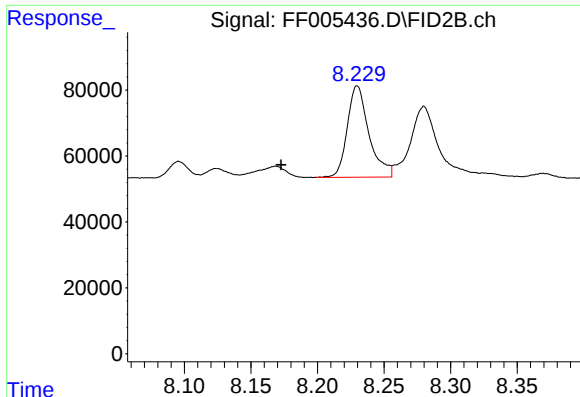

#4 N-TETRADECANE


R.T.: 8.230 min
Delta R.T.: 0.057 min
Response: 315438
Conc: 2.24 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-31-COMP

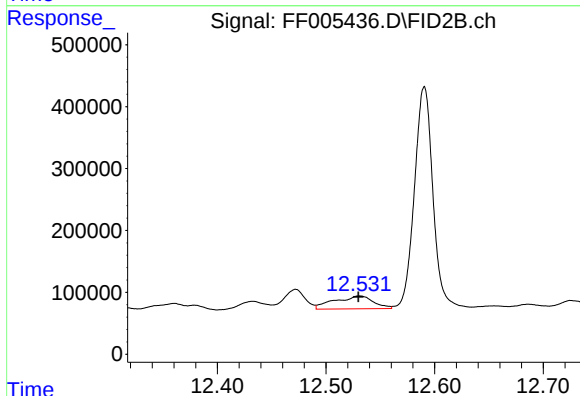


#7 N-EICOSANE

R.T.: 12.531 min
Delta R.T.: 0.000 min
Response: 520446
Conc: 3.97 ug/ml

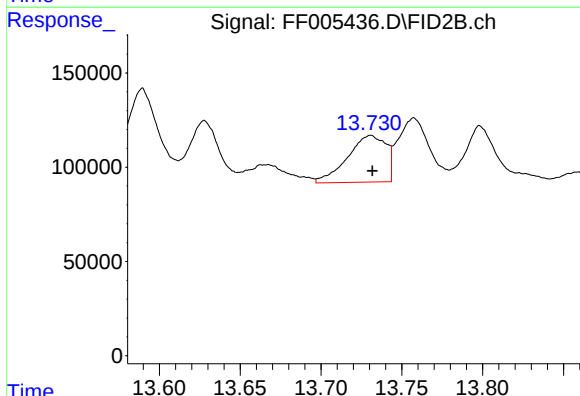


#8 N-DOCOSANE

R.T.: 13.731 min
Delta R.T.: -0.001 min
Response: 411461
Conc: 3.27 ug/ml

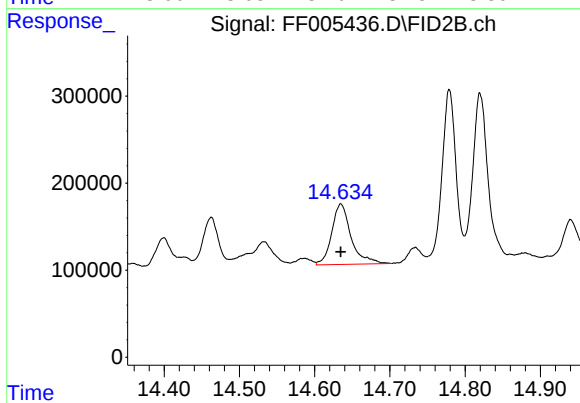

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.635 min
Delta R.T.: 0.000 min
Response: 1243716
Conc: 11.62 ug/ml

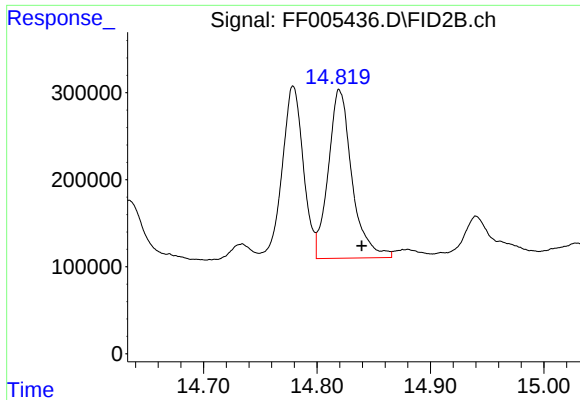

#10 N-TETRACOSANE


R.T.: 14.820 min
Delta R.T.: -0.020 min
Response: 2816350
Conc: 23.03 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-31-COMP

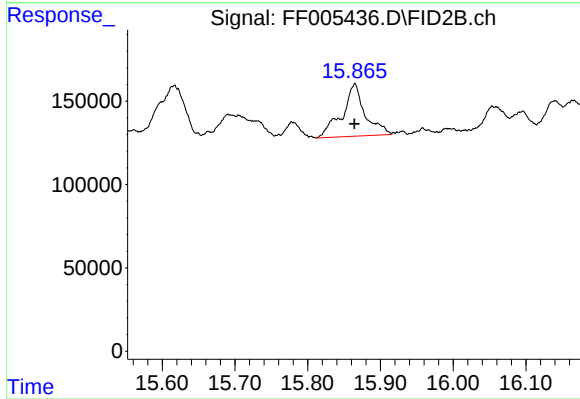


#11 N-HEXACOSANE

R.T.: 15.865 min
Delta R.T.: 0.000 min
Response: 686616
Conc: 5.74 ug/ml

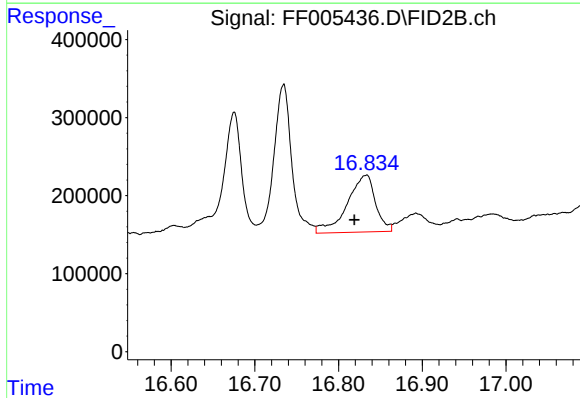


#12 N-OCTACOSANE

R.T.: 16.833 min
Delta R.T.: 0.014 min
Response: 1716455
Conc: 14.38 ug/ml

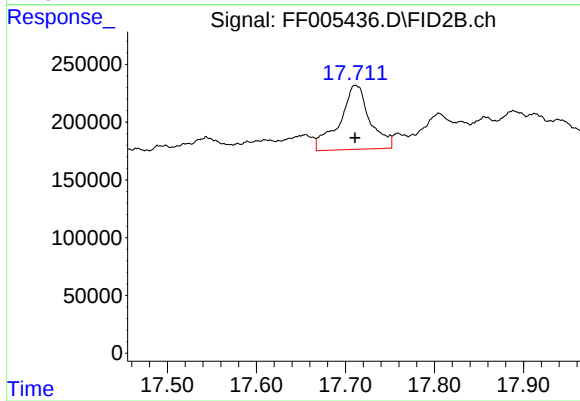

#13 N-TRIACONTANE


R.T.: 17.711 min
Delta R.T.: 0.000 min
Response: 1315817
Conc: 10.88 ug/ml

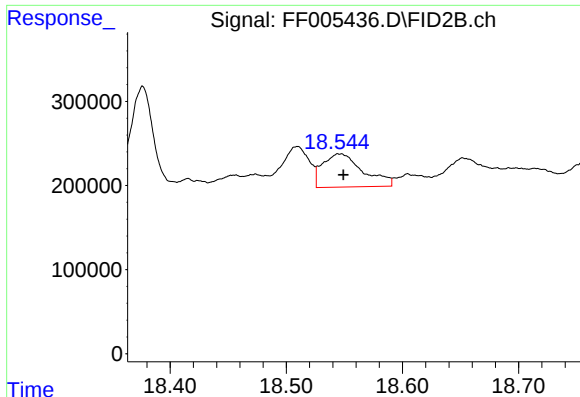

#14 N-DOTRIACONTANE


R.T.: 18.546 min
Delta R.T.: -0.003 min
Response: 950190
Conc: 7.67 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-31-COMP

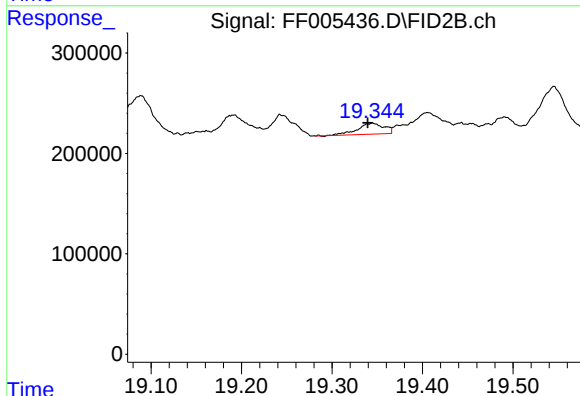


#15 N-TETRATRIACONTANE

R.T.: 19.345 min
Delta R.T.: 0.005 min
Response: 222561
Conc: 1.85 ug/ml

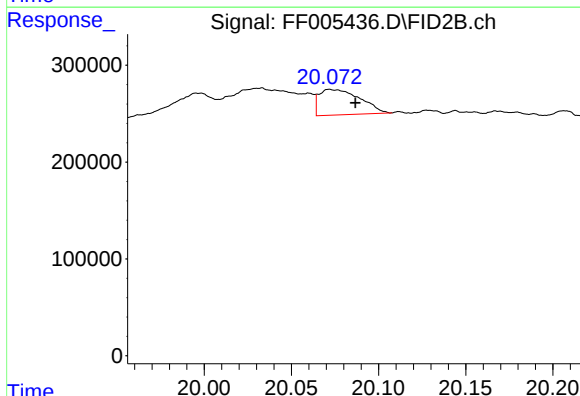


#16 N-HEXATRIACONTANE

R.T.: 20.072 min
Delta R.T.: -0.014 min
Response: 431545
Conc: 3.60 ug/ml

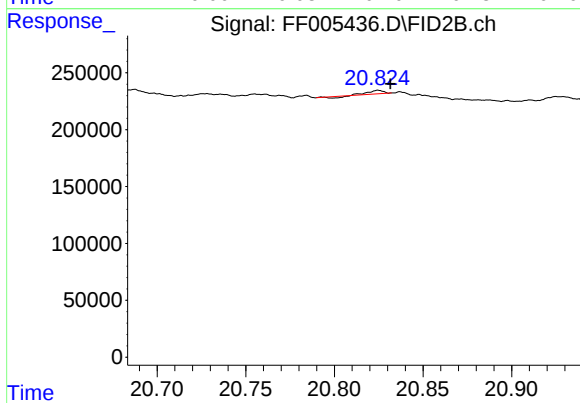

#17 N-OCTATRIACONTANE

R.T.: 20.825 min
Delta R.T.: -0.007 min
Response: 12429
Conc: 0.11 ug/ml

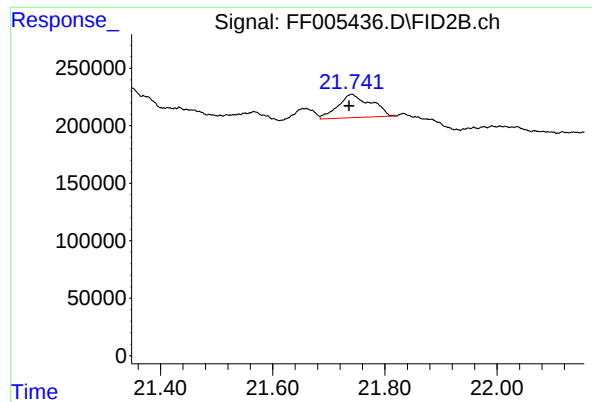

#18 N-TETRACONTANE

R.T.: 21.741 min
Delta R.T.: 0.005 min
Response: 832001
Conc: 6.54 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-31-COMP