

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
Data File : FF005439.D
Signal(s) : FID2B.ch
Acq On : 05 Sep 2019 23:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 06 01:18:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	2055425	19.208 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.555	145469	1.173 ug/ml
16) N-HEXATRIACONTANE	20.081	249606	2.080 ug/ml
18) N-TETRACONTANE	21.764	893206	7.026 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
Data File : FF005439.D
Signal(s) : FID2B.ch
Acq On : 05 Sep 2019 23:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 06 01:18:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

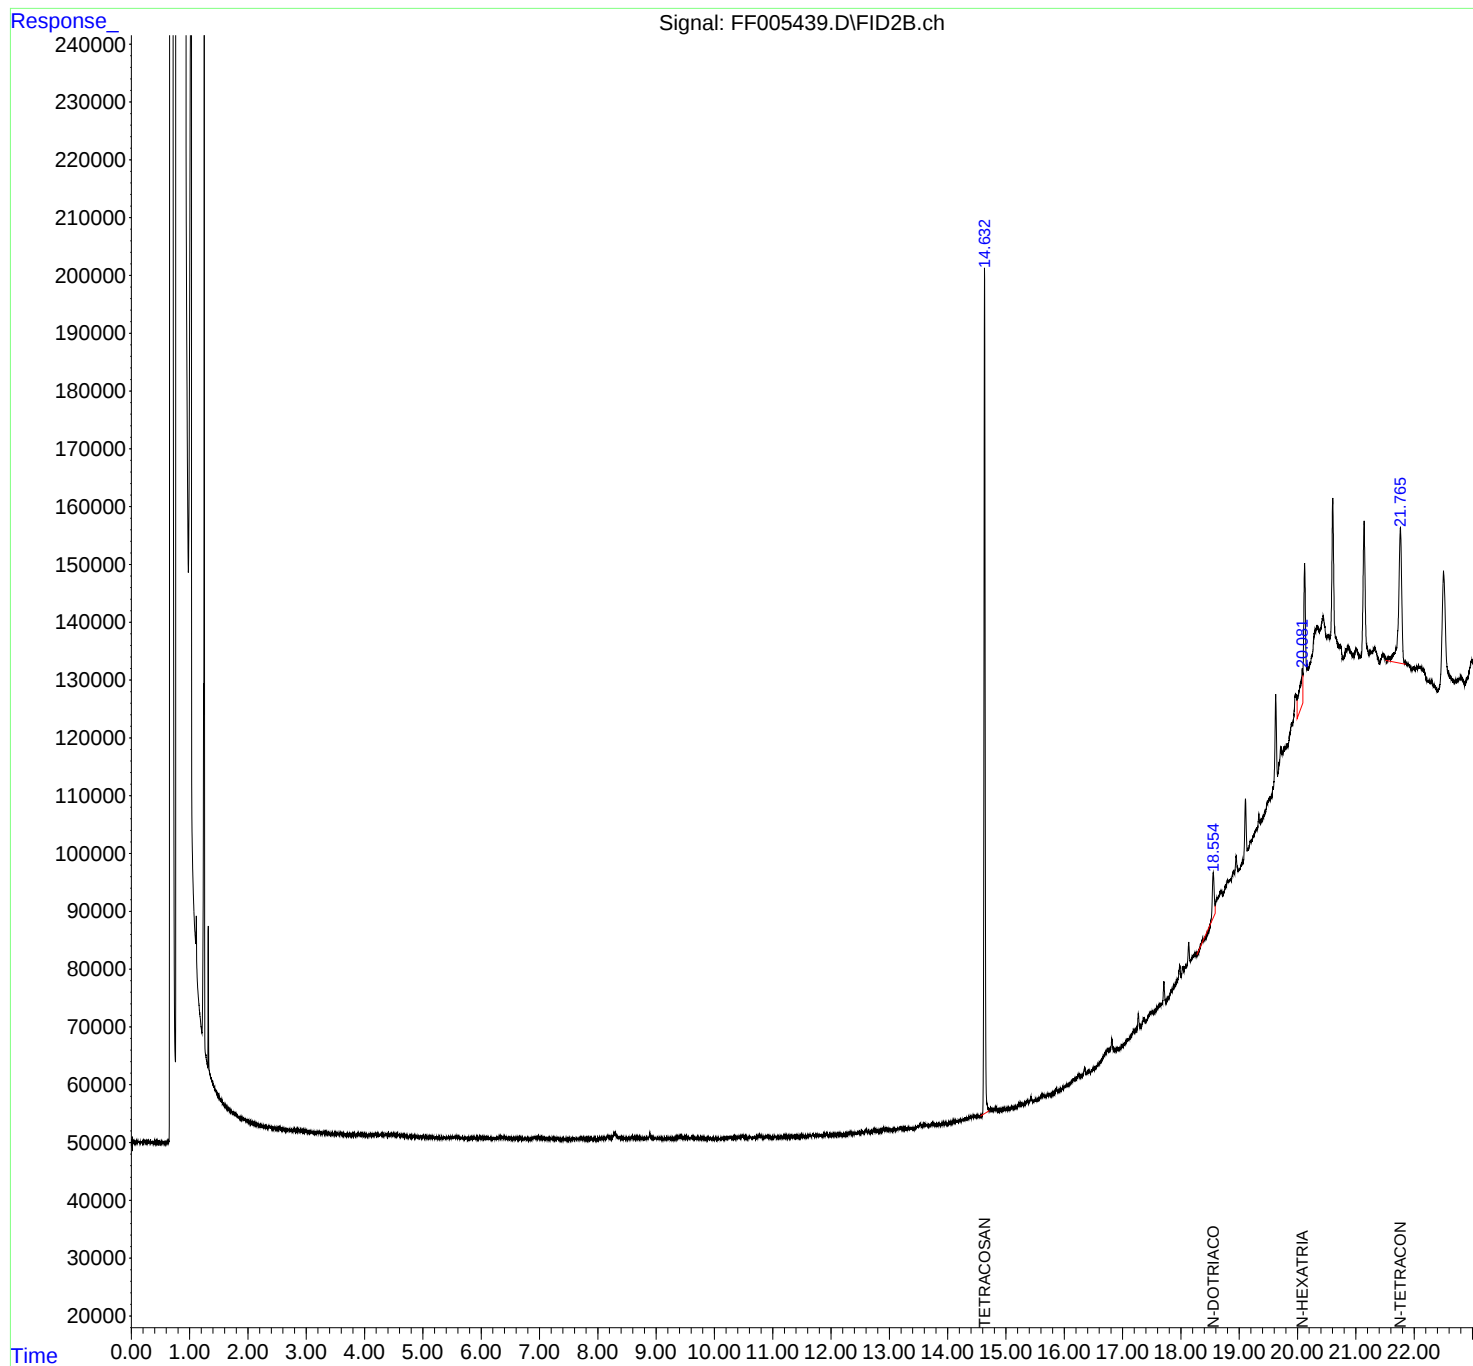


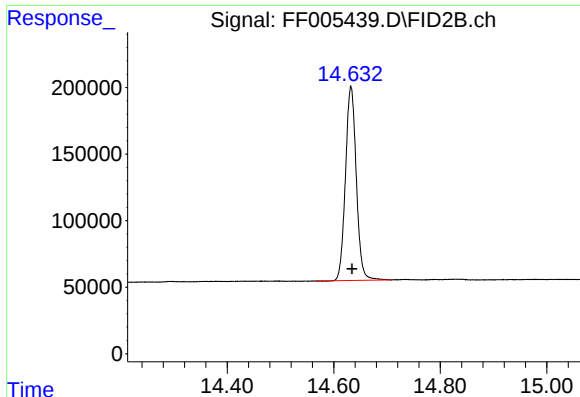

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.632 min
Delta R.T.: -0.002 min
Response: 2055425
Conc: 19.21 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

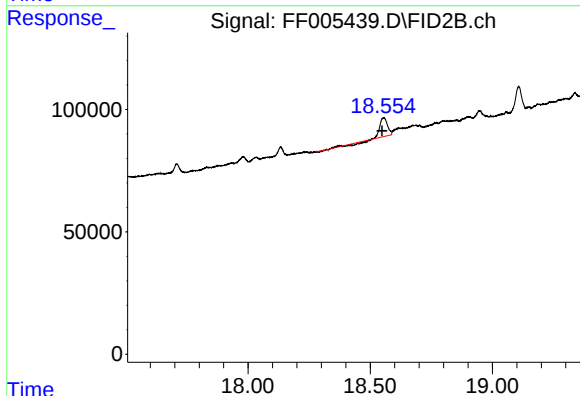


#14 N-DOTRIACONTANE

R.T.: 18.555 min
Delta R.T.: 0.006 min
Response: 145469
Conc: 1.17 ug/ml

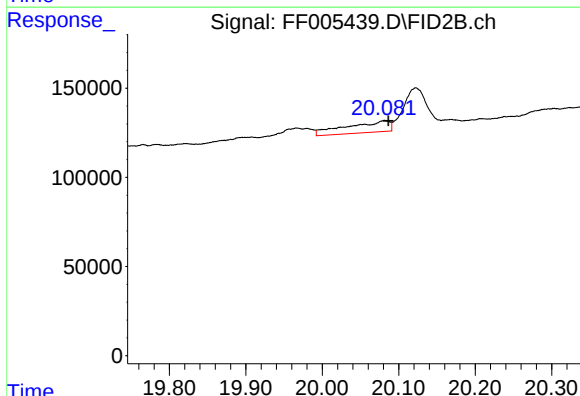

#16 N-HEXATRIACONTANE

R.T.: 20.081 min
Delta R.T.: -0.005 min
Response: 249606
Conc: 2.08 ug/ml

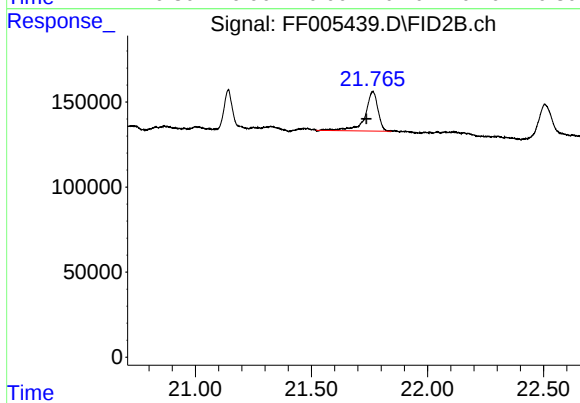

#18 N-TETRACONTANE

R.T.: 21.764 min
Delta R.T.: 0.028 min
Response: 893206
Conc: 7.03 ug/ml