

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
 Data File : FF005432.D
 Signal(s) : FID2B.ch
 Acq On : 05 Sep 2019 19:55
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: Sample.e
 Quant Time: Sep 06 01:16:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	5311594	49.637 ug/ml
Target Compounds			
2) N-DECANE	4.358	7084655	49.552 ug/ml
3) N-DODECANE	6.378	7093698	49.486 ug/ml
4) N-TETRADECANE	8.172	6998174	49.635 ug/ml
5) N-HEXADECANE	9.772	6930532	49.552 ug/ml
6) N-OCTADECANE	11.216	6687651	49.706 ug/ml
7) N-EICOSANE	12.528	6529079	49.785 ug/ml
8) N-DOCOSANE	13.729	6233814	49.511 ug/ml
10) N-TETRACOSANE	14.836	6013717	49.173 ug/ml
11) N-HEXACOSANE	15.861	5886813	49.178 ug/ml
12) N-OCTACOSANE	16.817	5921833	49.628 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090519\
Data File : FF05432.D
Signal(s) : FID2B.ch
Acq On : 05 Sep 2019 19:55
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: Sample.e
Quant Time: Sep 06 01:16:03 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

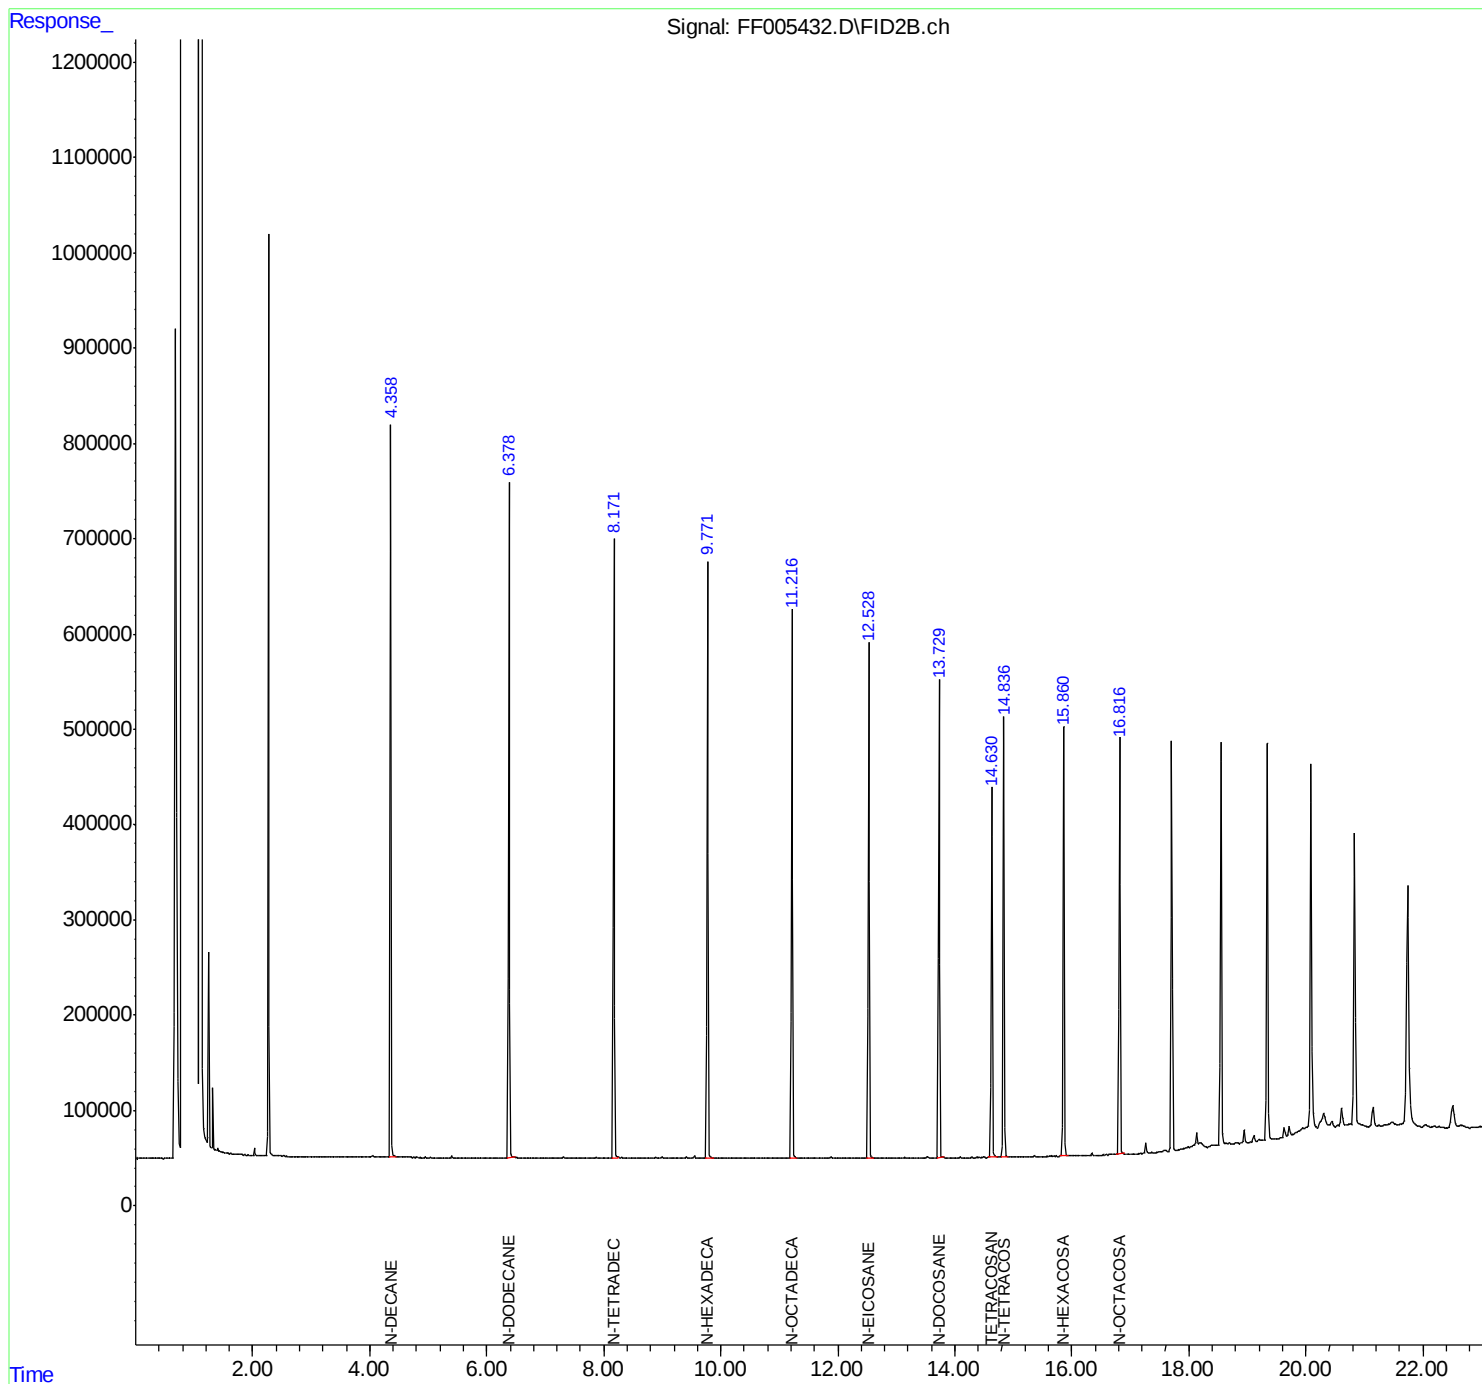


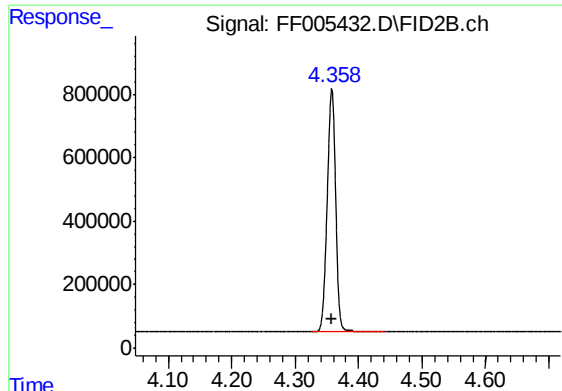

#2 N-DECANE


R.T.: 4.358 min
Delta R.T.: -0.001 min
Response: 7084655
Conc: 49.55 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

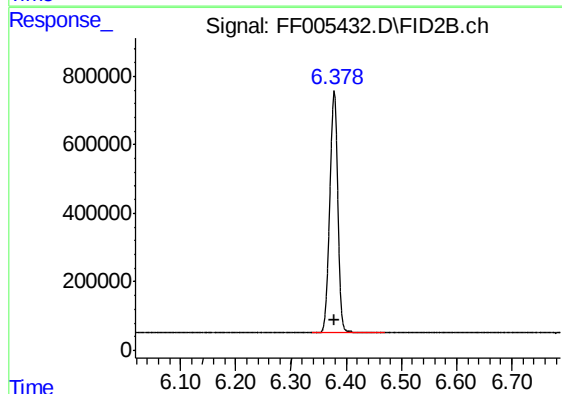


#3 N-DODECANE

R.T.: 6.378 min
Delta R.T.: -0.001 min
Response: 7093698
Conc: 49.49 ug/ml

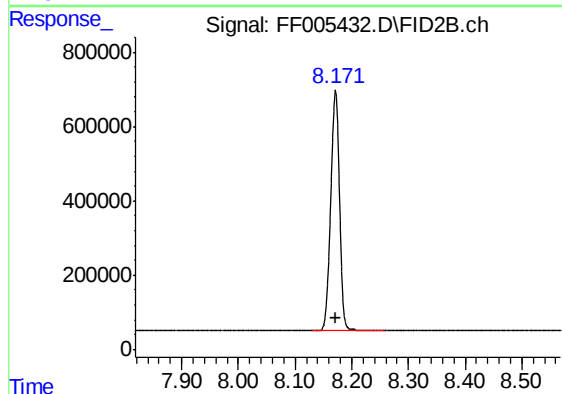


#4 N-TETRADECANE

R.T.: 8.172 min
Delta R.T.: -0.001 min
Response: 6998174
Conc: 49.63 ug/ml

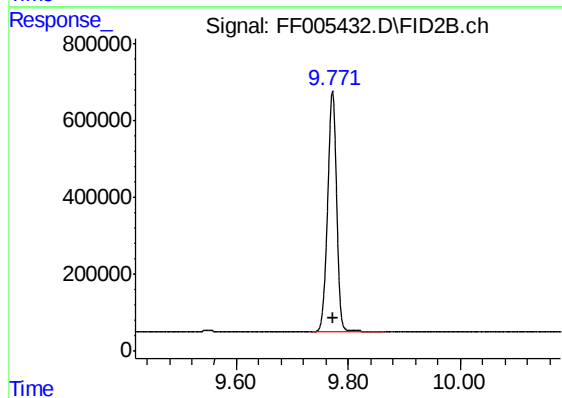

#5 N-HEXADECANE


R.T.: 9.772 min
Delta R.T.: -0.002 min
Response: 6930532
Conc: 49.55 ug/ml

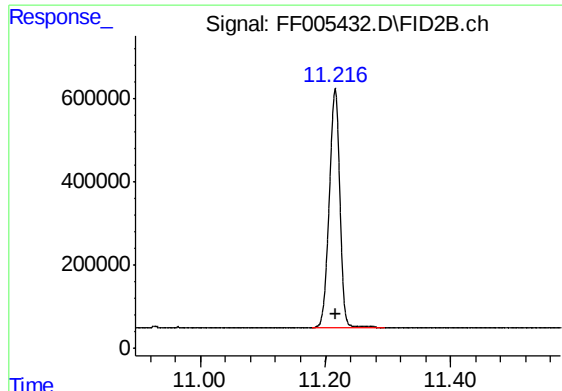

#6 N-OCTADECANE


R.T.: 11.216 min
Delta R.T.: -0.002 min
Response: 6687651
Conc: 49.71 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

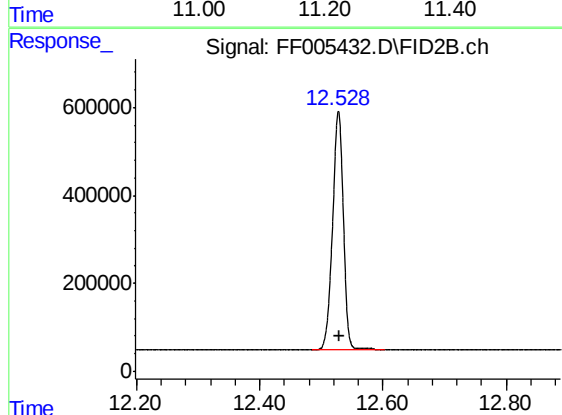


#7 N-EICOSANE

R.T.: 12.528 min
Delta R.T.: -0.002 min
Response: 6529079
Conc: 49.78 ug/ml

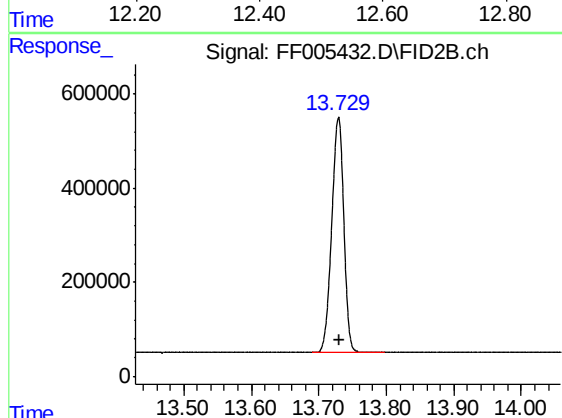


#8 N-DOCOSANE

R.T.: 13.729 min
Delta R.T.: -0.002 min
Response: 6233814
Conc: 49.51 ug/ml

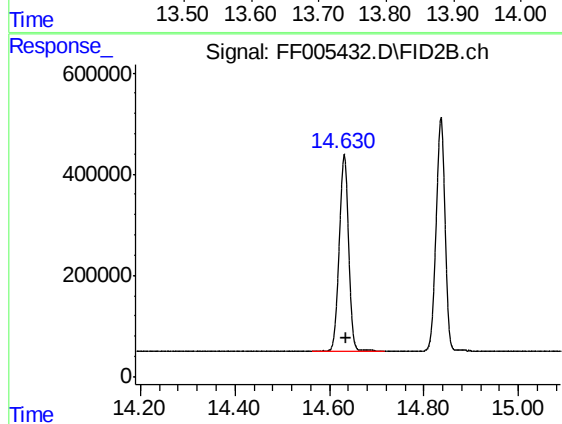

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.632 min
Delta R.T.: -0.003 min
Response: 5311594
Conc: 49.64 ug/ml

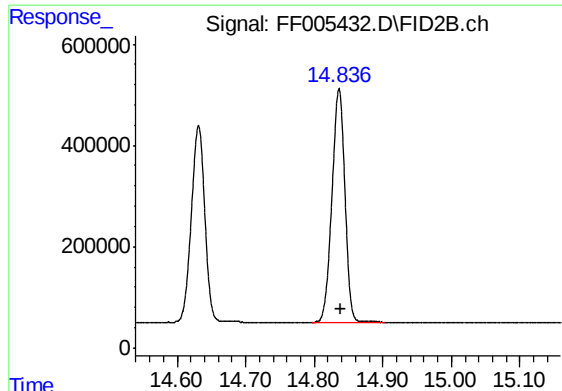

#10 N-TETRACOSANE


R.T.: 14.836 min
Delta R.T.: -0.003 min
Response: 6013717
Conc: 49.17 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

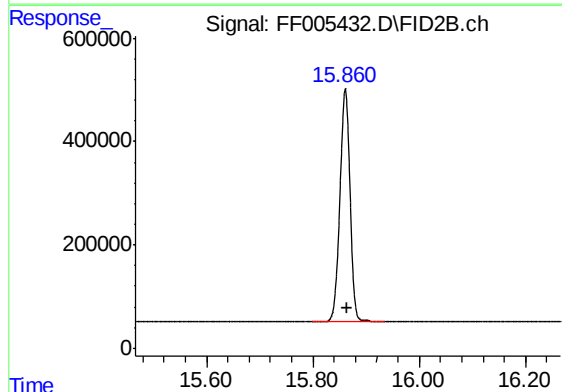

#11 N-HEXACOSANE

R.T.: 15.861 min
Delta R.T.: -0.003 min
Response: 5886813
Conc: 49.18 ug/ml

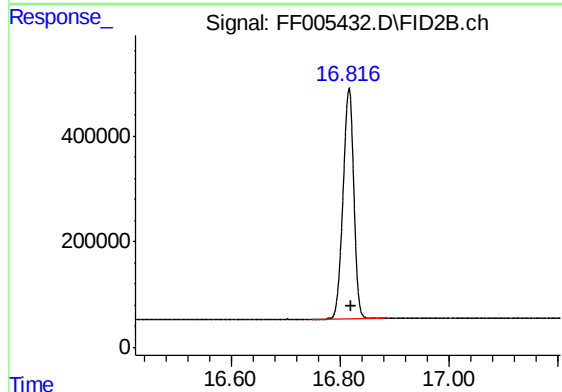

#12 N-OCTACOSANE

R.T.: 16.817 min
Delta R.T.: -0.002 min
Response: 5921833
Conc: 49.63 ug/ml