

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005441.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 07:59
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Sep 06 23:37:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.674	92076	0.860 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.558	366395	2.956 ug/ml
16)	N-HEXATRIACONTANE	20.126	1074121	8.949 ug/ml
18)	N-TETRACONTANE	21.768	3379751	26.583 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005441.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 07:59
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Sep 06 23:37:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

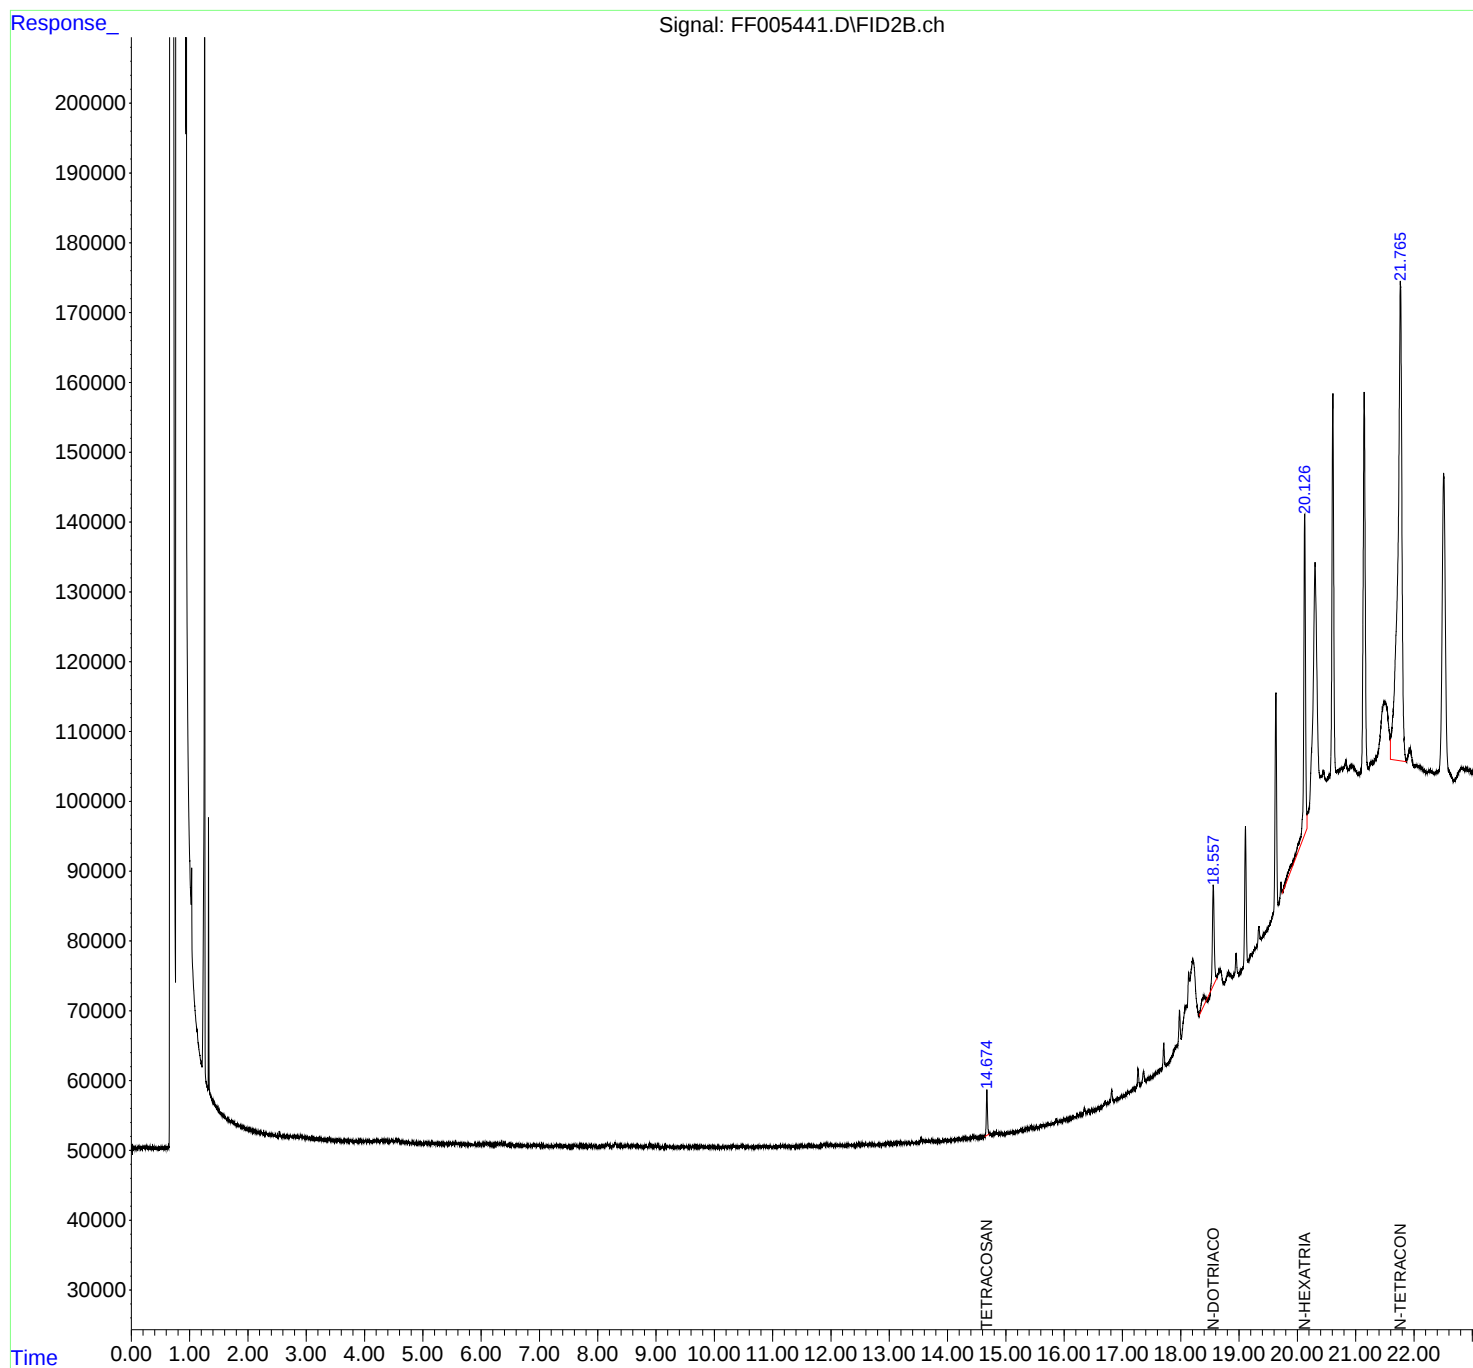


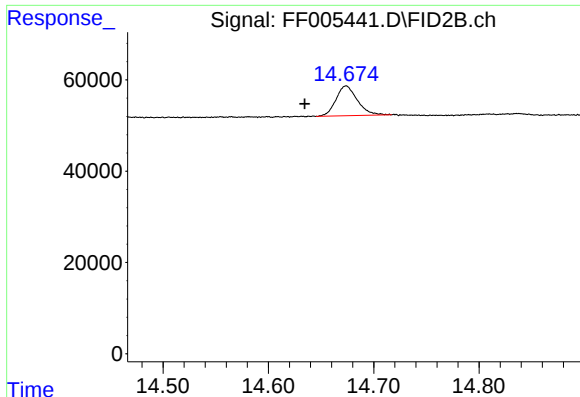

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.674 min
Delta R.T.: 0.039 min
Response: 92076
Conc: 0.86 ug/ml

Instrument :
FID_F
ClientSampleId :
MECL2

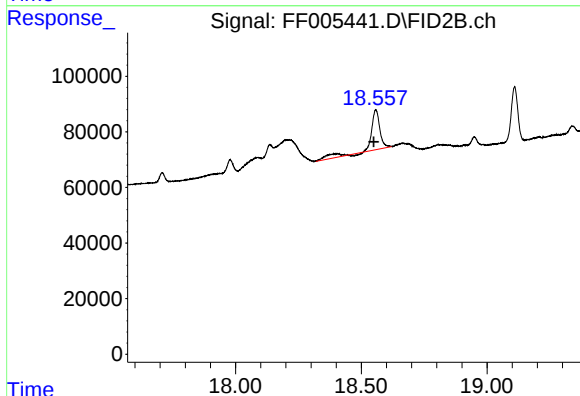


#14 N-DOTRIACONTANE

R.T.: 18.558 min
Delta R.T.: 0.008 min
Response: 366395
Conc: 2.96 ug/ml

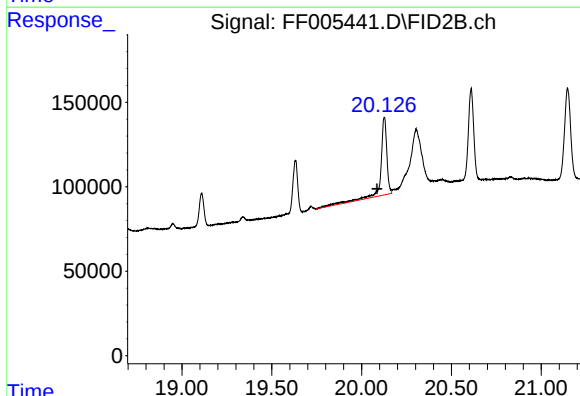

#16 N-HEXATRIACONTANE

R.T.: 20.126 min
Delta R.T.: 0.040 min
Response: 1074121
Conc: 8.95 ug/ml

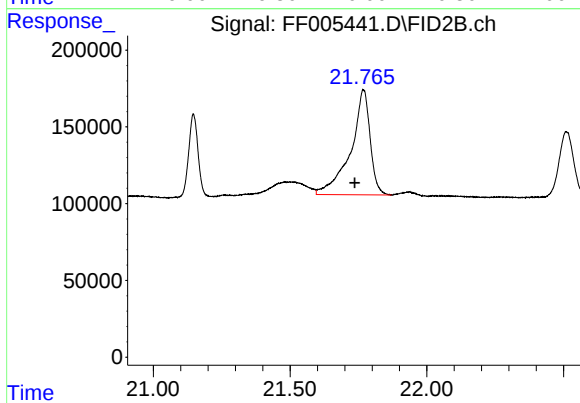

#18 N-TETRACONTANE

R.T.: 21.768 min
Delta R.T.: 0.032 min
Response: 3379751
Conc: 26.58 ug/ml