

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005444.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 10:10
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 06 23:38:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.369	5380611	37.535 ug/ml
12)	N-OCTACOSANE	16.820	4810928	40.318 ug/ml
13)	N-TRIACONTANE	17.710	165731	1.370 ug/ml
14)	N-DOTRIACONTANE	18.554	259951	2.097 ug/ml
15)	N-TETRATRIACONTANE	19.347	137773	1.143 ug/ml
16)	N-HEXATRIACONTANE	20.097	410331	3.419 ug/ml
18)	N-TETRACONTANE	21.783	1191251	9.370 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005444.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 10:10
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 06 23:38:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

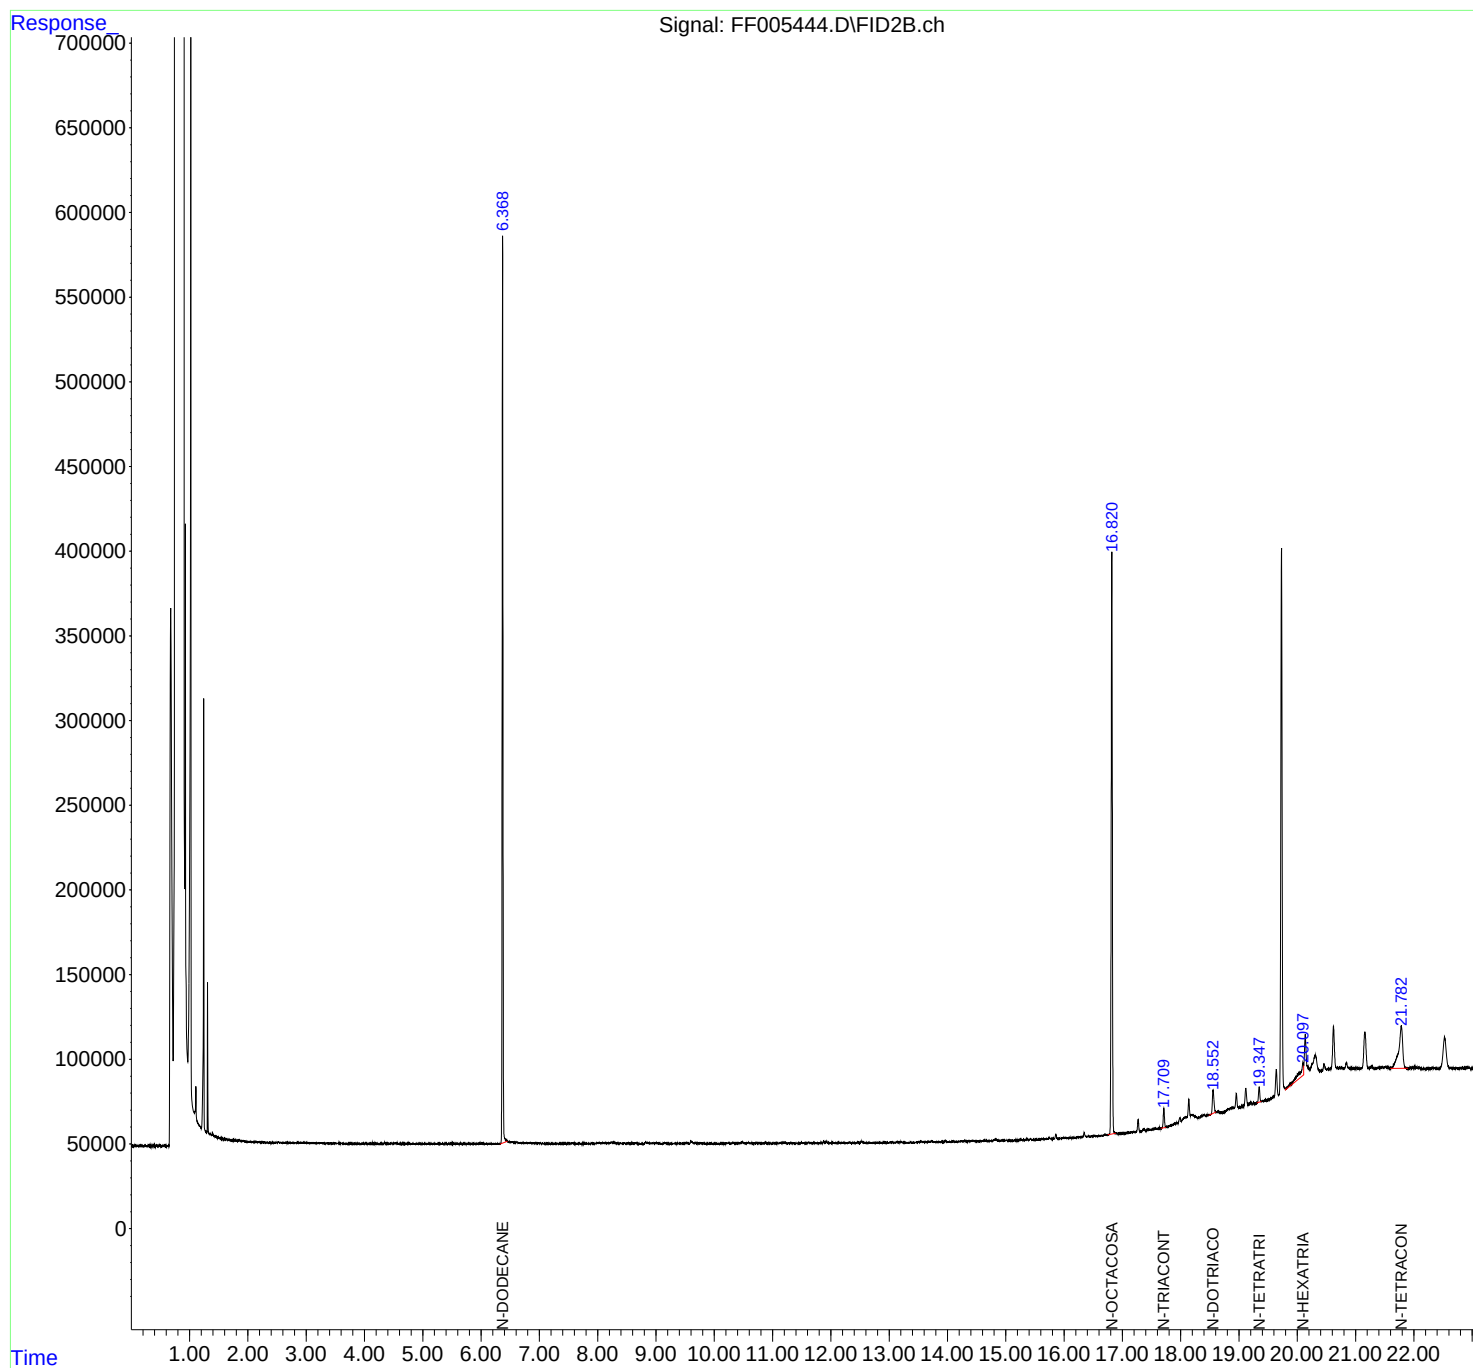


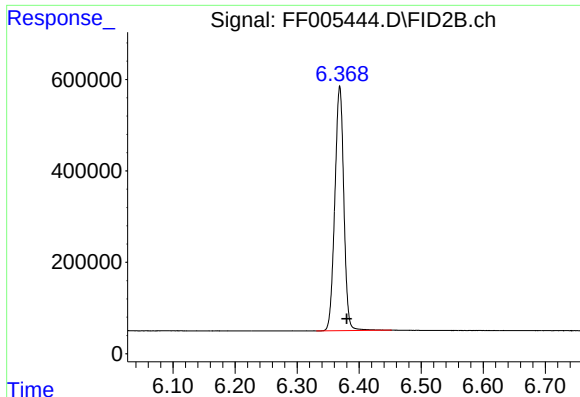

#3 N-DODECANE


R.T.: 6.369 min
Delta R.T.: -0.011 min
Response: 5380611
Conc: 37.54 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

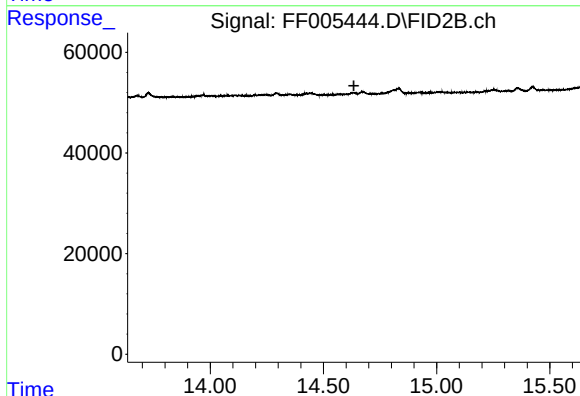


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.635 min
Response: 0
Conc: N.D.

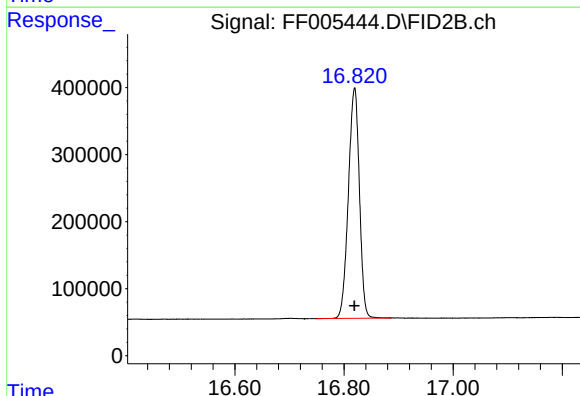


#12 N-OCTACOSANE

R.T.: 16.820 min
Delta R.T.: 0.000 min
Response: 4810928
Conc: 40.32 ug/ml

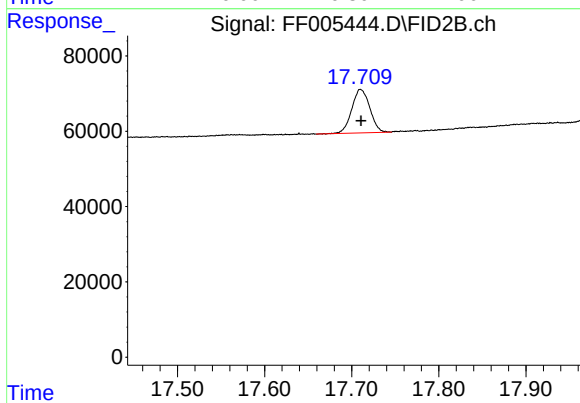

#13 N-TRIACONTANE


R.T.: 17.710 min
Delta R.T.: 0.000 min
Response: 165731
Conc: 1.37 ug/ml

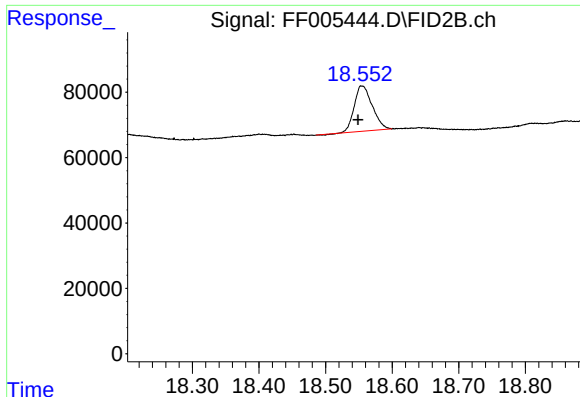

#14 N-DOTRIACONTANE


R.T.: 18.554 min
Delta R.T.: 0.005 min
Response: 259951
Conc: 2.10 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

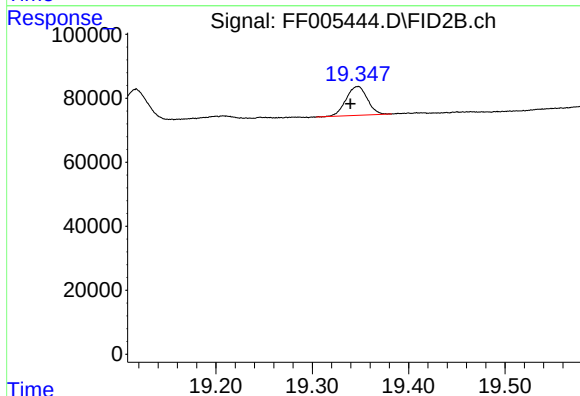


#15 N-TETRATRIACONTANE

R.T.: 19.347 min
Delta R.T.: 0.008 min
Response: 137773
Conc: 1.14 ug/ml

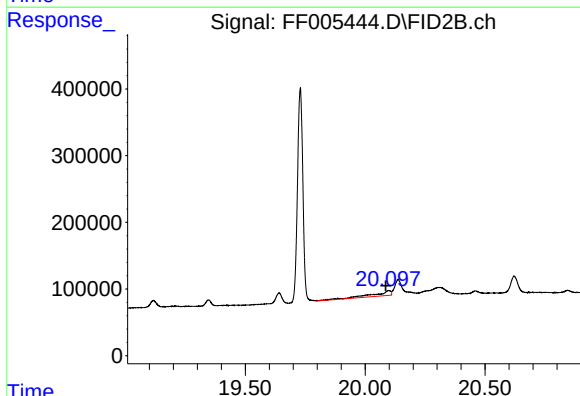

#16 N-HEXATRIACONTANE

R.T.: 20.097 min
Delta R.T.: 0.011 min
Response: 410331
Conc: 3.42 ug/ml

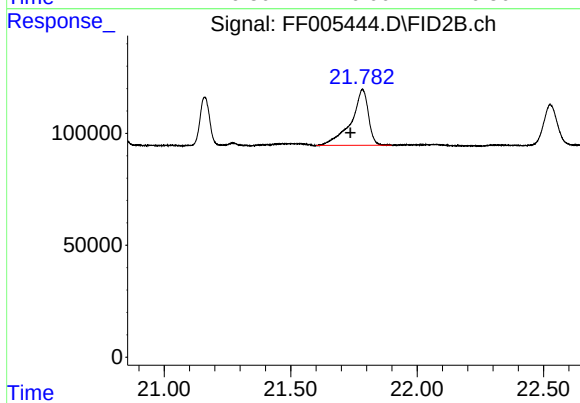

#18 N-TETRACONTANE

R.T.: 21.783 min
Delta R.T.: 0.047 min
Response: 1191251
Conc: 9.37 ug/ml