

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
 Data File : FF005445.D
 Signal(s) : FID2B.ch
 Acq On : 06 Sep 2019 11:40
 Operator : DD\AJ
 Sample : K4692-04 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-31-COMP

Integration File: autoint1.e
 Quant Time: Sep 06 23:38:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	507907	4.746 ug/ml
Target Compounds			
4) N-TETRADECANE	8.225f	93485	0.663 ug/ml
7) N-EICOSANE	12.526	143690	1.096 ug/ml
8) N-DOCOSANE	13.727	144214	1.145 ug/ml
10) N-TETRACOSANE	14.813	1122566	9.179 ug/ml
11) N-HEXACOSANE	15.863	203975	1.704 ug/ml
12) N-OCTACOSANE	16.826	423167	3.546 ug/ml
13) N-TRIACONTANE	17.709	235929	1.950 ug/ml
14) N-DOTRIACONTANE	18.507	126880	1.024 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005445.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 11:40
Operator : DD\AJ
Sample : K4692-04 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-31-COMP

Integration File: autoint1.e
Quant Time: Sep 06 23:38:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

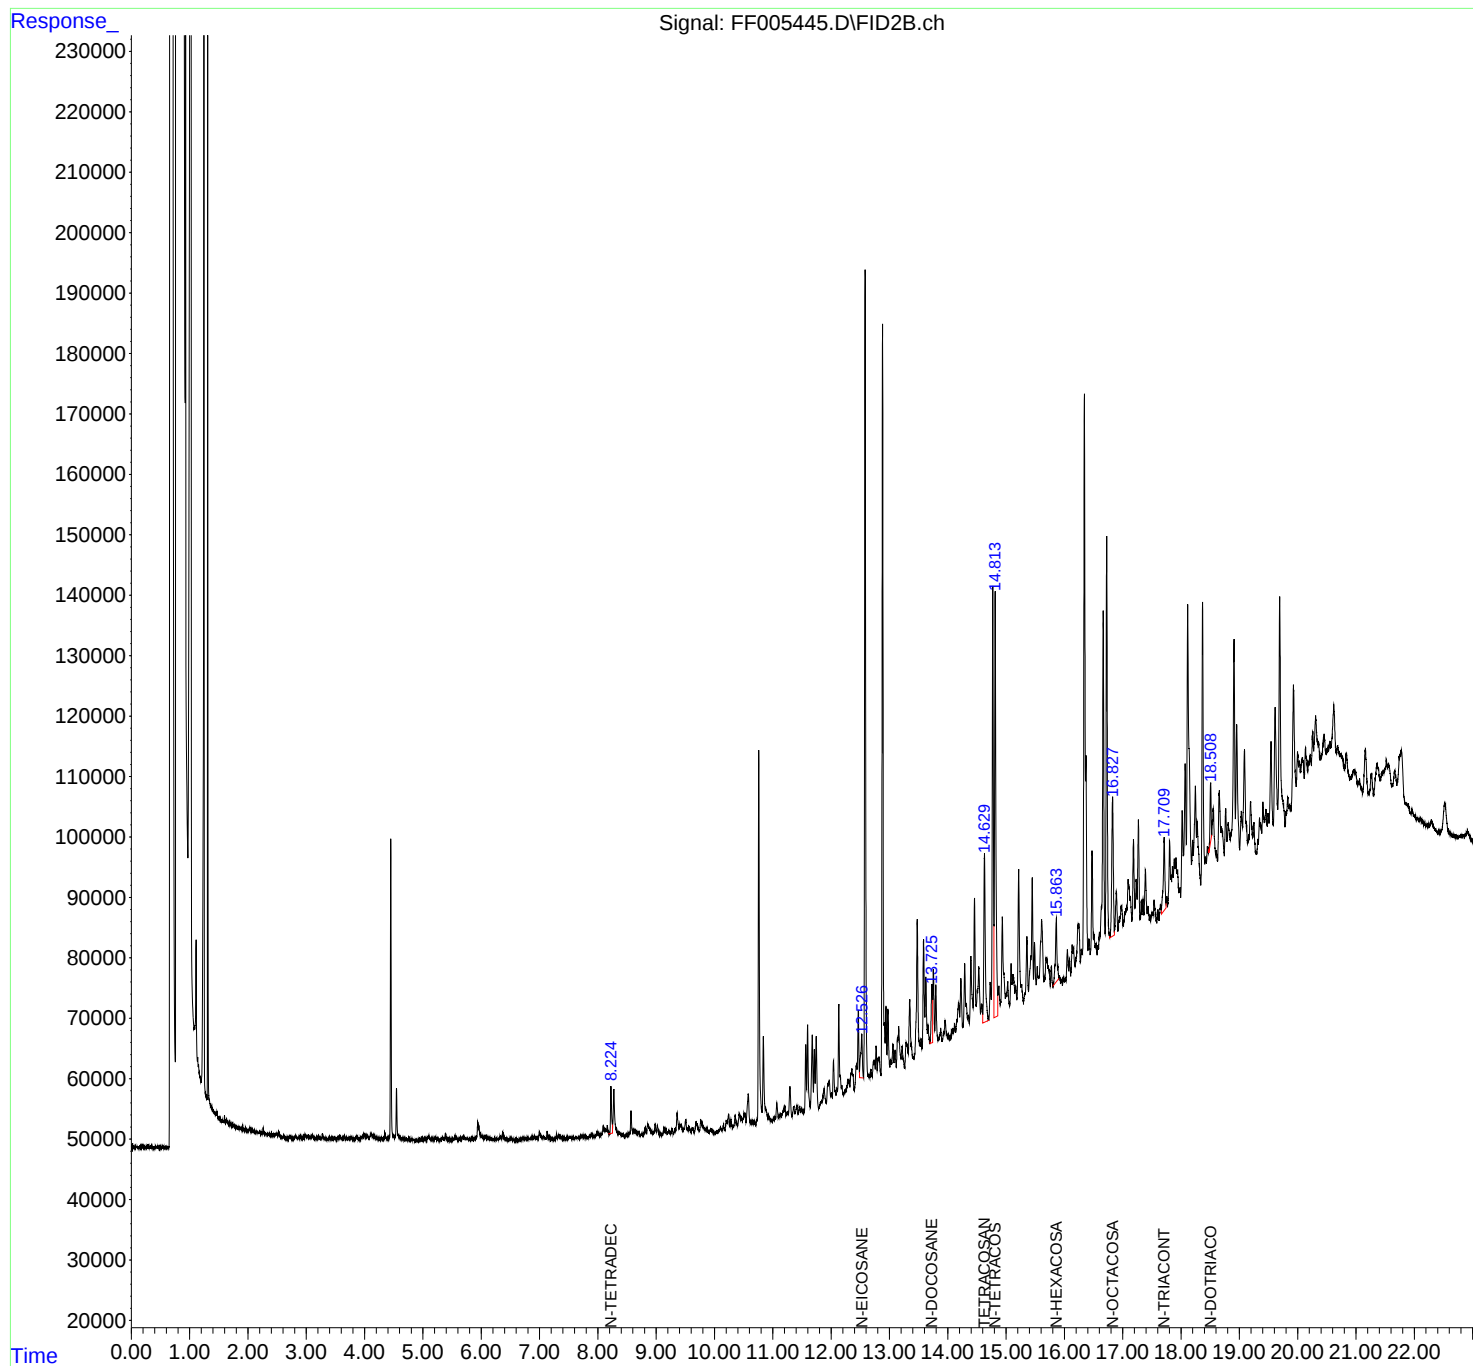


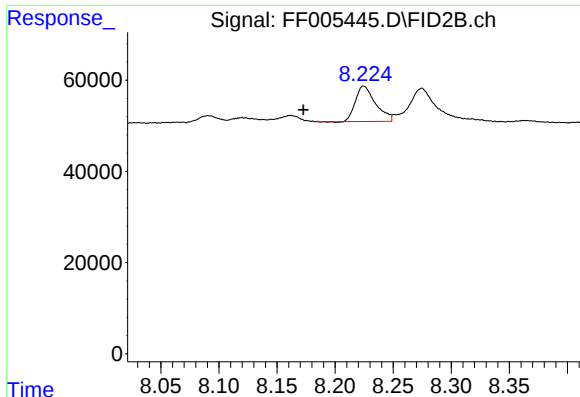

#4 N-TETRADECANE


R.T.: 8.225 min
Delta R.T.: 0.052 min
Response: 93485
Conc: 0.66 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-31-COMP

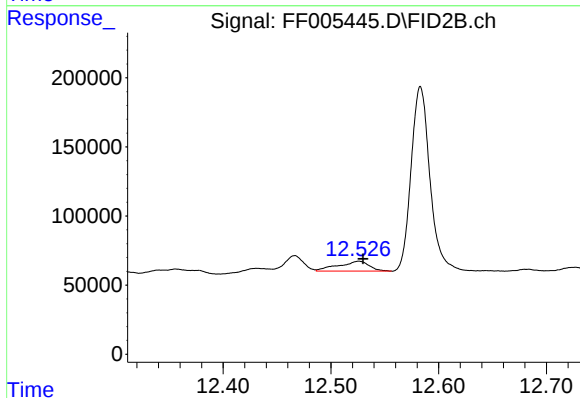


#7 N-EICOSANE

R.T.: 12.526 min
Delta R.T.: -0.004 min
Response: 143690
Conc: 1.10 ug/ml

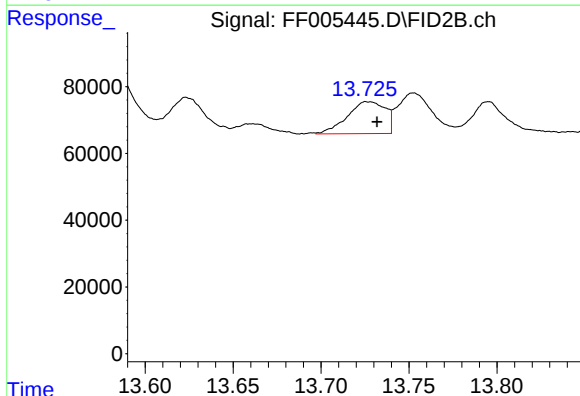


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: -0.005 min
Response: 144214
Conc: 1.15 ug/ml

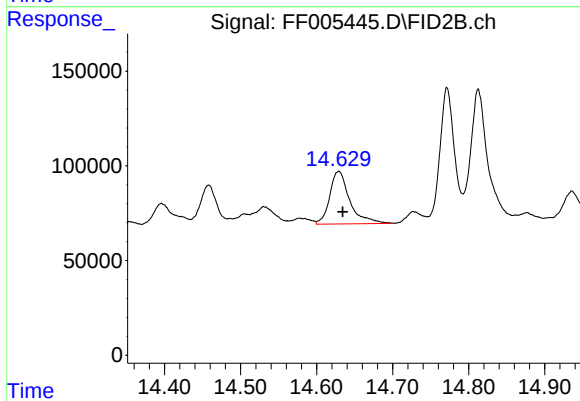

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.629 min
Delta R.T.: -0.005 min
Response: 507907
Conc: 4.75 ug/ml

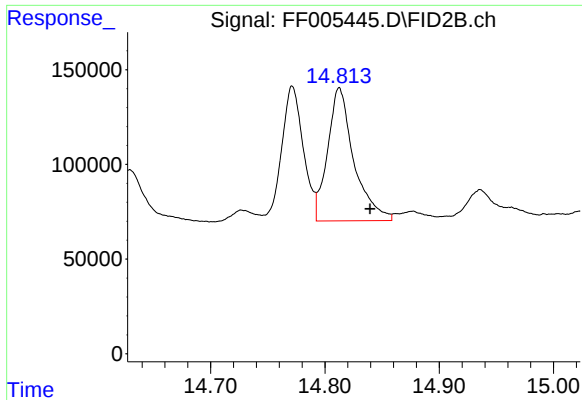

#10 N-TETRACOSANE


R.T.: 14.813 min
Delta R.T.: -0.027 min
Response: 1122566
Conc: 9.18 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-31-COMP

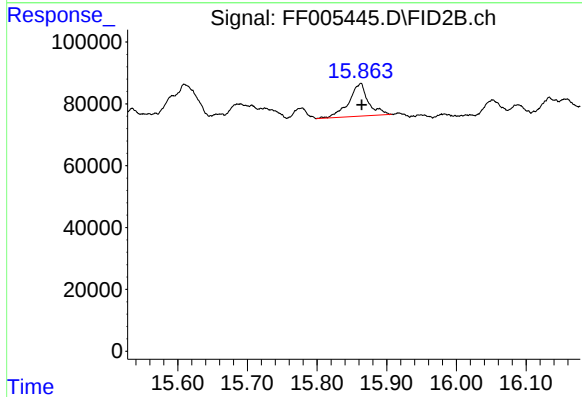


#11 N-HEXACOSANE

R.T.: 15.863 min
Delta R.T.: -0.002 min
Response: 203975
Conc: 1.70 ug/ml

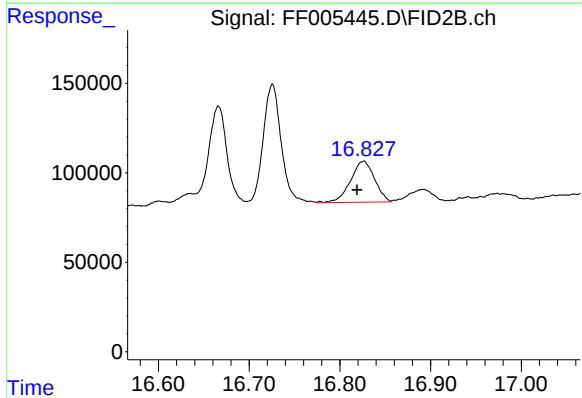


#12 N-OCTACOSANE

R.T.: 16.826 min
Delta R.T.: 0.007 min
Response: 423167
Conc: 3.55 ug/ml

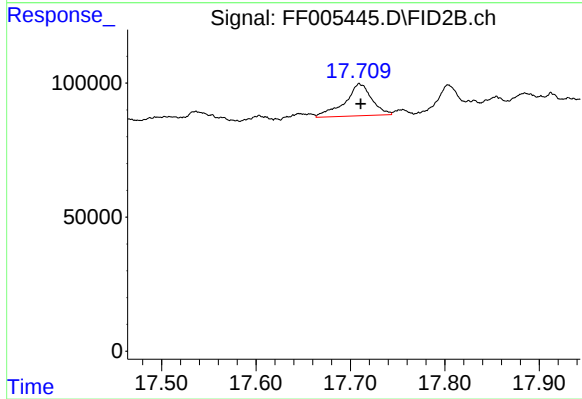

#13 N-TRIACONTANE

R.T.: 17.709 min
Delta R.T.: -0.001 min
Response: 235929
Conc: 1.95 ug/ml

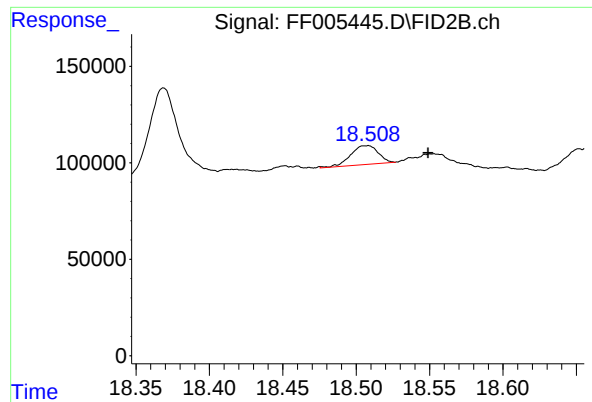

#14 N-DOTRIACONTANE

R.T.: 18.507 min
Delta R.T.: -0.042 min
Response: 126880
Conc: 1.02 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-31-COMP