

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
 Data File : FF005446.D
 Signal(s) : FID2B.ch
 Acq On : 06 Sep 2019 12:10
 Operator : DD\AJ
 Sample : K4692-06 10X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-30-COMP

Integration File: autoint1.e
 Quant Time: Sep 06 23:39:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	146027	1.365 ug/ml
Target Compounds			
7) N-EICOSANE	12.584f	834062	6.360 ug/ml
10) N-TETRACOSANE	14.815	438234	3.583 ug/ml
12) N-OCTACOSANE	16.829	215091	1.803 ug/ml
16) N-HEXATRIACONTANE	20.130	248706	2.072 ug/ml
18) N-TETRACONTANE	21.769	362005	2.847 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005446.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 12:10
Operator : DD\AJ
Sample : K4692-06 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-30-COMP

Integration File: autoint1.e
Quant Time: Sep 06 23:39:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

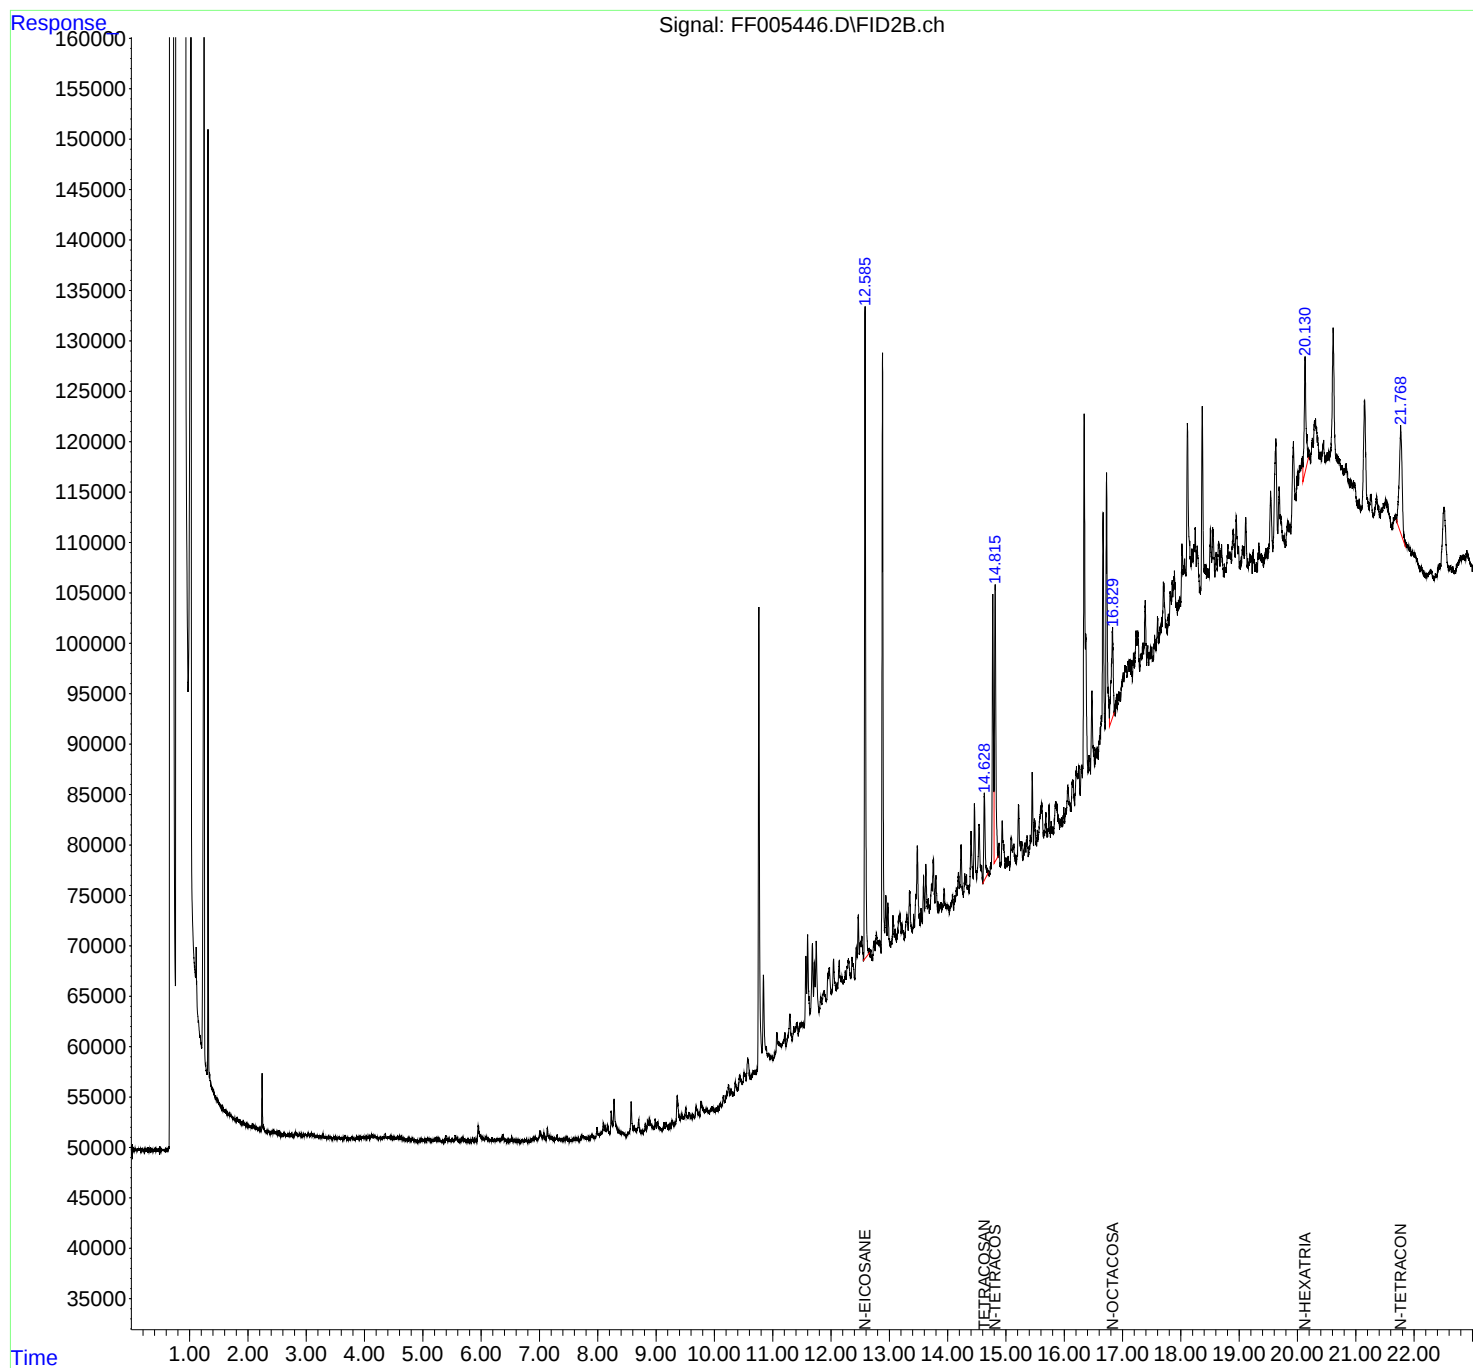


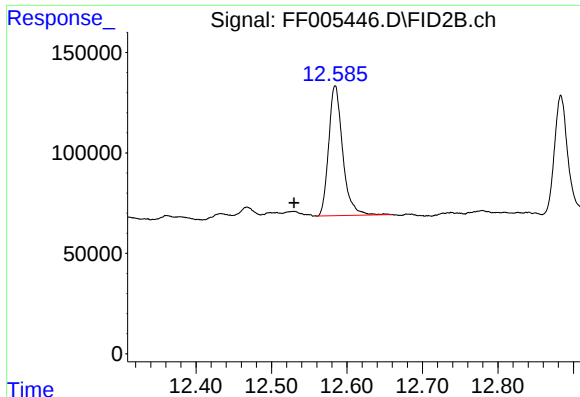

#7 N-EICOSANE


R.T.: 12.584 min
Delta R.T.: 0.054 min
Response: 834062
Conc: 6.36 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-30-COMP

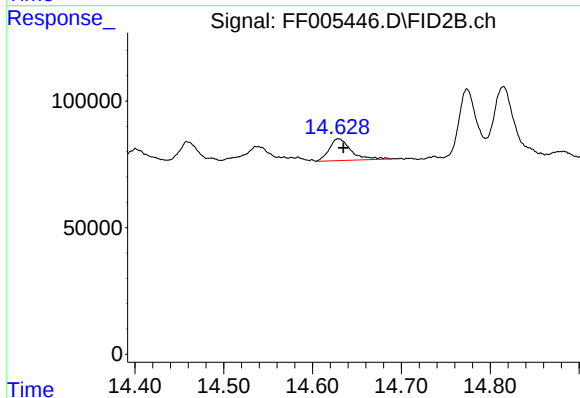


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.629 min
Delta R.T.: -0.005 min
Response: 146027
Conc: 1.36 ug/ml

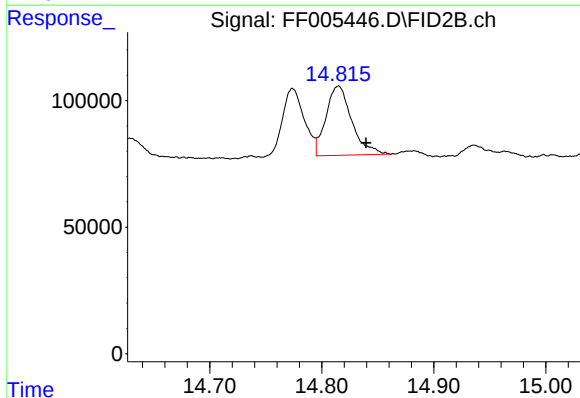


#10 N-TETRACOSANE

R.T.: 14.815 min
Delta R.T.: -0.025 min
Response: 438234
Conc: 3.58 ug/ml

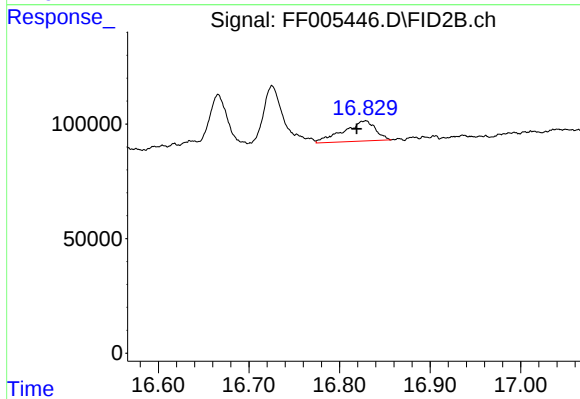

#12 N-OCTACOSANE


R.T.: 16.829 min
Delta R.T.: 0.010 min
Response: 215091
Conc: 1.80 ug/ml

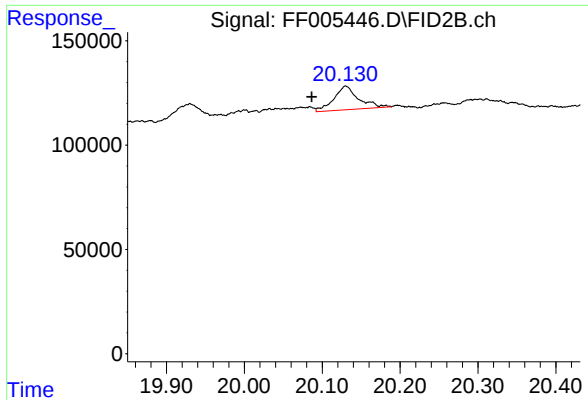

#16 N-HEXATRIACONTANE

R.T.: 20.130 min
Delta R.T.: 0.044 min
Response: 248706
Conc: 2.07 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-30-COMP

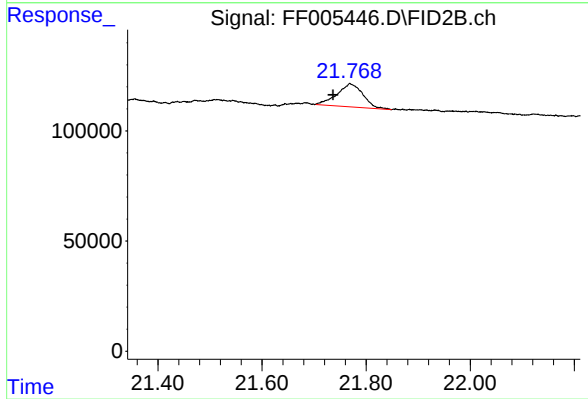

#18 N-TETRACONTANE

R.T.: 21.769 min
Delta R.T.: 0.033 min
Response: 362005
Conc: 2.85 ug/ml