

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005448.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 13:38
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 06 23:39:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.631	1989036	18.588 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.129	16274	0.136 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005448.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 13:38
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 06 23:39:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

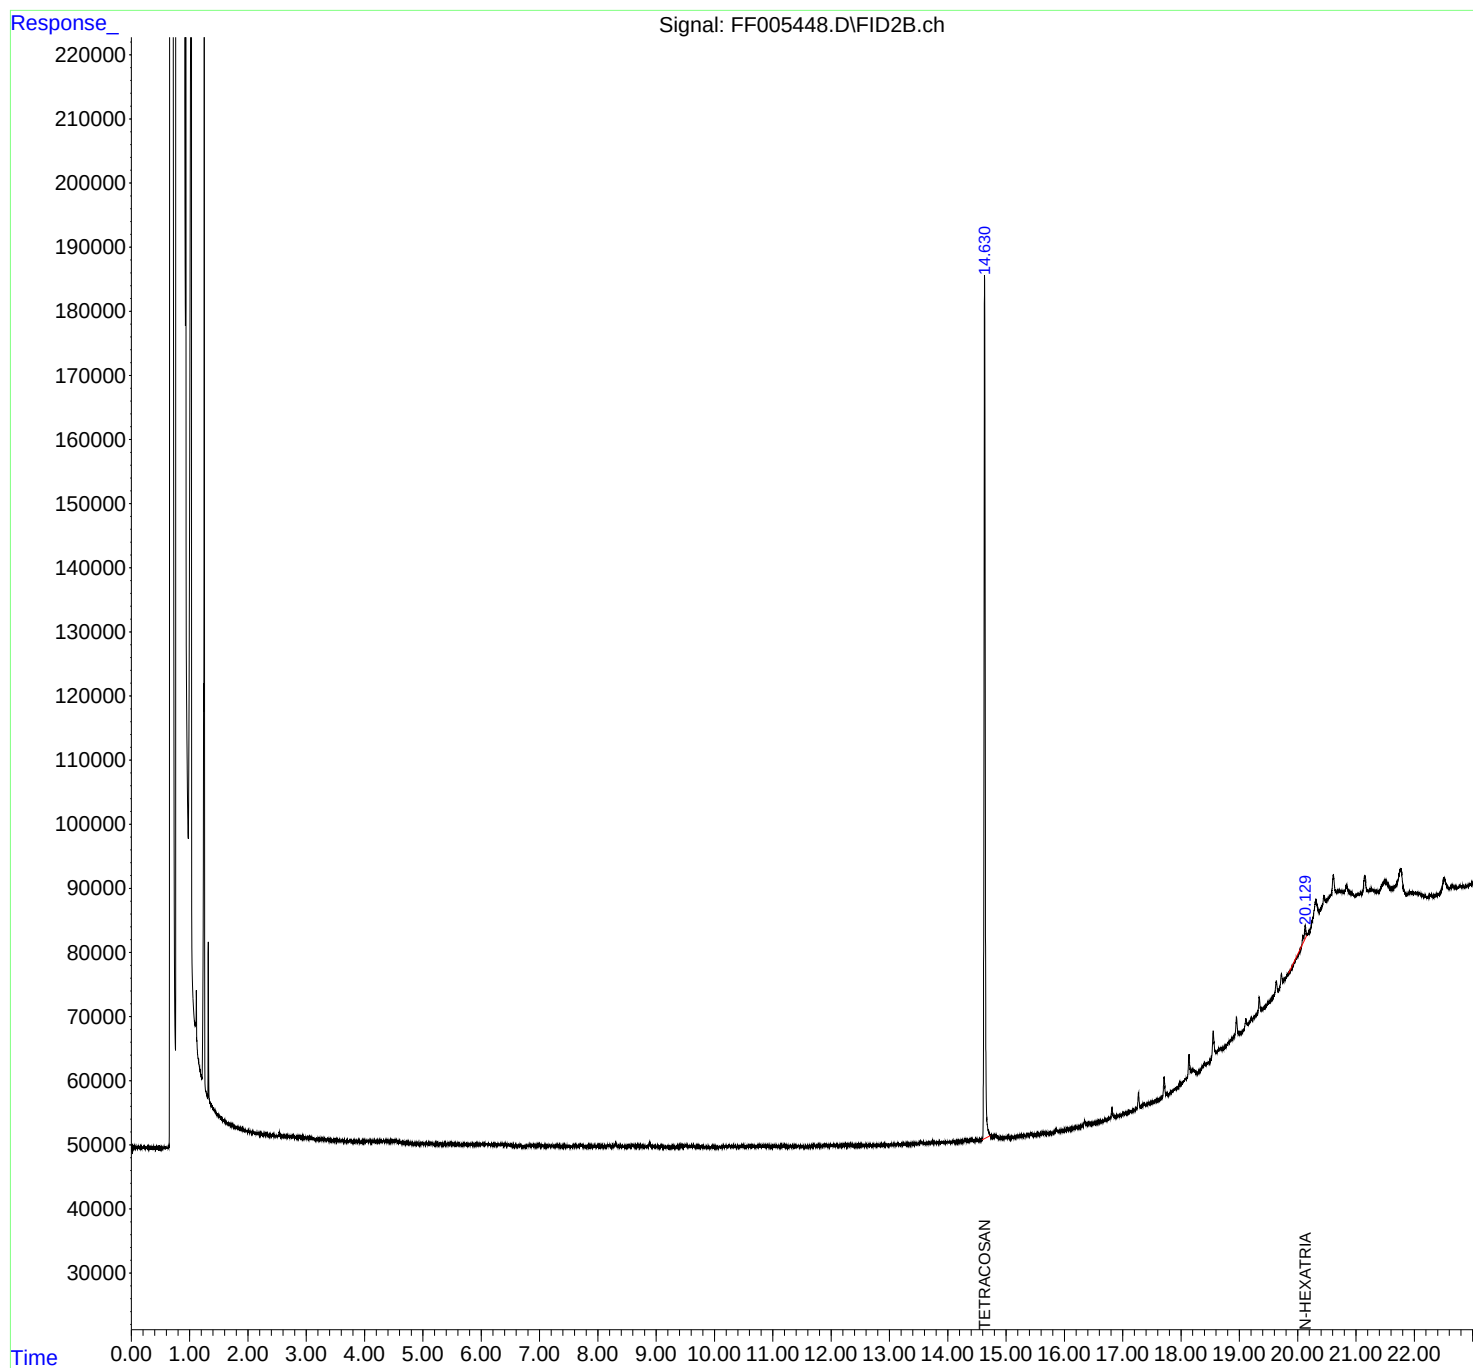


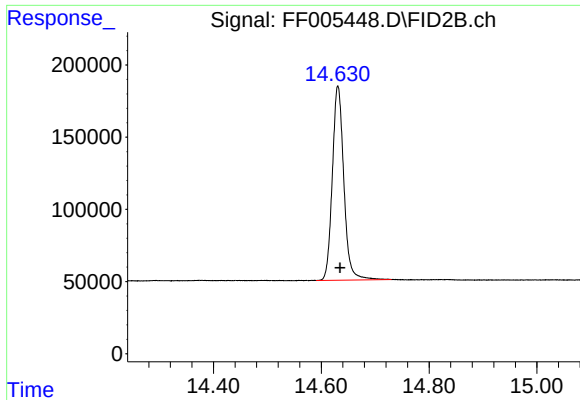

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.631 min
Delta R.T.: -0.004 min
Response: 1989036
Conc: 18.59 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

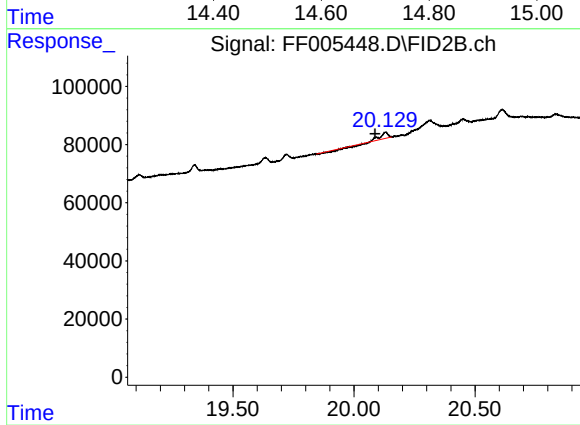

#16 N-HEXATRIACONTANE

R.T.: 20.129 min
Delta R.T.: 0.043 min
Response: 16274
Conc: 0.14 ug/ml