

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005445.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 11:40
Operator : DD\AJ
Sample : K4692-04 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-31-COMP

Integration File: autoint1.e
Quant Time: Sep 06 23:38:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	507907	4.746 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090619\
Data File : FF005445.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2019 11:40
Operator : DD\AJ
Sample : K4692-04 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-31-COMP

Integration File: autoint1.e
Quant Time: Sep 06 23:38:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

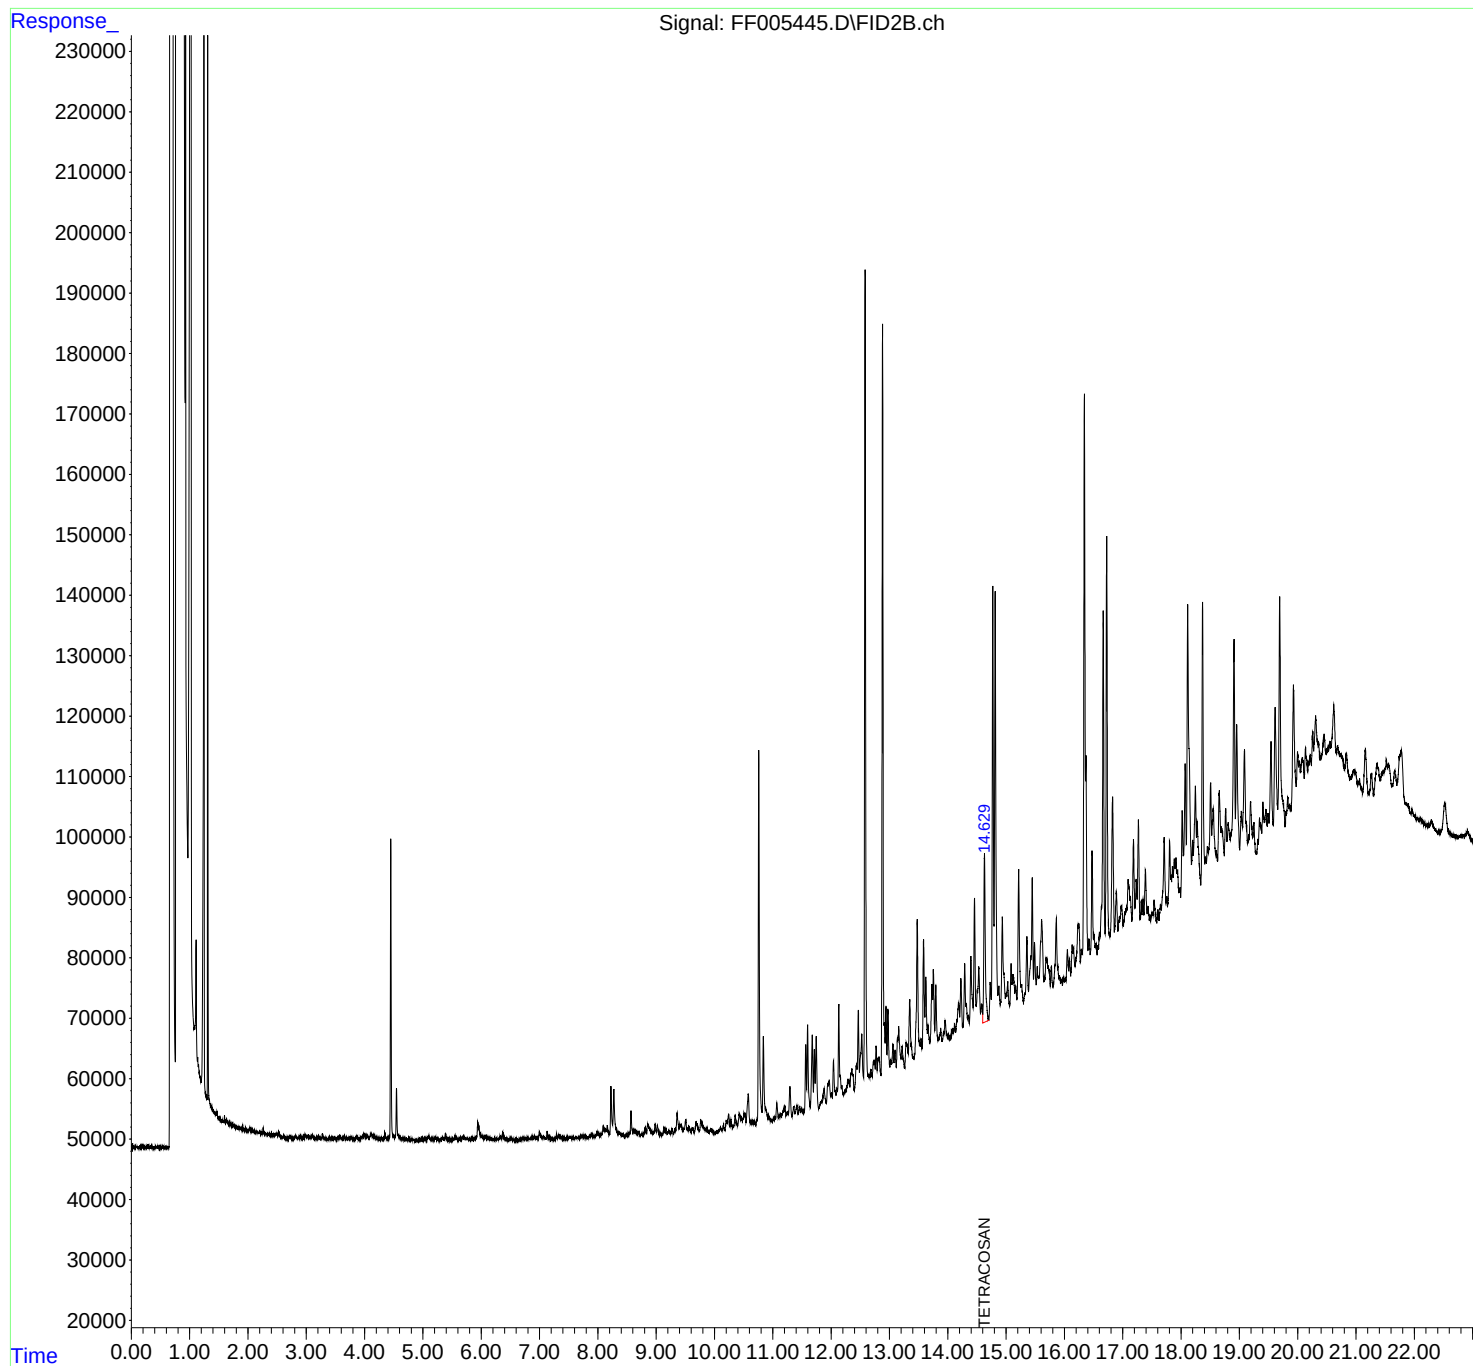

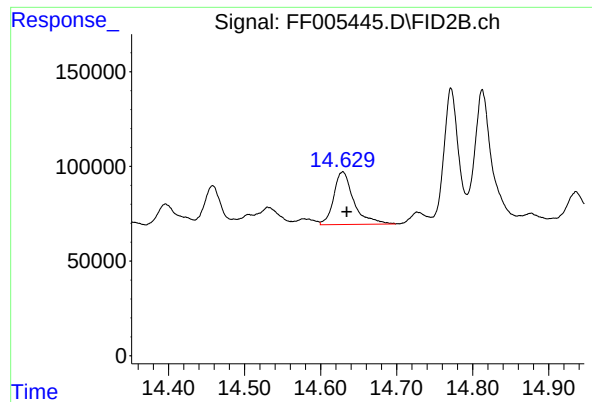

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.629 min
Delta R.T.: -0.005 min
Response: 507907
Conc: 4.75 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-31-COMP